
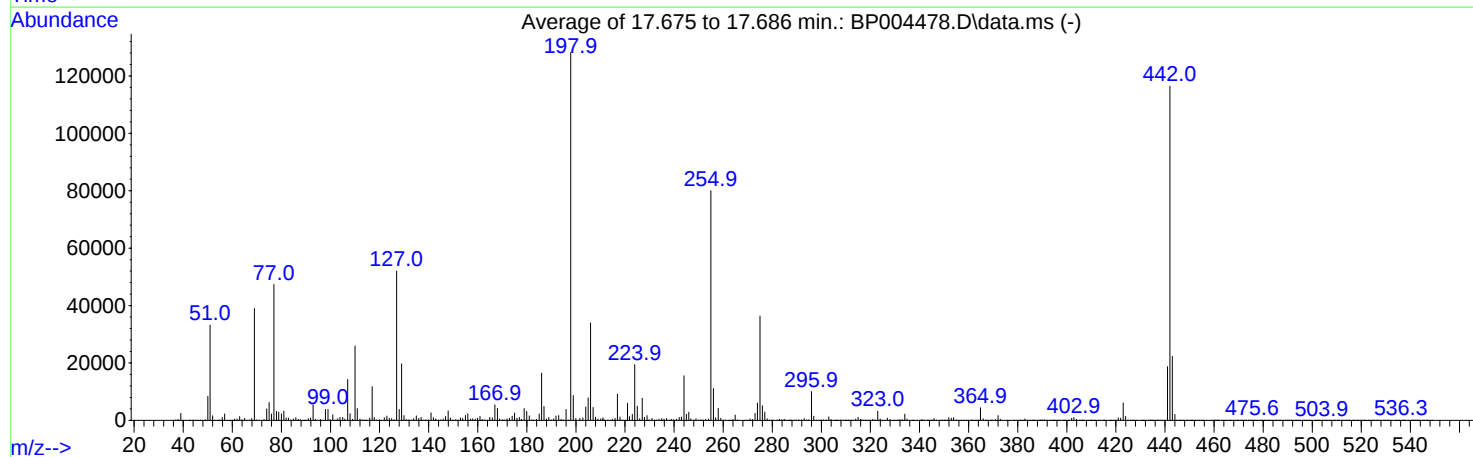


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010721\
 Data File : BP004478.D
 Acq On : 07 Jan 2021 13:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP121120.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 07 14:50:44 2021

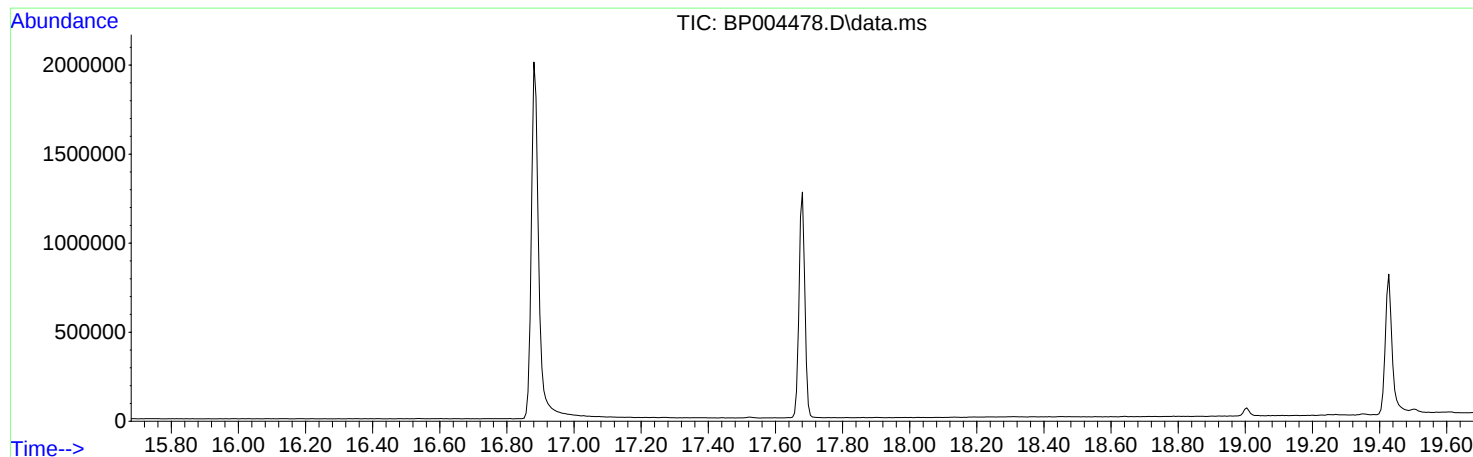

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.9	33165	PASS
68	69	0.00	2	1.6	629	PASS
69	198	0.00	100	30.4	38996	PASS
70	69	0.00	2	0.4	170	PASS
127	198	10	80	40.6	52044	PASS
197	198	0.00	2	0.1	128	PASS
198	198	100	100	100.0	128182	PASS
199	198	5	9	6.7	8626	PASS
275	198	10	60	28.4	36379	PASS
365	198	1	100	3.4	4387	PASS
441	198	0.01	100	14.6	18717	PASS
442	442	100	100	100.0	116492	PASS
443	442	15	24	19.1	22304	PASS