
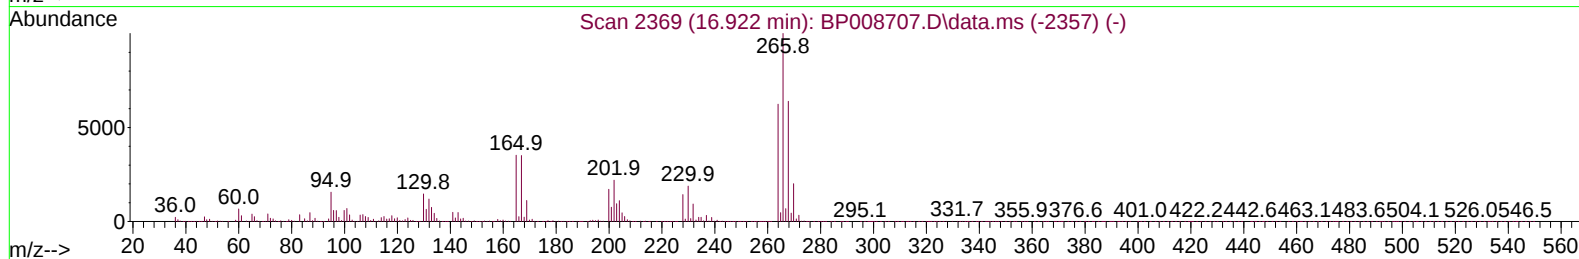
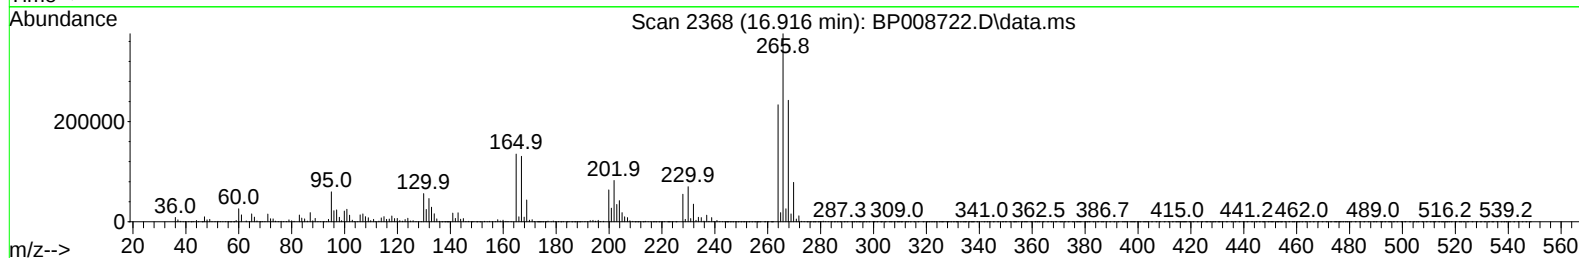


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010722\
 Data File : BP008722.D
 Acq On : 07 Jan 2022 12:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 07 17:15:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 07 07:45:52 2022
 Response via : Initial Calibration

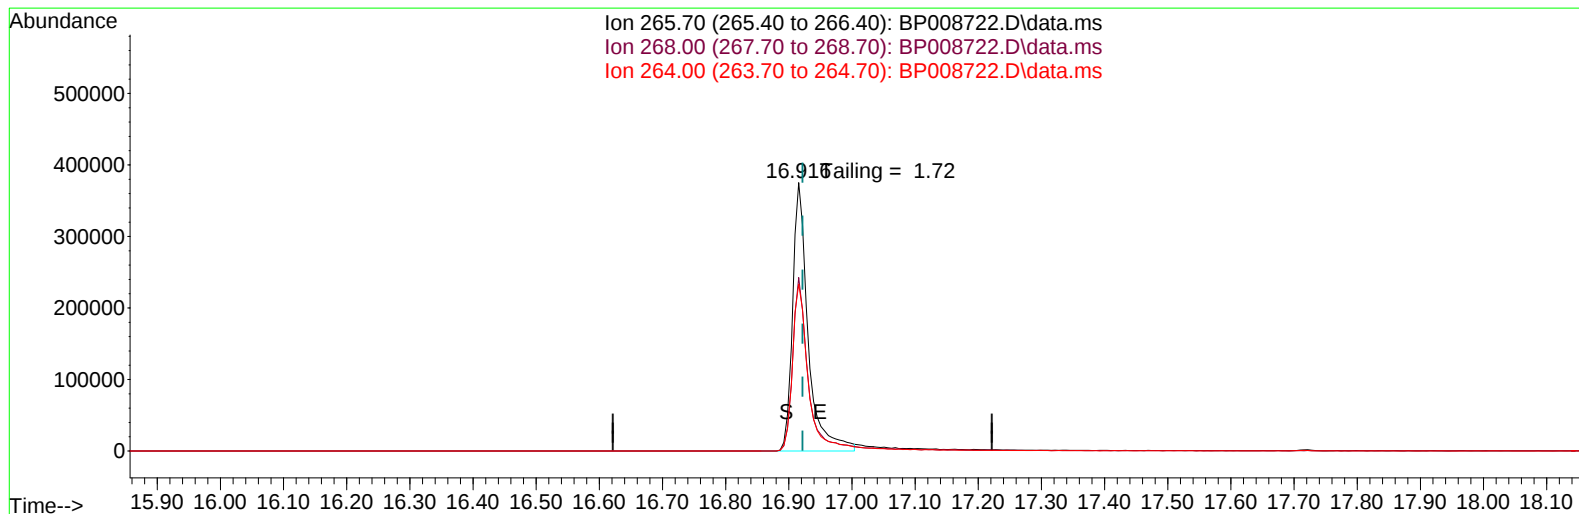

TIC: BP008722.D\data.ms

(70) Pentachlorophenol (C)




16.916min (-0.006) 3296901.96 ng

response 679987

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.61
264.00	62.90	62.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010722\
 Data File : BP008722.D
 Acq On : 07 Jan 2022 12:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 07 17:15:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 07 07:45:52 2022
 Response via : Initial Calibration

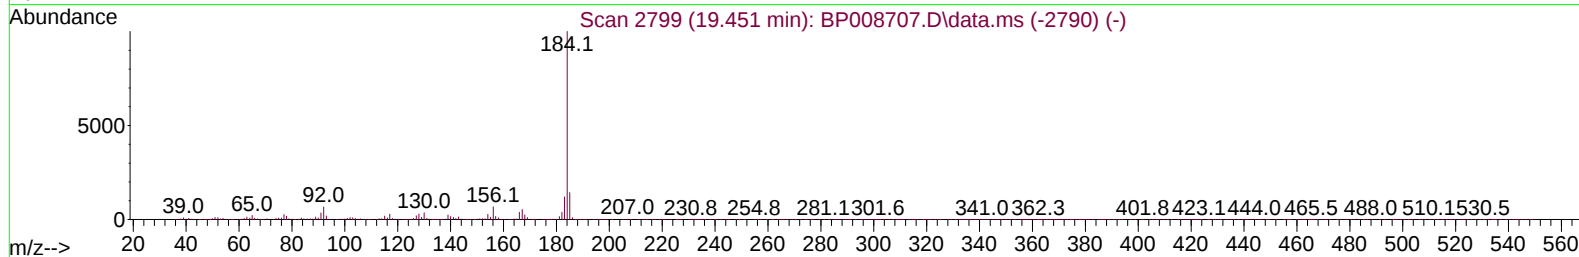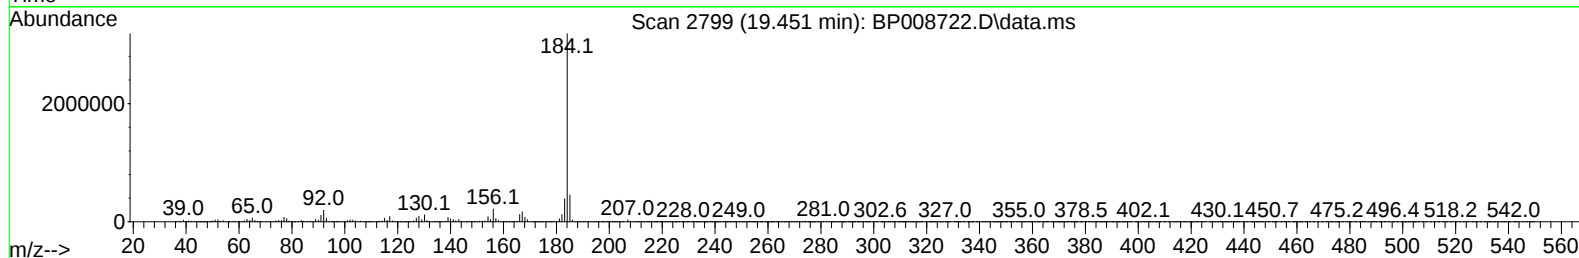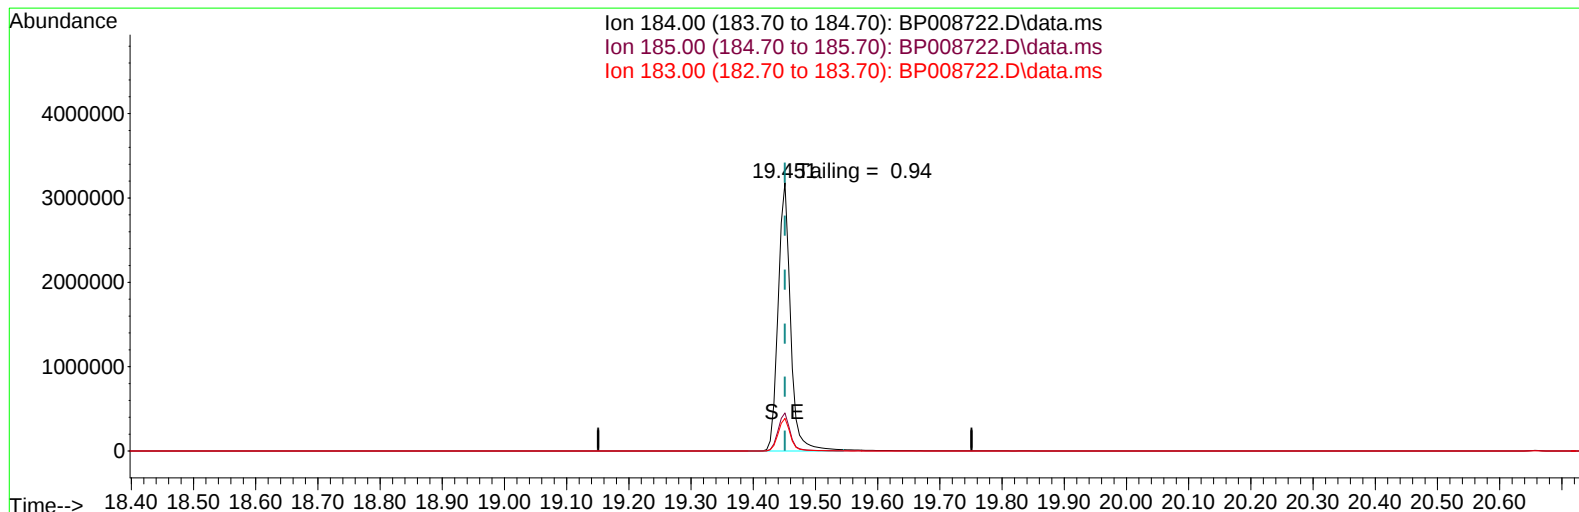

TIC: BP008722.D\data.ms

(77) Benzidine**19.451min (-0.000) 1530289.46 ng****response 4452577**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.22
183.00	11.90	12.17
0.00	0.00	0.00