

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP010722\  
 Data File : BP008728.D  
 Acq On : 07 Jan 2022 16:09  
 Operator : CG/JU  
 Sample : PB141824BL  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 PB141824BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP010622.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008728.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.452       | 412           | 419         | 438          | rBV      | 4076544        | 6498662       | 28.69%          | 8.079%        |
| 2         | 7.046       | 682           | 690         | 716          | rBV      | 4043215        | 6919108       | 30.55%          | 8.602%        |
| 3         | 7.869       | 824           | 830         | 844          | rVB      | 761629         | 1282101       | 5.66%           | 1.594%        |
| 4         | 9.028       | 1019          | 1027        | 1045         | rBV      | 2008880        | 3450198       | 15.23%          | 4.289%        |
| 5         | 10.675      | 1299          | 1307        | 1328         | rBV      | 897450         | 1614797       | 7.13%           | 2.008%        |
| 6         | 13.134      | 1716          | 1725        | 1748         | rBV      | 6871899        | 10714821      | 47.31%          | 13.321%       |
| 7         | 14.510      | 1950          | 1959        | 1980         | rBV      | 1606072        | 2649346       | 11.70%          | 3.294%        |
| 8         | 15.998      | 2205          | 2212        | 2249         | rBV      | 5571392        | 9778606       | 43.17%          | 12.157%       |
| 9         | 17.257      | 2420          | 2426        | 2441         | rBV      | 2391322        | 3801929       | 16.79%          | 4.727%        |
| 10        | 19.822      | 2856          | 2862        | 2874         | rBV      | 18285279       | 22649355      | 100.00%         | 28.158%       |
| 11        | 21.345      | 3116          | 3121        | 3132         | rBV      | 3707708        | 5254256       | 23.20%          | 6.532%        |
| 12        | 23.774      | 3527          | 3534        | 3547         | rVB2     | 2807731        | 5823992       | 25.71%          | 7.240%        |




Sum of corrected areas: 80437171

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP010722\  
Data File : BP008728.D  
Acq On : 07 Jan 2022 16:09  
Operator : CG/JU  
Sample : PB141824BL  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB141824BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP010622.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

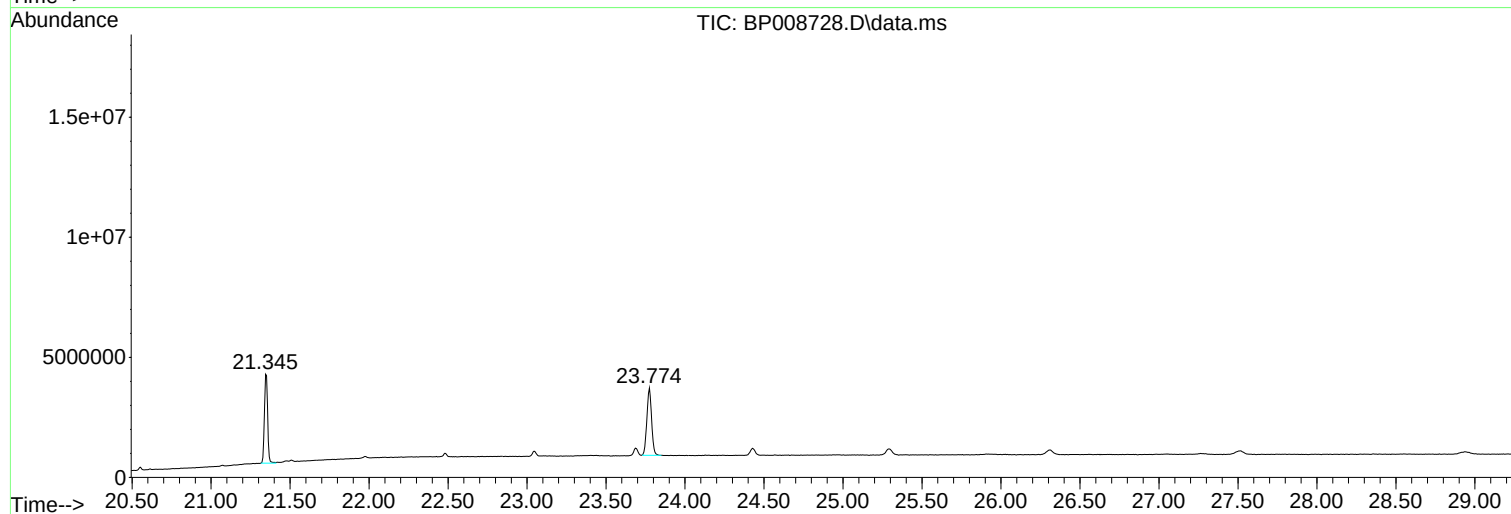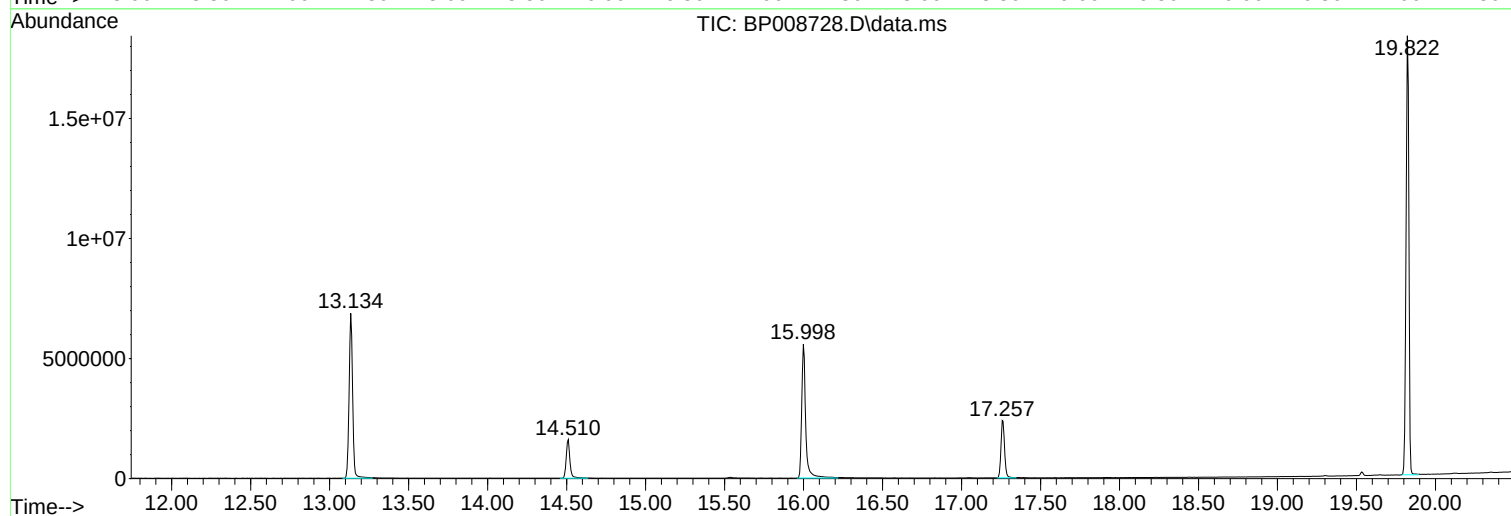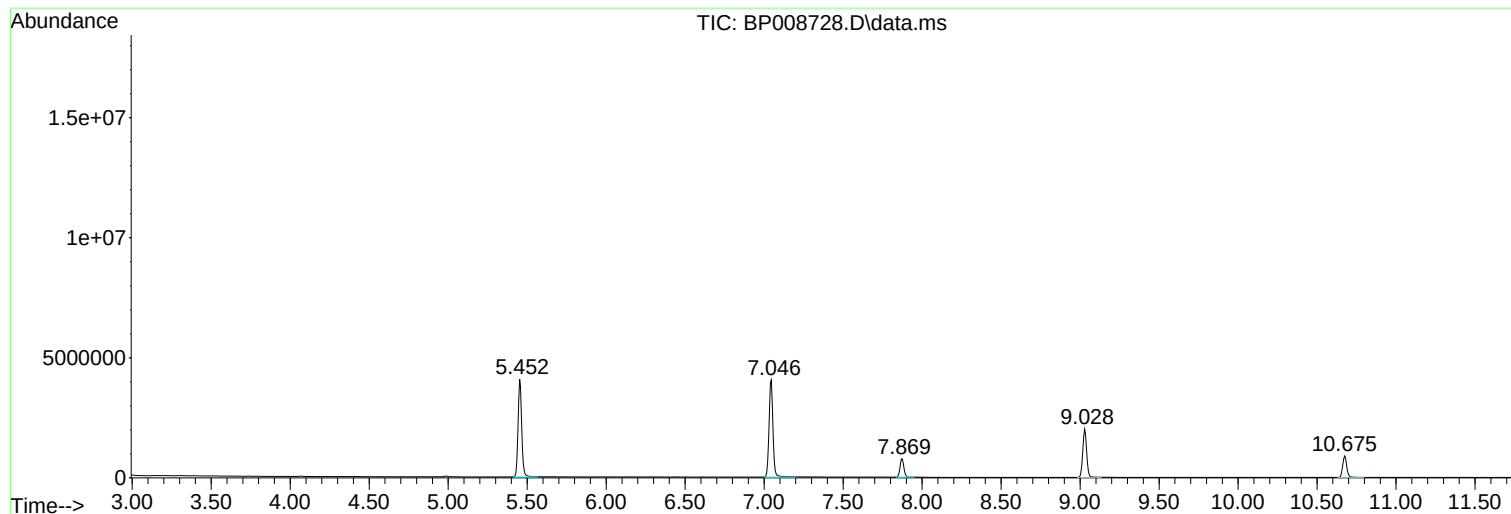

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP010722\  
Data File : BP008728.D  
Acq On : 07 Jan 2022 16:09  
Operator : CG/JU  
Sample : PB141824BL  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB141824BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP010622.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP010722\  
Data File : BP008728.D  
Acq On : 07 Jan 2022 16:09  
Operator : CG/JU  
Sample : PB141824BL  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
PB141824BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP010622.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|