
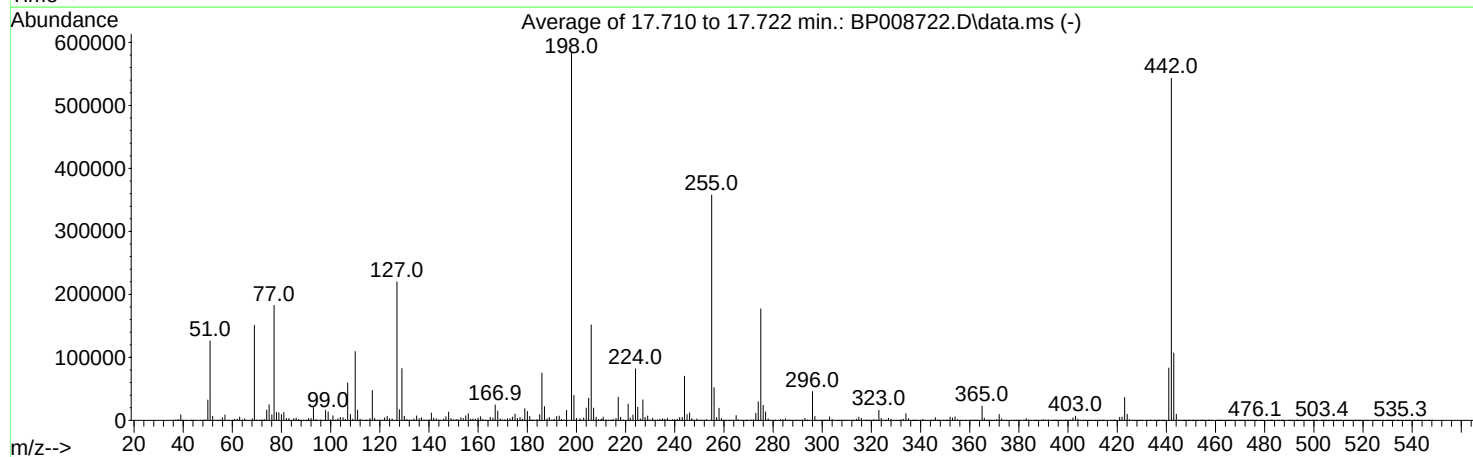


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010722\
 Data File : BP008722.D
 Acq On : 07 Jan 2022 12:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 07 07:45:52 2022

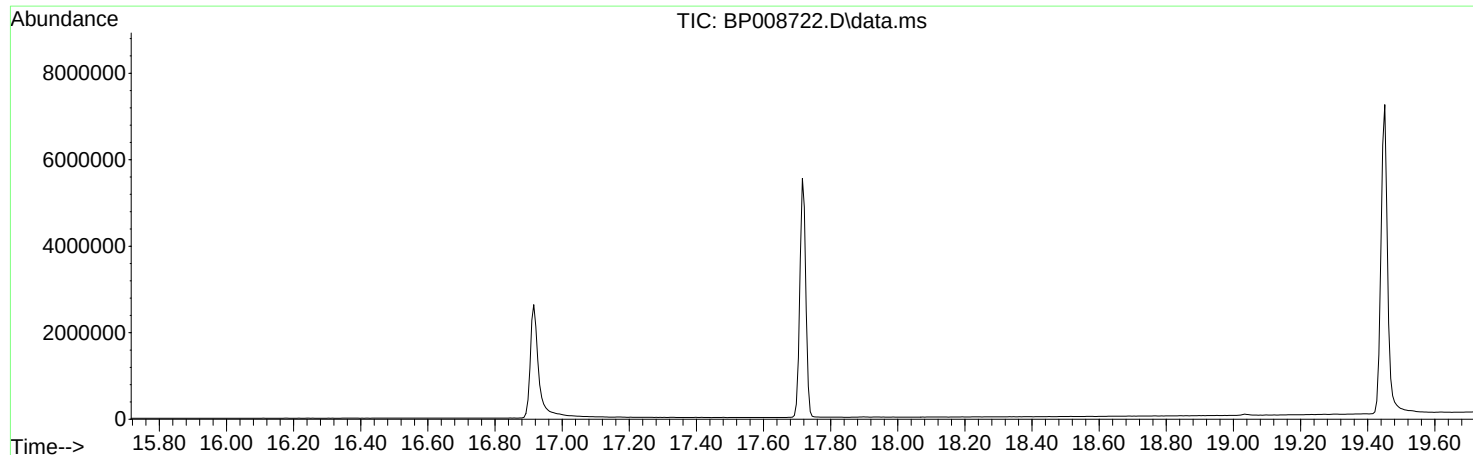

AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.6	126304	PASS
68	69	0.00	2	1.7	2626	PASS
69	198	0.00	100	25.9	151171	PASS
70	69	0.00	2	0.5	719	PASS
127	198	10	80	37.7	220102	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	584009	PASS
199	198	5	9	6.8	39700	PASS
275	198	10	60	30.3	177012	PASS
365	198	1	100	3.9	22497	PASS
441	198	0.01	100	14.2	83045	PASS
442	442	100	100	100.0	543158	PASS
443	442	15	24	19.7	106957	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/7/2022	BNA_P	<u>BP008722.D</u>
Compound Name	Response	Retention Time
DDT	2234063	20.65
DDD	18269	20.22
DDE	3534	19.73
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21803	2255866	0.97

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010722\
 Data File : BP008722.D
 Acq On : 07 Jan 2022 12:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jan 07 17:15:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 07 07:45:52 2022
 Response via : Initial Calibration

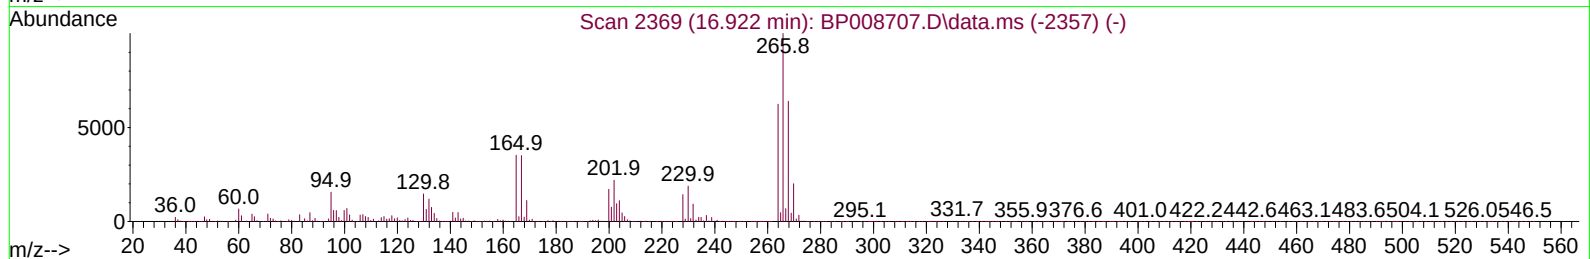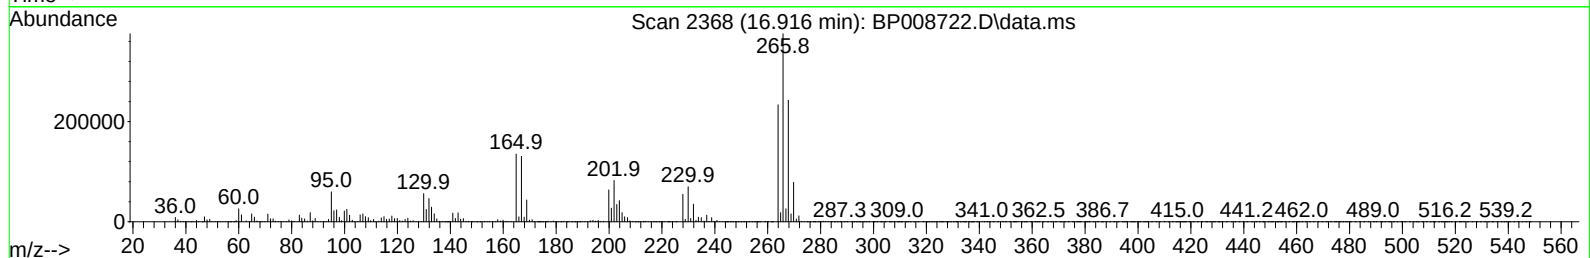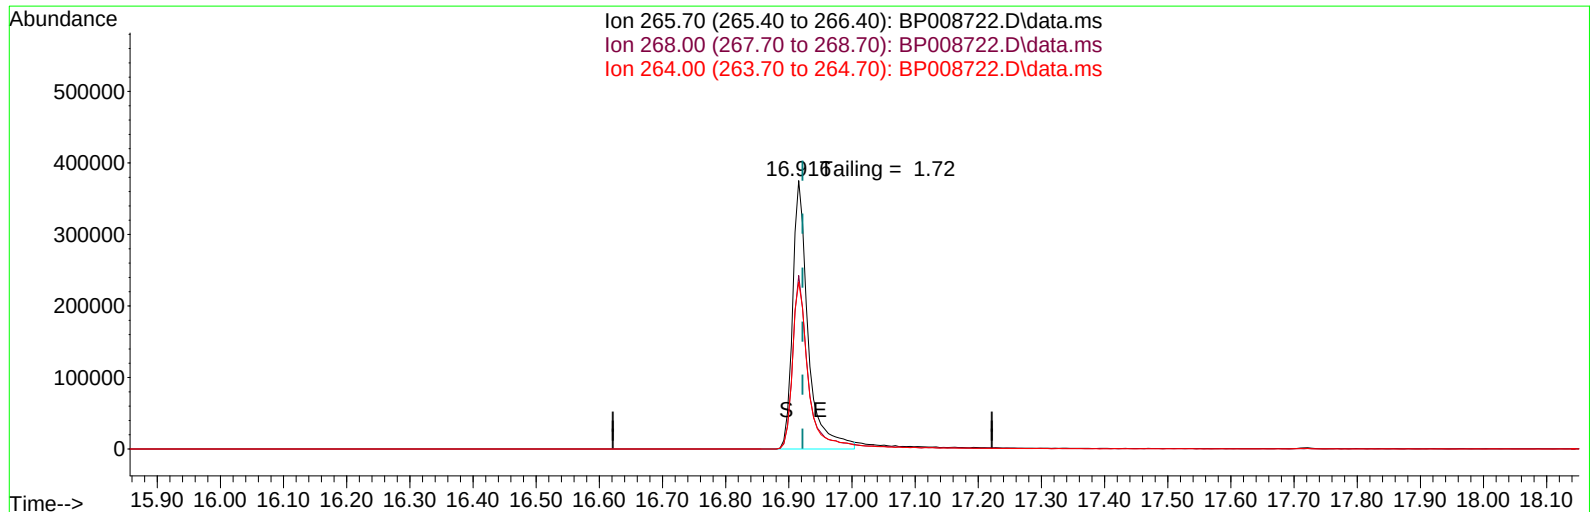

TIC: BP008722.D\data.ms

(70) Pentachlorophenol (C)

16.916min (-0.006) 3296901.96 ng




response 679987

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.61
264.00	62.90	62.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010722\
Data File : BP008722.D
Acq On : 07 Jan 2022 12:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 07 17:15:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 07 07:45:52 2022
Response via : Initial Calibration

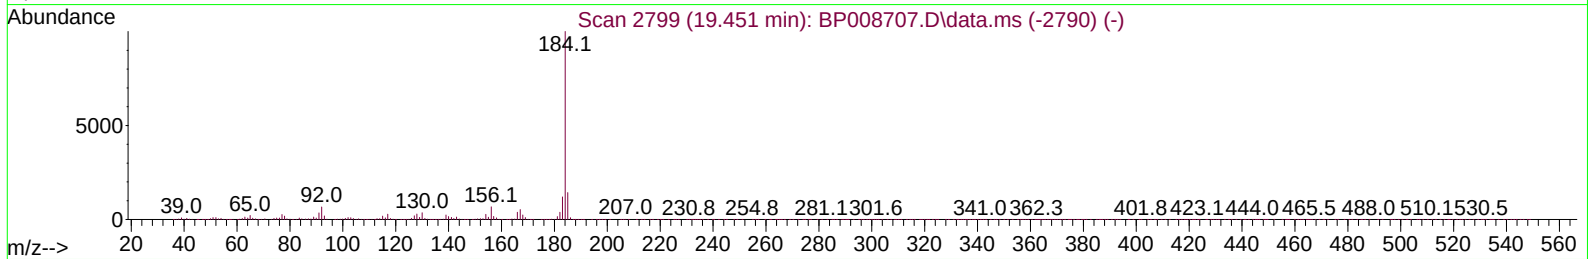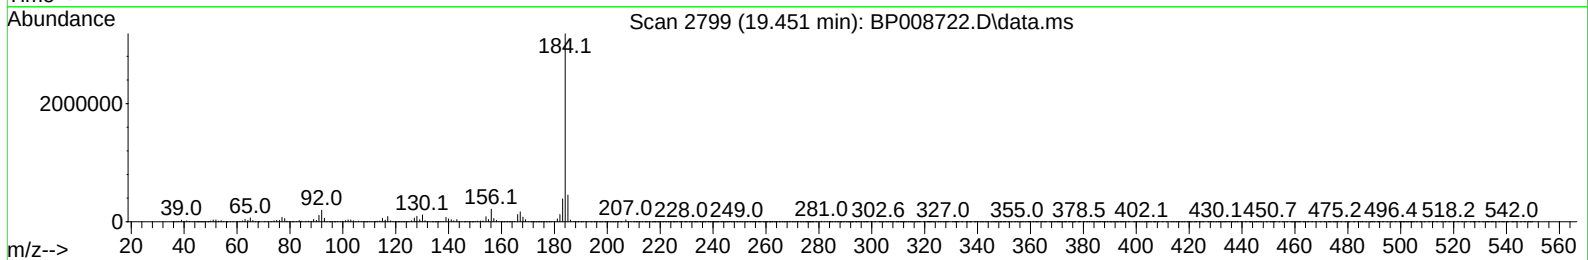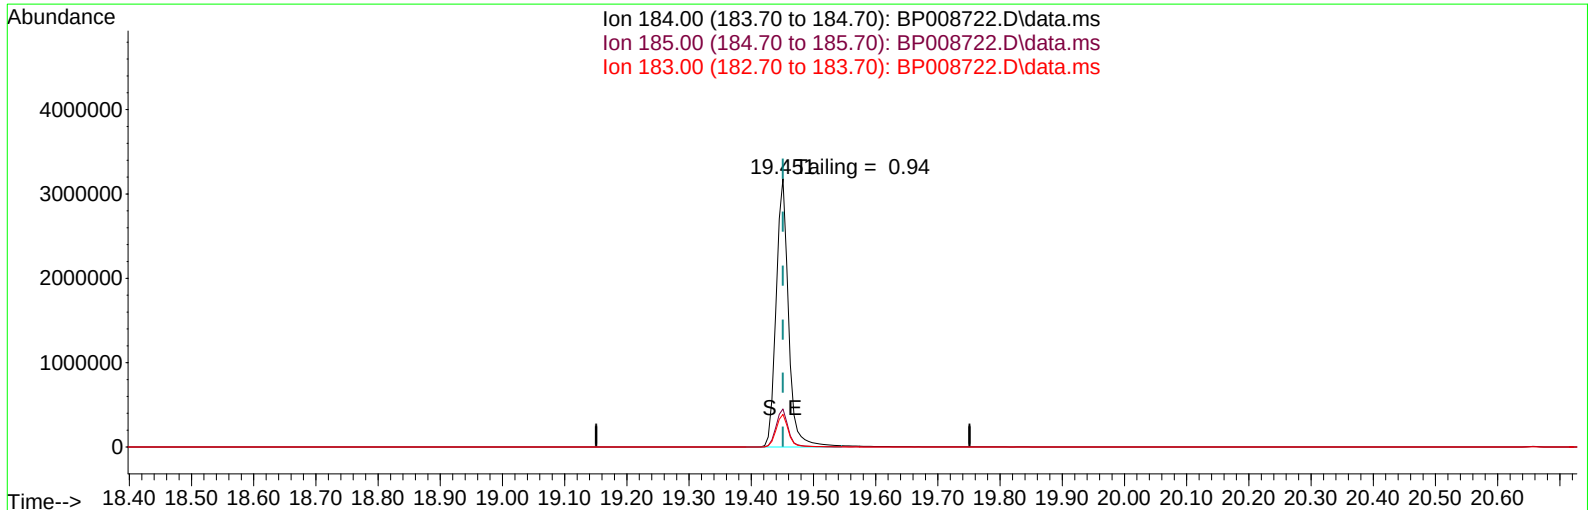

TIC: BP008722.D\data.ms

(77) Benzidine

19.451min (-0.000) 1530289.46 ng

response 4452577

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.22
183.00	11.90	12.17
0.00	0.00	0.00