

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010824\
 Data File : BP019305.D
 Acq On : 08 Jan 2024 20:42
 Operator : MA/JU
 Sample : SST080808
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST080648

Quant Time: Jan 09 01:57:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 09 01:51:15 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.787	152	134634	20.000	ng/u1	0.00
20) Naphthalene-d8	10.581	136	544362	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.428	164	381659	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.186	188	896126	20.000	ng/u1	0.00
79) Chrysene-d12	21.292	240	889135	20.000	ng/u1	0.00
88) Perylene-d12	23.645	264	812378	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.217	96	113570	28.810	ng/uL	0.00
4) Pyridine-d5	3.640	84	844032	85.304	ng/u1	0.00
7) Phenol-d5	6.981	99	1073057	88.876	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.134	67	618340	88.527	ng/u1	0.00
11) 2-Chlorophenol-d4	7.322	132	760261	78.108	ng/u1	0.00
15) 4-Methylphenol-d8	8.528	113	851556	90.592	ng/u1	0.01
21) Nitrobenzene-d5	8.957	128	394437	83.821	ng/u1	0.00
24) 2-Nitrophenol-d4	9.675	143	475985	93.594	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.216	165	922684	89.847	ng/u1	0.00
31) 4-Chloroaniline-d4	10.740	131	1128036	89.302	ng/u1	0.01
46) Dimethylphthalate-d6	13.857	166	2789793	82.756	ng/u1	0.01
49) Acenaphthylene-d8	14.128	160	3013681	82.390	ng/u1	0.00
54) 4-Nitrophenol-d4	14.687	143	448739	78.829	ng/u1	0.02
60) Fluorene-d10	15.428	176	2288201	78.569	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.575	200	578954	98.550	ng/u1	0.01
73) Anthracene-d10	17.292	188	3783438	80.845	ng/u1	0.00
81) Pyrene-d10	19.533	212	4706229	86.851	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.498	264	3847767	82.401	ng/u1	0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.252	88	119129	27.485	ng/uL	99
5) Pyridine	3.658	79	847210	84.355	ng/u1	96
6) Benzaldehyde	6.934	77	359483	64.126	ng/u1	97
8) Phenol	7.010	94	1073703	90.035	ng/u1	97
10) Bis(2-Chloroethyl)ether	7.222	93	838634	86.914	ng/u1	98
12) 2-Chlorophenol	7.358	128	780492	78.345	ng/u1	98
13) 2-Methylphenol	8.252	108	807924	91.581	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.316	45	989062	86.893	ng/u1	100
16) Acetophenone	8.622	105	1332439	94.646	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.622	70	693797	98.831	ng/u1	98
18) 4-Methylphenol	8.593	108	857408	90.293	ng/u1	96
19) Hexachloroethane	8.852	117	337525	80.774	ng/u1	99
22) Nitrobenzene	9.005	77	1073274	93.357	ng/u1	96
23) Isophorone	9.534	82	2062628	99.494	ng/u1	99
25) 2-Nitrophenol	9.710	139	481718	88.714	ng/u1	99
26) 2,4-Dimethylphenol	9.781	107	1008454	105.492	ng/u1	99
27) Bis(2-Chloroethoxy)met...	10.010	93	1149360	83.882	ng/u1	99
29) 2,4-Dichlorophenol	10.246	162	890173	88.703	ng/u1	100
30) Naphthalene	10.634	128	2526717	76.986	ng/u1	100
32) 4-Chloroaniline	10.763	127	1110619	91.629	ng/u1	99
33) Hexachlorobutadiene	10.910	225	727645	94.215	ng/u1	99
34) Caprolactam	11.593	113	150109	56.629	ng/u1	93
35) 4-Chloro-3-methylphenol	11.910	107	978084	99.285	ng/u1	95
36) 2-Methylnaphthalene	12.251	142	1830521	82.723	ng/u1	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010824\
 Data File : BP019305.D
 Acq On : 08 Jan 2024 20:42
 Operator : MA/JU
 Sample : SST080808
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST080648

Quant Time: Jan 09 01:57:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 09 01:51:15 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.469	142	1794287	80.408	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.616	216	1392648	88.598	ng/ul	98
40) Hexachlorocyclopentadiene	12.587	237	887882	101.765	ng/ul	99
41) 2,4,6-Trichlorophenol	12.869	196	881404	93.959	ng/ul	98
42) 2,4,5-Trichlorophenol	12.951	196	950349	95.437	ng/ul	99
43) 1,1'-Biphenyl	13.269	154	2571017	77.224	ng/ul	100
44) 2-Chloronaphthalene	13.310	162	2099885	78.604	ng/ul	99
45) 2-Nitroaniline	13.534	65	655375	102.190	ng/ul	94
47) Dimethylphthalate	13.904	163	2774394	83.373	ng/ul	100
48) 2,6-Dinitrotoluene	14.034	165	604007	98.778	ng/ul	96
50) Acenaphthylene	14.157	152	3278899	79.672	ng/ul	99
51) 3-Nitroaniline	14.363	138	474636	79.398	ng/ul	96
52) Acenaphthene	14.498	153	2154065	77.227	ng/ul	99
53) 2,4-Dinitrophenol	14.575	184	397110	100.804	ng/ul	92
55) 4-Nitrophenol	14.704	109	478136	105.098	ng/ul	94
56) Dibenzofuran	14.834	168	3001362	75.350	ng/ul	99
57) 2,4-Dinitrotoluene	14.828	165	832507	92.573	ng/ul	99
58) 2,3,4,6-Tetrachlorophenol	15.069	232	859211	98.759	ng/ul	98
59) Diethylphthalate	15.269	149	2601011	80.615	ng/ul	100
61) Fluorene	15.487	166	2513748	78.846	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.481	204	1528698	87.802	ng/ul	97
63) 4-Nitroaniline	15.539	138	350191	58.224	ng/ul	98
66) 4,6-Dinitro-2-methylph...	15.592	198	603352	97.000	ng/ul#	94
67) N-Nitrosodiphenylamine	15.704	169	2138137	78.178	ng/ul	99
68) 4-Bromophenyl-phenylether	16.375	248	1024875	92.015	ng/ul	98
69) Hexachlorobenzene	16.492	284	1181960	86.834	ng/ul	97
70) Atrazine	16.669	200	944226	122.334	ng/ul	98
71) Pentachlorophenol	16.845	266	763634	95.554	ng/ul	99
72) Phenanthrene	17.233	178	4220283	77.712	ng/ul	99
74) Anthracene	17.328	178	4261809	78.828	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.228	216	1353868	86.891	ng/ul	99
76) Pentachlorobenzene	14.751	250	1307643	84.457	ng/ul	99
77) Carbazole	17.604	167	3593511	79.907	ng/ul	100
78) Di-n-butylphthalate	18.151	149	4455459	79.884	ng/ul	99
80) Fluoranthene	19.210	202	5451354	87.670	ng/ul	98
82) Pyrene	19.563	202	5560467	85.352	ng/ul	98
83) Butylbenzylphthalate	20.439	149	2018640	86.745	ng/ul	91
84) 3,3'-Dichlorobenzidine	21.216	252	1592861	71.614	ng/ul	97
85) Benzo(a)anthracene	21.280	228	5748646	81.831	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.198	149	2912070	84.983	ng/ul	98
87) Chrysene	21.333	228	5146468	78.564	ng/ul	99
89) Di-n-octyl phthalate	22.104	149	4802067	103.368	ng/ul	100
90) Benzo(b)fluoranthene	22.933	252	5066092	88.782	ng/ul	100
91) Benzo(k)fluoranthene	22.980	252	4857990	86.640	ng/ul	99
93) Benzo(a)pyrene	23.551	252	4452797	82.908	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.109	276	4817788	69.976	ng/ul	99
95) Dibenzo(a,h)anthracene	26.121	278	4017436	70.143	ng/ul	99
96) Benzo(g,h,i)perylene	26.857	276	3727305	67.556	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010824\
 Data File : BP019305.D
 Acq On : 08 Jan 2024 20:42
 Operator : MA/JU
 Sample : SST0808080
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST080648

Quant Time: Jan 09 01:57:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 09 01:51:15 2024
 Response via : Initial Calibration




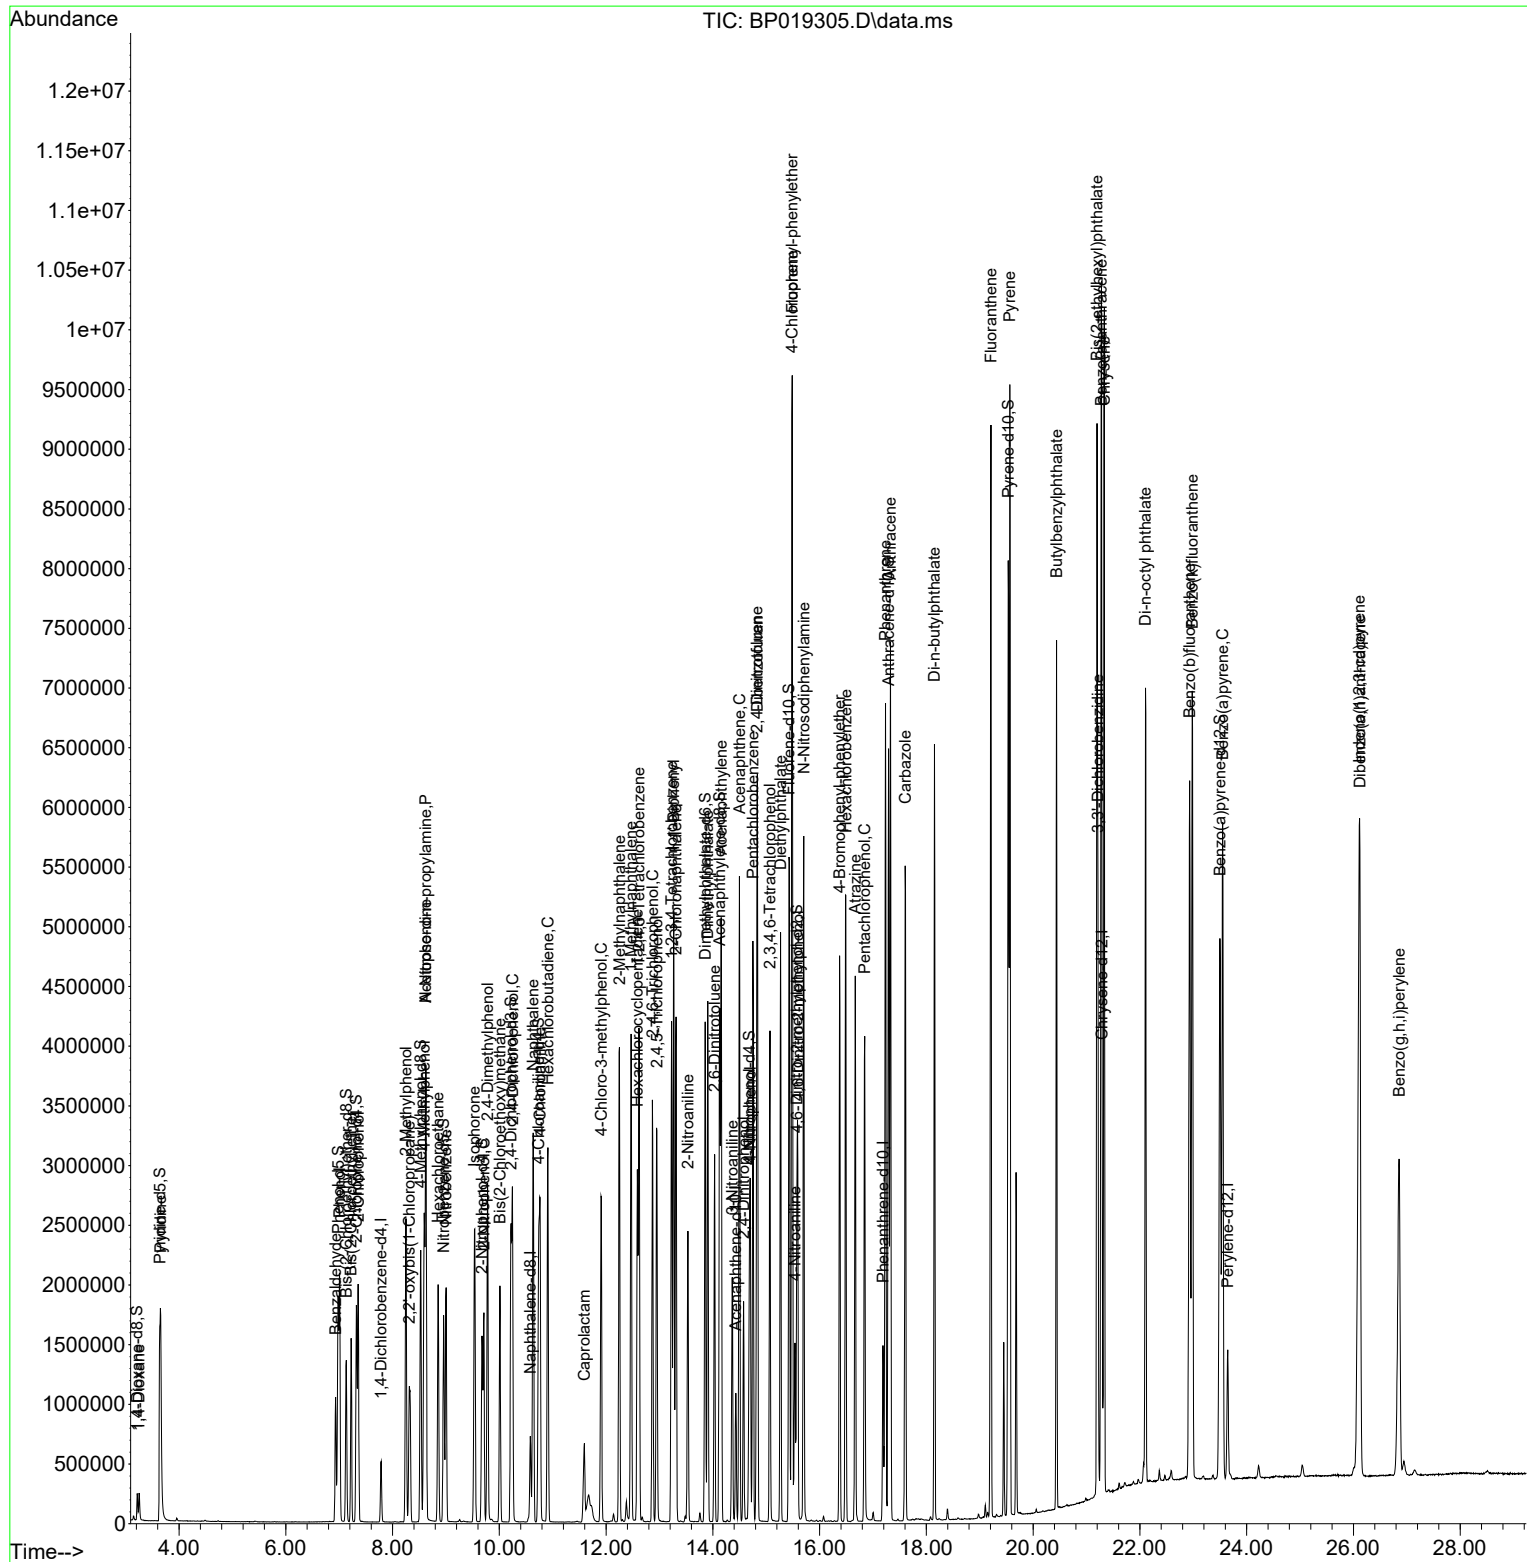


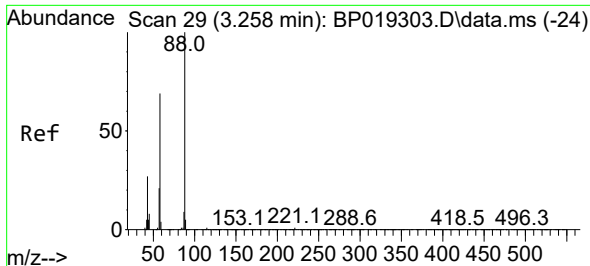

#2
1,4-Dioxane
Concen: 27.485 ng/uL
RT: 3.252 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42




Instrument :
BNA_P
ClientSampleId :
SSTD080648


Tgt Ion: 88 Resp: 119129
Ion Ratio Lower Upper
88 100
43 27.2 22.0 33.0
58 67.1 54.6 82.0

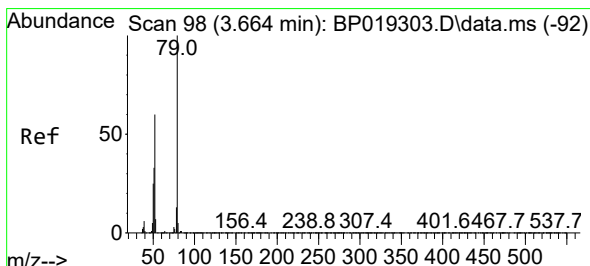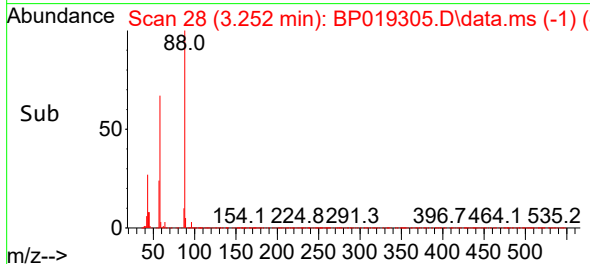

#5
Pyridine
Concen: 84.355 ng/uL
RT: 3.658 min Scan# 97
Delta R.T. -0.006 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42

Tgt Ion: 79 Resp: 847210
Ion Ratio Lower Upper
79 100
52 68.1 50.7 76.1
51 32.7 26.8 40.2


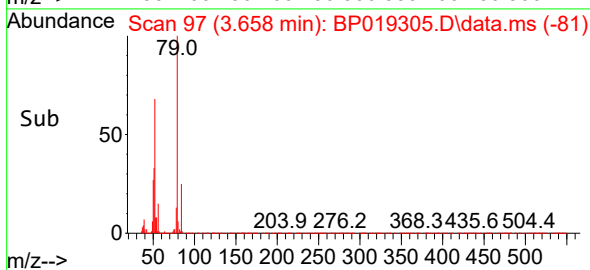

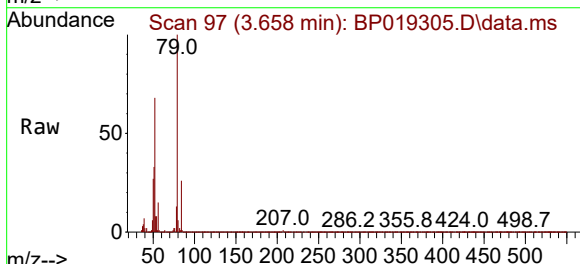




#6
Benzaldehyde
Concen: 64.126 ng/ul
RT: 6.934 min Scan# 61
Delta R.T. -0.000 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42




Instrument :
BNA_P
ClientSampleId :
SSTD080648


Tgt Ion: 77 Resp: 359483
Ion Ratio Lower Upper
77 100
105 92.0 75.3 112.9
106 85.4 71.5 107.3



#8
Phenol
Concen: 90.035 ng/ul
RT: 7.010 min Scan# 667
Delta R.T. 0.012 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42

Tgt Ion: 94 Resp: 1073703
Ion Ratio Lower Upper
94 100
65 30.2 25.3 37.9
66 44.2 36.8 55.2



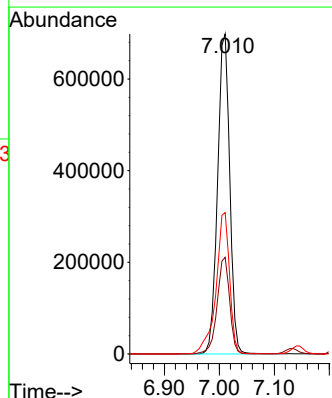





#10
Bis(2-Chloroethyl)ether
Concen: 86.914 ng/ul
RT: 7.222 min Scan# 703
Delta R.T. 0.006 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42




Instrument :
BNA_P
ClientSampleId :
SSTD080648


Tgt Ion: 93 Resp: 838634
Ion Ratio Lower Upper
93 100
63 73.8 60.7 91.1
95 31.3 26.2 39.2



#12
2-Chlorophenol
Concen: 78.345 ng/ul
RT: 7.358 min Scan# 726
Delta R.T. 0.006 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42

Tgt Ion:128 Resp: 780492
Ion Ratio Lower Upper
128 100
64 49.8 41.3 61.9
130 32.3 25.9 38.9









#13
2-Methylphenol
Concen: 91.581 ng/ul
RT: 8.252 min Scan# 81
Delta R.T. 0.006 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42




Instrument :
BNA_P
ClientSampleId :
SSTD080648


Tgt Ion:108 Resp: 807924
Ion Ratio Lower Upper
108 100
107 91.0 71.9 107.9



#14
2,2'-oxybis(1-Chloropropane)
Concen: 86.893 ng/ul
RT: 8.316 min Scan# 889
Delta R.T. 0.006 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42

Tgt Ion: 45 Resp: 989062
Ion Ratio Lower Upper
45 100
77 17.9 14.2 21.4
79 13.2 10.5 15.7




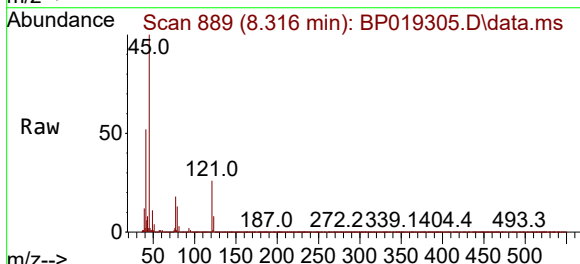




#16
Acetophenone
Concen: 94.646 ng/ul
RT: 8.622 min Scan# 941
Delta R.T. 0.006 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42




Instrument :
BNA_P
ClientSampleId :
SSTD080648


Tgt Ion:105 Resp: 1332439
Ion Ratio Lower Upper
105 100
77 80.3 66.1 99.1
51 25.1 20.9 31.3



#17
N-Nitroso-di-n-propylamine
Concen: 98.831 ng/ul
RT: 8.622 min Scan# 941
Delta R.T. 0.024 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42

Tgt Ion: 70 Resp: 693797
Ion Ratio Lower Upper
70 100
42 49.3 38.5 57.7
101 9.8 7.9 11.9
130 19.1 14.3 21.5



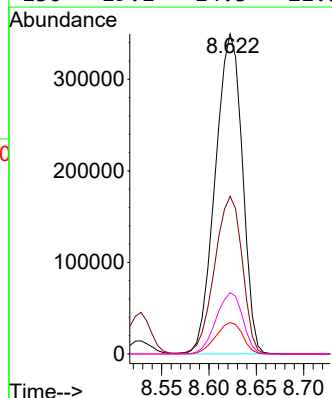





#18
4-Methylphenol
Concen: 90.293 ng/ul
RT: 8.593 min Scan# 91
Delta R.T. 0.018 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42




Instrument :
BNA_P
ClientSampleId :
SSTD080648


Tgt Ion:108 Resp: 857408
Ion Ratio Lower Upper
108 100
107 111.9 92.6 139.0



#19
Hexachloroethane
Concen: 80.774 ng/ul
RT: 8.852 min Scan# 980
Delta R.T. -0.000 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42

Tgt Ion:117 Resp: 337525
Ion Ratio Lower Upper
117 100
201 128.7 101.8 152.6
199 79.6 62.6 93.8



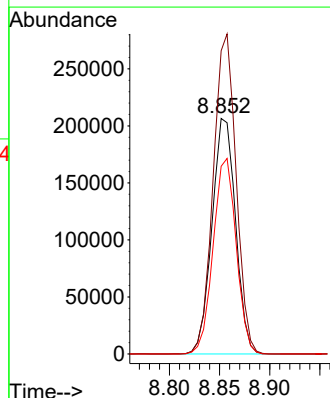





#22
Nitrobenzene
Concen: 93.357 ng/ul
RT: 9.005 min Scan# 1006
Delta R.T. 0.012 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42




Instrument :
BNA_P
ClientSampleId :
SSTD080648


Tgt Ion: 77 Resp: 1073274
Ion Ratio Lower Upper
77 100
123 40.4 30.0 45.0
65 13.5 10.5 15.7



#23
Isophorone
Concen: 99.494 ng/ul
RT: 9.534 min Scan# 1096
Delta R.T. 0.012 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42

Tgt Ion: 82 Resp: 2062628
Ion Ratio Lower Upper
82 100
95 8.3 6.6 10.0
138 15.5 13.0 19.4









#25
2-Nitrophenol
Concen: 88.714 ng/ul
RT: 9.710 min Scan# 1125
Delta R.T. 0.006 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42




Instrument :
BNA_P
ClientSampleId :
SSTD080648


Tgt Ion:139 Resp: 481718
Ion Ratio Lower Upper
139 100
65 56.1 45.6 68.4
109 41.3 32.6 49.0



#26
2,4-Dimethylphenol
Concen: 105.492 ng/ul
RT: 9.781 min Scan# 1138
Delta R.T. 0.006 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42

Tgt Ion:107 Resp: 1008454
Ion Ratio Lower Upper
107 100
121 45.0 35.3 52.9
122 75.4 60.6 91.0









#27
Bis(2-Chloroethoxy)methane
Concen: 83.882 ng/ul
RT: 10.010 min Scan# 1177
Delta R.T. 0.006 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42




Instrument :
BNA_P
ClientSampleId :
SSTD080648


Tgt Ion: 93 Resp: 1149360
Ion Ratio Lower Upper
93 100
95 31.9 25.9 38.9
123 10.0 7.9 11.9



#29
2,4-Dichlorophenol
Concen: 88.703 ng/ul
RT: 10.246 min Scan# 1217
Delta R.T. 0.006 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42

Tgt Ion:162 Resp: 890173
Ion Ratio Lower Upper
162 100
164 65.6 52.3 78.5
98 35.9 28.3 42.5




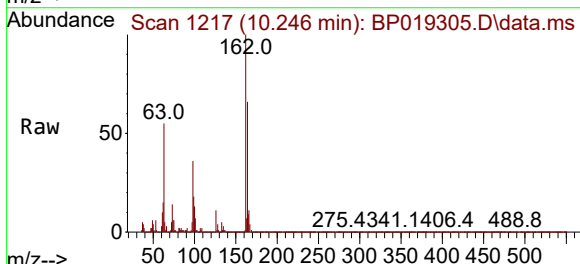




#30
Naphthalene
Concen: 76.986 ng/ul
RT: 10.634 min Scan# 1282
Delta R.T. 0.006 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42




Instrument :
BNA_P
ClientSampleId :
SSTD080648


Tgt Ion:128 Resp: 2526717
Ion Ratio Lower Upper
128 100
129 10.9 8.6 12.8
127 13.3 10.6 15.8



#32
4-Chloroaniline
Concen: 91.629 ng/ul
RT: 10.763 min Scan# 1305
Delta R.T. 0.006 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42

Tgt Ion:127 Resp: 1110619
Ion Ratio Lower Upper
127 100
129 31.5 25.8 38.8

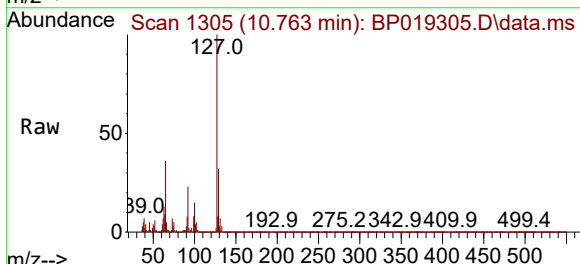



#33

Hexachlorobutadiene

Concen: 94.215 ng/ul

RT: 10.910 min Scan# 11

Delta R.T. 0.006 min

Lab File: BP019305.D

Acq: 08 Jan 2024 20:42

Instrument :

BNA_P

ClientSampleId :

SSTD080648





Tgt Ion:225 Resp: 727645

Ion Ratio Lower Upper

225 100

223 62.7 49.9 74.9

227 64.4 51.0 76.6

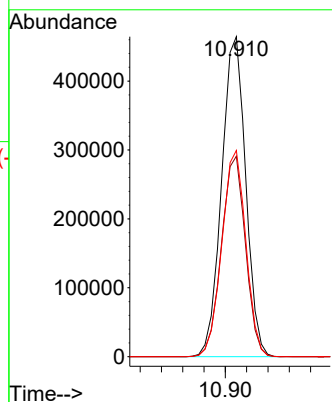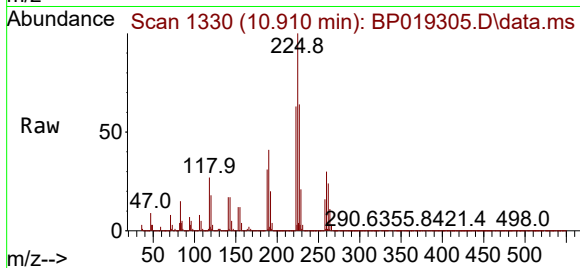

#34

Caprolactam

Concen: 56.629 ng/ul

RT: 11.593 min Scan# 1446

Delta R.T. 0.047 min

Lab File: BP019305.D

Acq: 08 Jan 2024 20:42




Tgt Ion:113 Resp: 150109


Ion Ratio Lower Upper

113 100

55 159.7 133.3 199.9

56 125.0 108.0 162.0









#35
4-Chloro-3-methylphenol
Concen: 99.285 ng/ul
RT: 11.910 min Scan# 11
Delta R.T. 0.018 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42




Instrument :
BNA_P
ClientSampleId :
SSTD080648


Tgt Ion:107 Resp: 978084
Ion Ratio Lower Upper
107 100
144 24.3 17.8 26.8
142 74.6 56.3 84.5

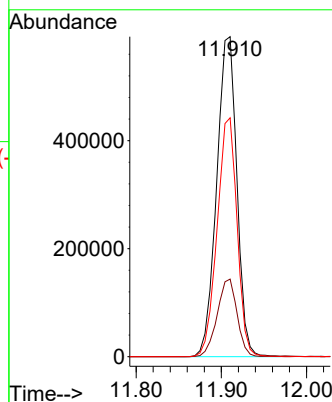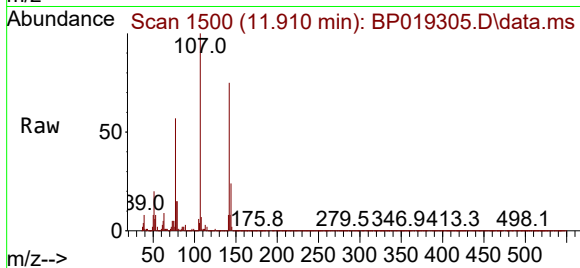

#36
2-Methylnaphthalene
Concen: 82.723 ng/ul
RT: 12.251 min Scan# 1558
Delta R.T. 0.006 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42

Tgt Ion:142 Resp: 1830521
Ion Ratio Lower Upper
142 100
141 89.5 71.1 106.7









#37
1-Methylnaphthalene
Concen: 80.408 ng/ul
RT: 12.469 min Scan# 1594
Delta R.T. 0.006 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42




Instrument :
BNA_P
ClientSampleId :
SSTD080648


Tgt Ion:142 Resp: 1794287
Ion Ratio Lower Upper
142 100
141 92.9 74.4 111.6
116 4.5 3.9 5.9



#39
1,2,4,5-Tetrachlorobenzene
Concen: 88.598 ng/ul
RT: 12.616 min Scan# 1620
Delta R.T. -0.000 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42

Tgt Ion:216 Resp: 1392648
Ion Ratio Lower Upper
216 100
214 77.8 63.6 95.4
179 19.1 15.1 22.7
108 13.5 11.3 16.9



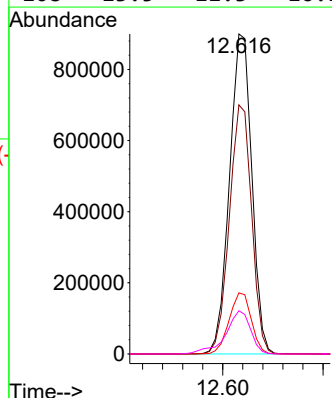
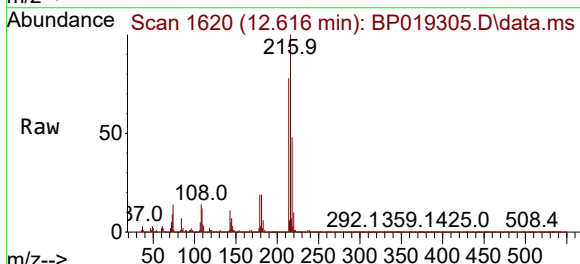




#40
Hexachlorocyclopentadiene
Concen: 101.765 ng/ul
RT: 12.587 min Scan# 1615
Delta R.T. -0.000 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42




Instrument :
BNA_P
ClientSampleId :
SSTD080648


Tgt Ion:237 Resp: 887882
Ion Ratio Lower Upper
237 100
235 62.6 50.0 75.0
272 12.6 11.4 17.2

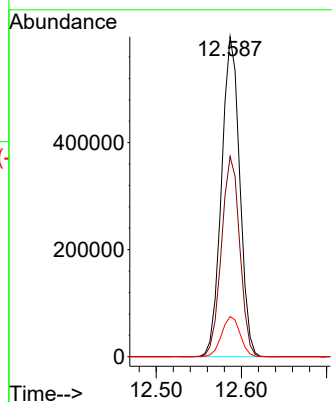

#41
2,4,6-Trichlorophenol
Concen: 93.959 ng/ul
RT: 12.869 min Scan# 1663
Delta R.T. 0.006 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42

Tgt Ion:196 Resp: 881404
Ion Ratio Lower Upper
196 100
198 95.6 78.2 117.2
200 31.8 24.6 36.8









#42
2,4,5-Trichlorophenol
Concen: 95.437 ng/ul
RT: 12.951 min Scan# 1677
Delta R.T. 0.006 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42




Instrument :
BNA_P
ClientSampleId :
SSTD080648


Tgt Ion:196 Resp: 950349
Ion Ratio Lower Upper
196 100
198 97.1 78.9 118.3
200 31.1 25.0 37.6



#43
1,1'-Biphenyl
Concen: 77.224 ng/ul
RT: 13.269 min Scan# 1731
Delta R.T. 0.006 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42

Tgt Ion:154 Resp: 2571017
Ion Ratio Lower Upper
154 100
153 40.7 32.6 48.8
76 11.3 9.3 13.9









#44
2-Chloronaphthalene
Concen: 78.604 ng/ul
RT: 13.310 min Scan# 1738
Delta R.T. 0.006 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42




Instrument :
BNA_P
ClientSampleId :
SSTD080648


Tgt Ion:162 Resp: 2099885
Ion Ratio Lower Upper
162 100
164 33.7 26.6 40.0
127 37.0 29.4 44.2



#45
2-Nitroaniline
Concen: 102.190 ng/ul
RT: 13.534 min Scan# 1776
Delta R.T. 0.012 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42

Tgt Ion: 65 Resp: 655375
Ion Ratio Lower Upper
65 100
92 69.5 52.1 78.1
138 100.0 74.8 112.2









#47
Dimethylphthalate
Concen: 83.373 ng/ul
RT: 13.904 min Scan# 1839
Delta R.T. 0.012 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42




Instrument :
BNA_P
ClientSampleId :
SSTD080648


Tgt Ion:163 Resp: 2774394
Ion Ratio Lower Upper
163 100
194 4.4 3.4 5.2
164 10.2 8.1 12.1

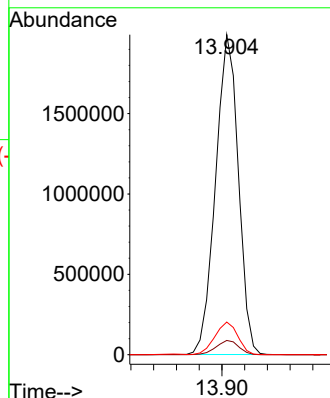

#48
2,6-Dinitrotoluene
Concen: 98.778 ng/ul
RT: 14.034 min Scan# 1861
Delta R.T. 0.012 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42

Tgt Ion:165 Resp: 604007
Ion Ratio Lower Upper
165 100
89 58.4 49.9 74.9
121 19.8 16.5 24.7



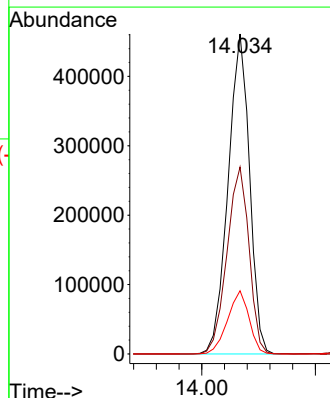



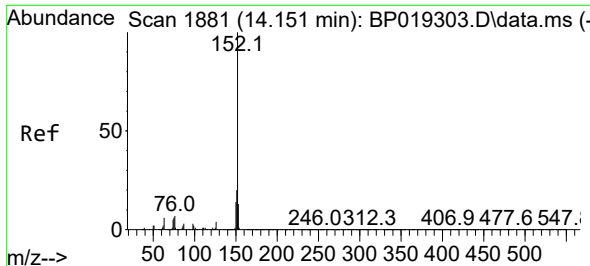

#50
Acenaphthylene
Concen: 79.672 ng/ul
RT: 14.157 min Scan# 1881
Delta R.T. 0.006 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42




Instrument :
BNA_P
ClientSampleId :
SSTD080648


Tgt Ion:152 Resp: 3278899
Ion Ratio Lower Upper
152 100
151 20.2 15.8 23.6
153 13.4 10.3 15.5

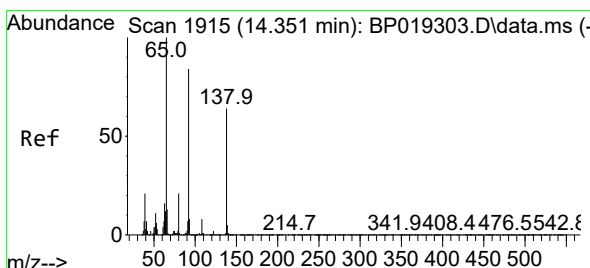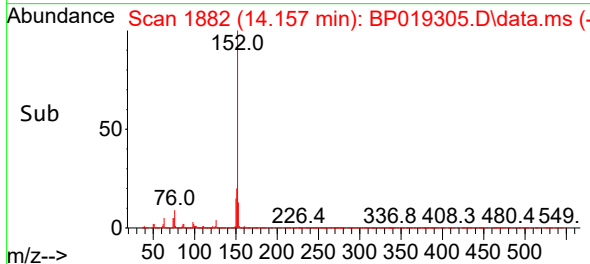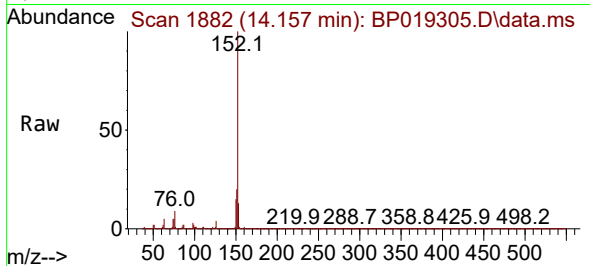

#51
3-Nitroaniline
Concen: 79.398 ng/ul
RT: 14.363 min Scan# 1917
Delta R.T. 0.012 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42

Tgt Ion:138 Resp: 474636
Ion Ratio Lower Upper
138 100
108 11.4 10.6 15.8
92 127.7 105.8 158.6


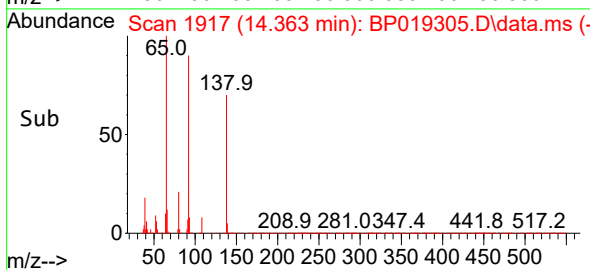

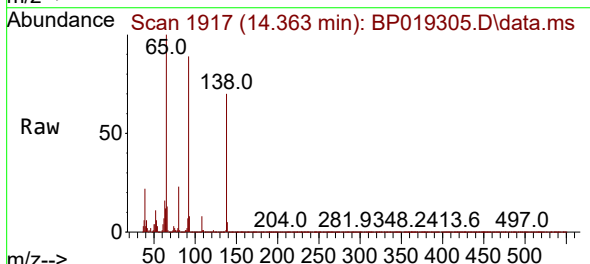




#52
Acenaphthene
Concen: 77.227 ng/ul
RT: 14.498 min Scan# 1939
Delta R.T. 0.006 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42




Instrument :
BNA_P
ClientSampleId :
SSTD080648


Tgt Ion:153 Resp: 2154065
Ion Ratio Lower Upper
153 100
152 47.3 38.2 57.2
154 87.4 68.9 103.3



#53
2,4-Dinitrophenol
Concen: 100.804 ng/ul
RT: 14.575 min Scan# 1953
Delta R.T. 0.006 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42

Tgt Ion:184 Resp: 397110
Ion Ratio Lower Upper
184 100
63 61.1 43.6 65.4
154 70.0 52.1 78.1









#55
4-Nitrophenol
Concen: 105.098 ng/ul
RT: 14.704 min Scan# 1975
Delta R.T. 0.024 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42




Instrument :
BNA_P
ClientSampleId :
SSTD080648


Tgt Ion:109 Resp: 478136
Ion Ratio Lower Upper
109 100
139 94.0 73.2 109.8
65 103.6 90.9 136.3



#56
Dibenzofuran
Concen: 75.350 ng/ul
RT: 14.834 min Scan# 1997
Delta R.T. 0.006 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42

Tgt Ion:168 Resp: 3001362
Ion Ratio Lower Upper
168 100
139 37.0 30.3 45.5

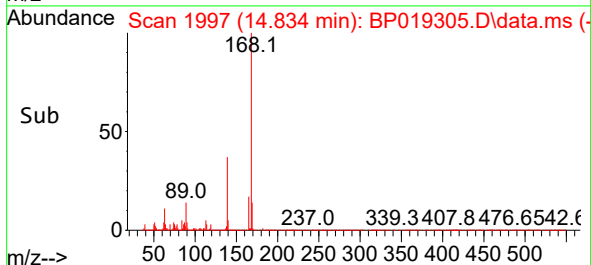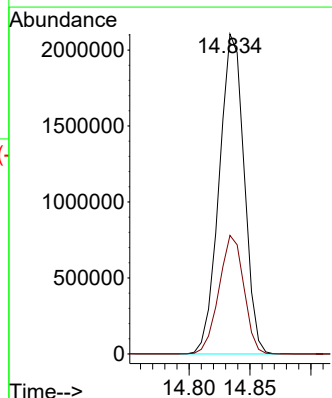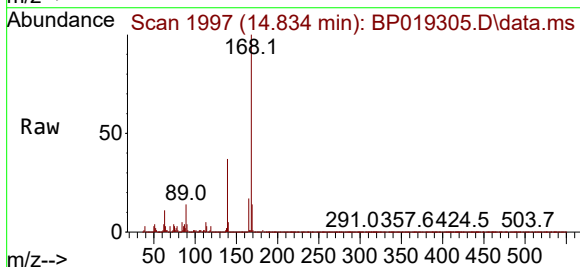



#57

2,4-Dinitrotoluene

Concen: 92.573 ng/ul

RT: 14.828 min Scan# 1994

Delta R.T. 0.012 min

Lab File: BP019305.D

Acq: 08 Jan 2024 20:42

Instrument :

BNA_P

ClientSampleId :

SSTD080648





Tgt Ion:165 Resp: 832507

Ion Ratio Lower Upper

165 100

63 50.5 41.3 61.9

182 2.9 2.4 3.6



#58

2,3,4,6-Tetrachlorophenol

Concen: 98.759 ng/ul

RT: 15.069 min Scan# 2037

Delta R.T. 0.006 min

Lab File: BP019305.D

Acq: 08 Jan 2024 20:42

Tgt Ion:232 Resp: 859211




Ion Ratio Lower Upper


232 100

131 33.2 27.9 41.9

130 2.0 1.8 2.8

166 25.4 20.9 31.3



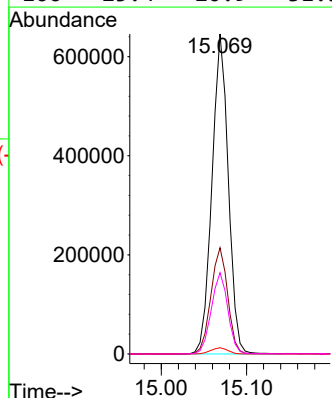





#59
Diethylphthalate
Concen: 80.615 ng/ul
RT: 15.269 min Scan# 2069
Delta R.T. 0.012 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42




Instrument :
BNA_P
ClientSampleId :
SSTD080648


Tgt Ion:149 Resp: 2601011
Ion Ratio Lower Upper
149 100
177 23.8 18.8 28.2
150 12.8 10.2 15.4



#61
Fluorene
Concen: 78.846 ng/ul
RT: 15.487 min Scan# 2108
Delta R.T. 0.006 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42

Tgt Ion:166 Resp: 2513748
Ion Ratio Lower Upper
166 100
165 97.9 78.6 118.0
167 13.7 10.6 15.8



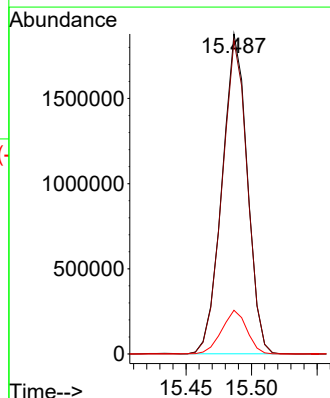
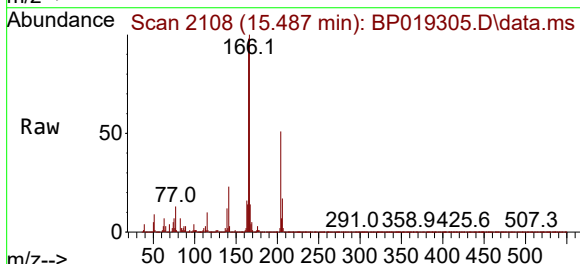




#62
4-Chlorophenyl-phenylether
Concen: 87.802 ng/ul
RT: 15.481 min Scan# 2106
Delta R.T. 0.006 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42




Instrument :
BNA_P
ClientSampleId :
SSTD080648


Tgt Ion:204 Resp: 1528698
Ion Ratio Lower Upper
204 100
206 33.1 27.0 40.4
141 49.1 41.5 62.3

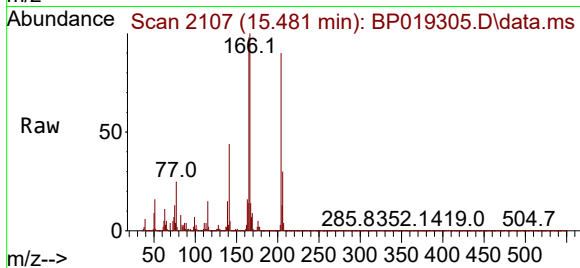

#63
4-Nitroaniline
Concen: 58.224 ng/ul
RT: 15.539 min Scan# 2117
Delta R.T. 0.018 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42

Tgt Ion:138 Resp: 350191
Ion Ratio Lower Upper
138 100
92 60.3 48.9 73.3
108 115.5 90.4 135.6









#66
4,6-Dinitro-2-methylphenol
Concen: 97.000 ng/ul
RT: 15.592 min Scan# 2126
Delta R.T. 0.018 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42




Instrument :
BNA_P
ClientSampleId :
SSTD080648


Tgt Ion:198 Resp: 603352
Ion Ratio Lower Upper
198 100
182 2.9 3.2 4.8#
77 22.6 20.6 30.8



#67
N-Nitrosodiphenylamine
Concen: 78.178 ng/ul
RT: 15.704 min Scan# 2145
Delta R.T. 0.006 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42

Tgt Ion:169 Resp: 2138137
Ion Ratio Lower Upper
169 100
168 67.4 54.8 82.2
167 37.1 29.3 43.9




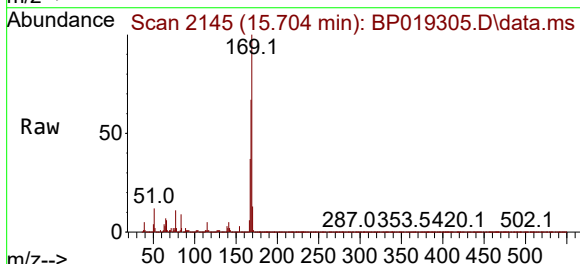




#68
4-Bromophenyl-phenylether
Concen: 92.015 ng/ul
RT: 16.375 min Scan# 21
Delta R.T. -0.000 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42




Instrument :
BNA_P
ClientSampleId :
SSTD080648


Tgt Ion:248 Resp: 1024875
Ion Ratio Lower Upper
248 100
250 97.6 75.6 113.4
141 61.6 48.7 73.1

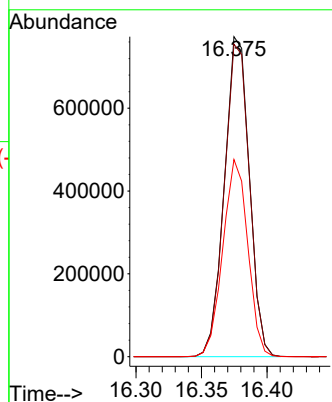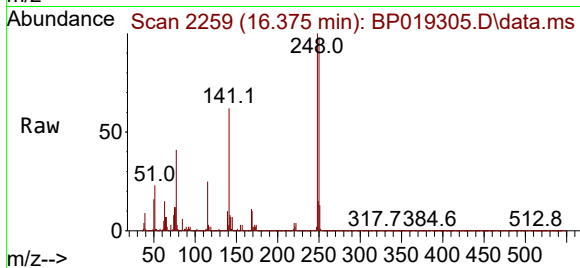

#69
Hexachlorobenzene
Concen: 86.834 ng/ul
RT: 16.492 min Scan# 2279
Delta R.T. 0.012 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42

Tgt Ion:284 Resp: 1181960
Ion Ratio Lower Upper
284 100
142 25.7 23.6 35.4
249 32.5 26.1 39.1





#70

Atrazine

Concen: 122.334 ng/ul

RT: 16.669 min Scan# 21

Delta R.T. 0.012 min

Lab File: BP019305.D

Acq: 08 Jan 2024 20:42

Instrument :

BNA_P

ClientSampleId :

SSTD080648





Tgt Ion:200 Resp: 944226

Ion Ratio Lower Upper

200 100

173 22.7 19.4 29.0

215 48.9 39.7 59.5

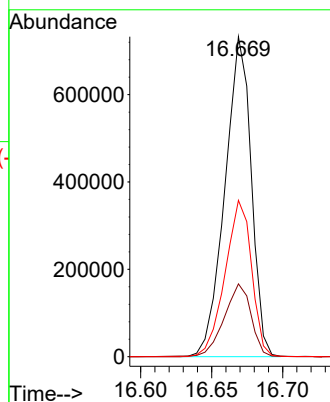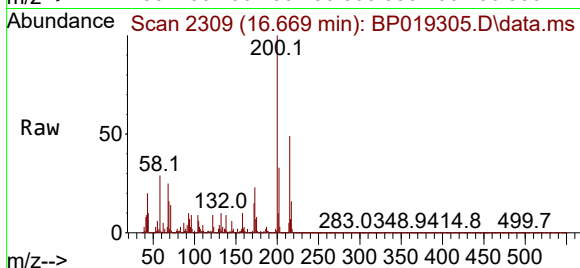

#71

Pentachlorophenol

Concen: 95.554 ng/ul

RT: 16.845 min Scan# 2339

Delta R.T. 0.006 min

Lab File: BP019305.D

Acq: 08 Jan 2024 20:42




Tgt Ion:266 Resp: 763634


Ion Ratio Lower Upper

266 100

264 62.7 49.4 74.2

268 63.4 51.6 77.4





#72

Phenanthrene

Concen: 77.712 ng/ul

RT: 17.233 min Scan# 2405

Delta R.T. 0.006 min

Lab File: BP019305.D

Acq: 08 Jan 2024 20:42

Instrument :

BNA_P

ClientSampleId :

SSTD080648





Tgt Ion:178 Resp: 4220283

Ion Ratio Lower Upper

178 100

179 15.5 12.1 18.1

176 19.7 15.4 23.2

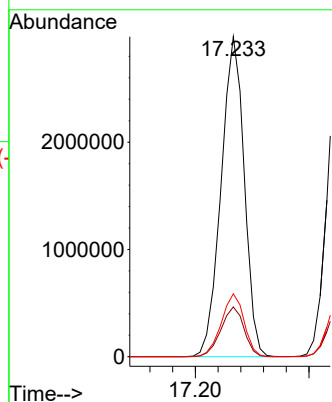

#74

Anthracene

Concen: 78.828 ng/ul

RT: 17.328 min Scan# 2421

Delta R.T. 0.012 min

Lab File: BP019305.D

Acq: 08 Jan 2024 20:42




Tgt Ion:178 Resp: 4261809


Ion Ratio Lower Upper

178 100

179 15.5 12.3 18.5

176 18.8 14.6 22.0

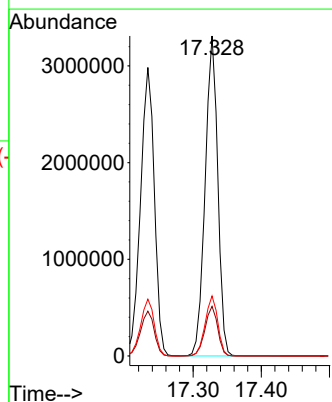



#75

1,2,3,4-Tetrachlorobenzene

Concen: 86.891 ng/uL

RT: 13.228 min Scan# 1723

Delta R.T. 0.006 min

Lab File: BP019305.D

Acq: 08 Jan 2024 20:42

Instrument :

BNA_P

ClientSampleId :

SSTD080648





Tgt Ion:216 Resp: 1353868

Ion Ratio Lower Upper

216 100

214 78.2 61.8 92.8

218 49.2 39.0 58.6

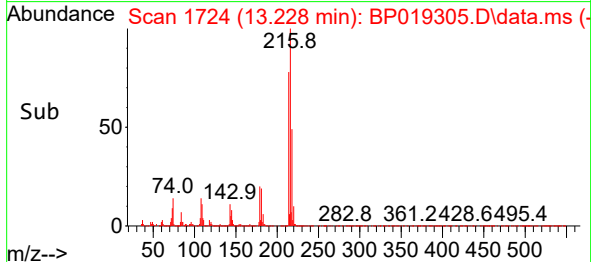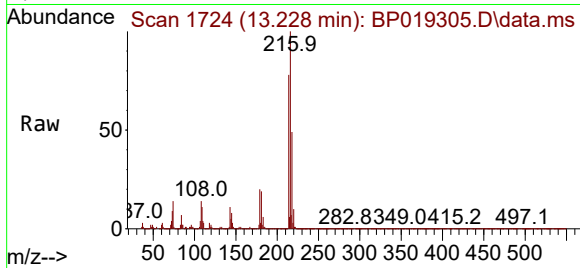

#76

Pentachlorobenzene

Concen: 84.457 ng/uL

RT: 14.751 min Scan# 1983

Delta R.T. 0.006 min

Lab File: BP019305.D

Acq: 08 Jan 2024 20:42




Tgt Ion:250 Resp: 1307643


Ion Ratio Lower Upper

250 100

248 62.9 50.8 76.2

252 63.4 50.2 75.4

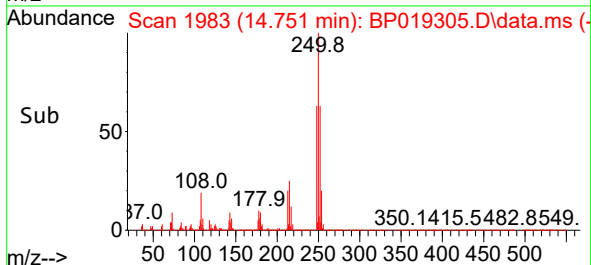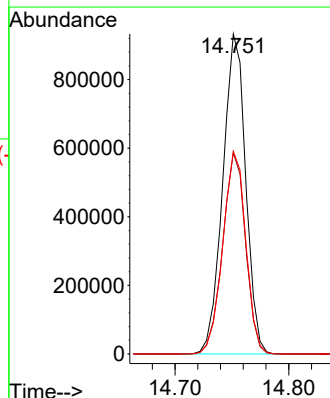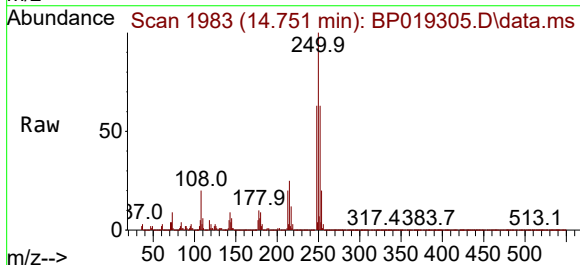



#77

Carbazole

Concen: 79.907 ng/ul

RT: 17.604 min Scan# 2468

Delta R.T. 0.006 min

Lab File: BP019305.D

Acq: 08 Jan 2024 20:42

Instrument :

BNA_P

ClientSampleId :

SSTD080648





Tgt Ion:167 Resp: 3593511

Ion Ratio Lower Upper

167 100

166 21.8 17.3 25.9

139 12.6 10.1 15.1



#78

Di-n-butylphthalate

Concen: 79.884 ng/ul

RT: 18.151 min Scan# 2561

Delta R.T. -0.000 min

Lab File: BP019305.D

Acq: 08 Jan 2024 20:42




Tgt Ion:149 Resp: 4455459


Ion Ratio Lower Upper

149 100

150 9.4 7.0 10.6

104 5.8 4.6 6.8




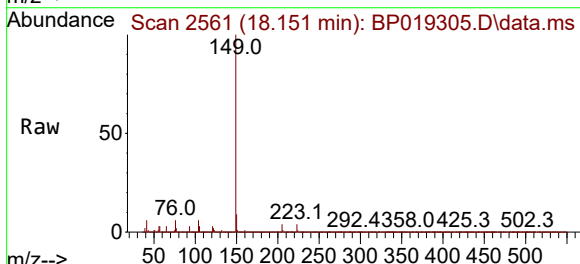




#80
Fluoranthene
Concen: 87.670 ng/u1
RT: 19.210 min Scan# 21
Delta R.T. 0.006 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42




Instrument :
BNA_P
ClientSampleId :
SSTD080648


Tgt Ion:202 Resp: 5451354
Ion Ratio Lower Upper
202 100
101 6.6 5.9 8.9
100 5.1 4.6 7.0

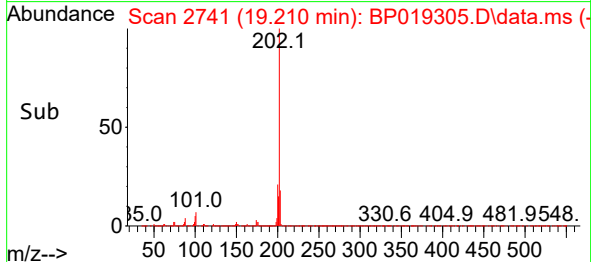

#82
Pyrene
Concen: 85.352 ng/u1
RT: 19.563 min Scan# 2801
Delta R.T. 0.006 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42

Tgt Ion:202 Resp: 5560467
Ion Ratio Lower Upper
202 100
101 8.0 7.2 10.8
100 6.6 5.8 8.6





#83

Butylbenzylphthalate

Concen: 86.745 ng/ul

RT: 20.439 min Scan# 2949

Delta R.T. 0.006 min

Lab File: BP019305.D

Acq: 08 Jan 2024 20:42

Instrument :

BNA_P

ClientSampleId :

SSTD080648





Tgt Ion:149 Resp: 2018640

Ion Ratio Lower Upper

149 100

91 69.6 61.7 92.5

206 27.1 18.6 27.8

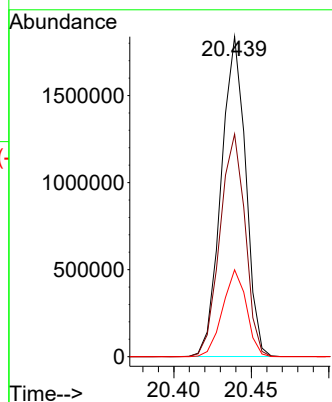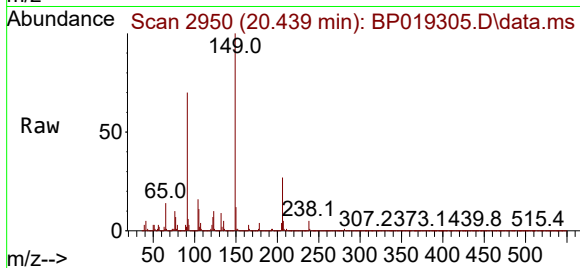

#84

3,3'-Dichlorobenzidine

Concen: 71.614 ng/ul

RT: 21.216 min Scan# 3082

Delta R.T. 0.006 min

Lab File: BP019305.D

Acq: 08 Jan 2024 20:42




Tgt Ion:252 Resp: 1592861


Ion Ratio Lower Upper

252 100

254 65.3 50.6 76.0

126 6.6 6.0 9.0









#85
Benzo(a)anthracene
Concen: 81.831 ng/ul
RT: 21.280 min Scan# 3093
Delta R.T. 0.012 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42




Instrument :
BNA_P
ClientSampleId :
SSTD080648


Tgt Ion:228 Resp: 5748646
Ion Ratio Lower Upper
228 100
229 19.9 15.8 23.6
226 27.6 21.6 32.4

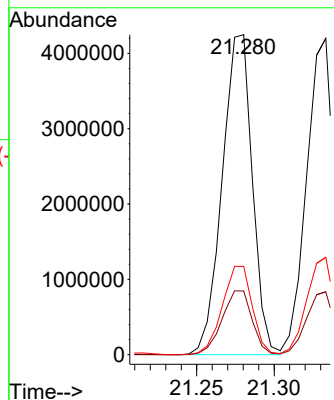

#86
Bis(2-ethylhexyl)phthalate
Concen: 84.983 ng/ul
RT: 21.198 min Scan# 3079
Delta R.T. -0.000 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42

Tgt Ion:149 Resp: 2912070
Ion Ratio Lower Upper
149 100
167 29.6 22.9 34.3
279 6.3 4.6 7.0

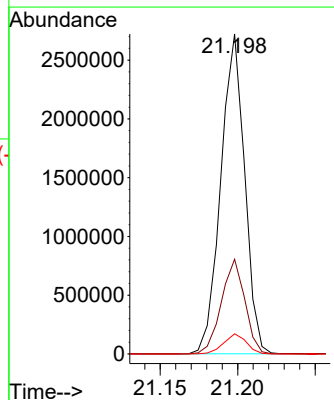



#87

Chrysene

Concen: 78.564 ng/ul

RT: 21.333 min Scan# 3100

Delta R.T. 0.012 min

Lab File: BP019305.D

Acq: 08 Jan 2024 20:42

Instrument :

BNA_P

ClientSampleId :

SSTD080648





Tgt Ion:228 Resp: 5146468

Ion Ratio Lower Upper

228 100

226 30.8 23.9 35.9

229 19.9 15.5 23.3



#89

Di-n-octyl phthalate

Concen: 103.368 ng/ul




RT: 22.104 min Scan# 3233


Delta R.T. -0.000 min

Lab File: BP019305.D

Acq: 08 Jan 2024 20:42

Tgt Ion:149 Resp: 4802067


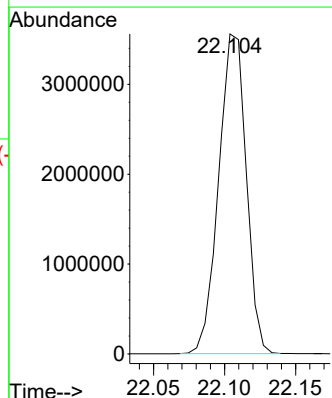






#90
Benzo(b)fluoranthene
Concen: 88.782 ng/ul
RT: 22.933 min Scan# 31
Delta R.T. 0.012 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42




Instrument :
BNA_P
ClientSampleId :
SSTD080648


Tgt Ion:252 Resp: 5066092
Ion Ratio Lower Upper
252 100
253 22.3 17.8 26.8
125 5.4 4.9 7.3



#91
Benzo(k)fluoranthene
Concen: 86.640 ng/ul
RT: 22.980 min Scan# 3382
Delta R.T. 0.012 min
Lab File: BP019305.D
Acq: 08 Jan 2024 20:42

Tgt Ion:252 Resp: 4857990
Ion Ratio Lower Upper
252 100
253 22.1 17.3 25.9
125 5.7 4.8 7.2

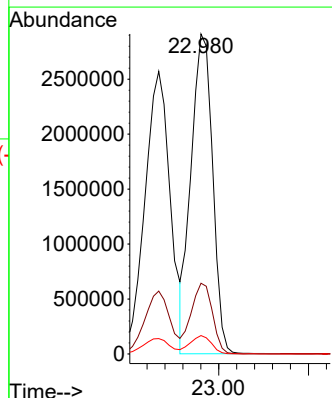



#93

Benzo(a)pyrene

Concen: 82.908 ng/ul

RT: 23.551 min Scan# 3477

Delta R.T. 0.012 min

Lab File: BP019305.D

Acq: 08 Jan 2024 20:42

Instrument :

BNA_P

ClientSampleId :

SSTD080648





Tgt Ion:252 Resp: 4452797

Ion Ratio Lower Upper

252 100

253 22.1 17.3 25.9

125 6.2 5.2 7.8



#94

Indeno(1,2,3-cd)pyrene

Concen: 69.976 ng/ul

RT: 26.109 min Scan# 3914

Delta R.T. 0.024 min

Lab File: BP019305.D

Acq: 08 Jan 2024 20:42




Tgt Ion:276 Resp: 4817788


Ion Ratio Lower Upper

276 100

138 14.7 12.2 18.4

277 25.3 19.9 29.9

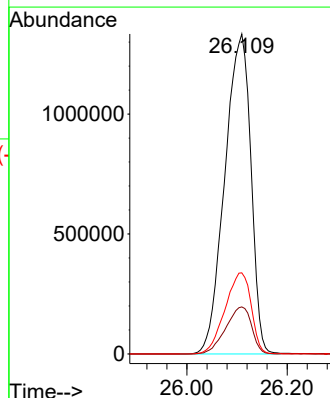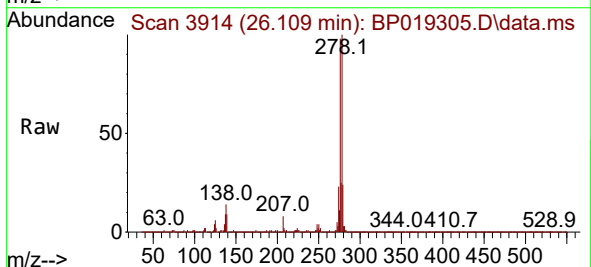




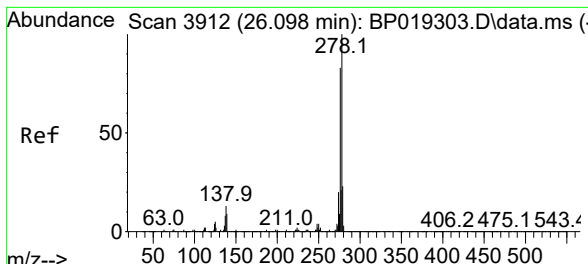


#95
 Dibenzo(a,h)anthracene
 Concen: 70.143 ng/ul
 RT: 26.121 min Scan# 3916
 Delta R.T. 0.023 min
 Lab File: BP019305.D
 Acq: 08 Jan 2024 20:42

Instrument :
 BNA_P
 ClientSampleId :
 SSTD080648

Tgt Ion:278 Resp: 4017436

Ion	Ratio	Lower	Upper
278	100		
139	9.0	7.4	11.2
279	23.6	18.7	28.1

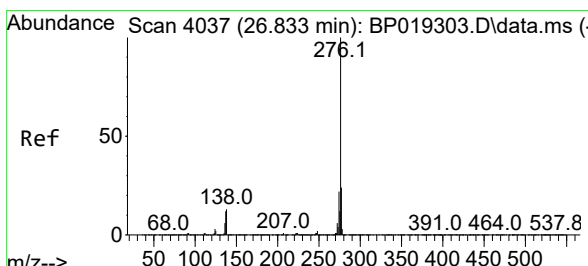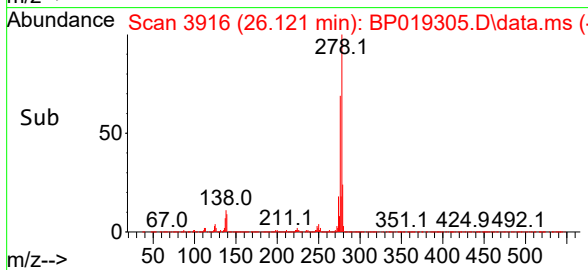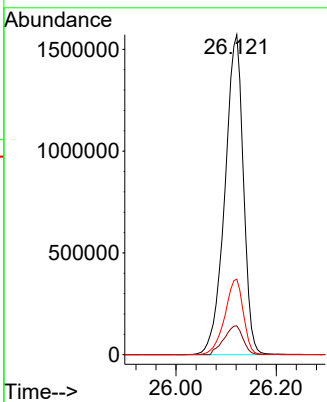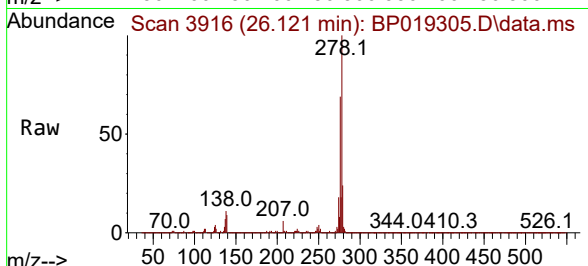

#96
 Benzo(g,h,i)perylene
 Concen: 67.556 ng/ul
 RT: 26.857 min Scan# 4041
 Delta R.T. 0.024 min
 Lab File: BP019305.D
 Acq: 08 Jan 2024 20:42

Tgt Ion:276 Resp: 3727305

Ion	Ratio	Lower	Upper
276	100		
138	12.2	10.7	16.1
277	23.7	19.2	28.8

