

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010924\
 Data File : BP019310.D
 Acq On : 09 Jan 2024 11:29
 Operator : MA/JU
 Sample : PB158300BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK300

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019310.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	19	22	28	rVB	36144	47462	1.30%	0.130%
2	3.640	90	94	114	rBV	457438	710362	19.47%	1.947%
3	3.958	145	148	156	rVB2	8322	13465	0.37%	0.037%
4	6.969	654	660	673	rVB	533012	847933	23.24%	2.324%
5	7.122	679	686	698	rVB	442408	674740	18.49%	1.849%
6	7.317	712	719	730	rBV	522026	821169	22.50%	2.251%
7	7.781	791	798	806	rBV	496162	764797	20.96%	2.096%
8	8.511	911	922	939	rBV	658503	1077742	29.53%	2.954%
9	8.946	989	996	1011	rBV	521811	870250	23.85%	2.385%
10	9.669	1111	1119	1132	rBV	464993	760882	20.85%	2.085%
11	10.210	1202	1211	1226	rBV	650140	1148835	31.48%	3.149%
12	10.575	1265	1273	1281	rBV	669487	1109192	30.40%	3.040%
13	10.728	1292	1299	1318	rBV	632263	1138060	31.19%	3.119%
14	12.181	1538	1546	1560	rVB3	9842	25024	0.69%	0.069%
15	12.399	1578	1583	1588	rVB9	1809	3727	0.10%	0.010%
16	12.787	1641	1649	1653	rBV9	3066	7341	0.20%	0.020%
17	13.322	1734	1740	1747	rVB5	9522	16466	0.45%	0.045%
18	13.704	1798	1805	1809	rBV8	3509	7338	0.20%	0.020%
19	13.846	1823	1829	1839	rBV	1326693	1876347	51.42%	5.143%
20	14.116	1868	1875	1885	rBV	1353926	2053555	56.28%	5.628%
21	14.428	1921	1928	1935	rBV	1115862	1625778	44.55%	4.456%
22	14.663	1961	1968	1990	rBV	482866	847071	23.21%	2.322%
23	15.422	2089	2097	2107	rBV	1849992	2693496	73.81%	7.382%
24	15.563	2114	2121	2134	rBV	572269	842427	23.09%	2.309%
25	15.663	2134	2138	2143	rVB3	8632	14262	0.39%	0.039%
26	16.210	2226	2231	2236	rBV7	7200	13168	0.36%	0.036%
27	16.857	2336	2341	2345	rBV8	5326	9089	0.25%	0.025%
28	16.969	2357	2360	2365	rBV6	4719	7354	0.20%	0.020%
29	17.181	2389	2396	2406	rBV	1553705	2147742	58.86%	5.887%
30	17.281	2406	2413	2427	rVV2	2134006	3066748	84.04%	8.405%
31	17.592	2460	2466	2469	rBV8	2596	5498	0.15%	0.015%
32	18.081	2545	2549	2553	rBV5	11680	18803	0.52%	0.052%
33	19.104	2719	2723	2728	rBV2	31059	41992	1.15%	0.115%
34	19.175	2731	2735	2739	rVV	25504	31601	0.87%	0.087%
35	19.528	2789	2795	2804	rBV	2855450	3649114	100.00%	10.002%
36	21.286	3089	3094	3100	rBV	1825890	2294448	62.88%	6.289%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010924\
Data File : BP019310.D
Acq On : 09 Jan 2024 11:29
Operator : MA/JU
Sample : PB158300BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK300

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Title : SVOA CALIBRATION

37	23.486	3462	3468	3479	rVB	1657561	3150262	86.33%	8.634%
38	23.639	3488	3494	3503	rVB	1047627	2051834	56.23%	5.624%




Sum of corrected areas: 36485374

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010924\
Data File : BP019310.D
Acq On : 09 Jan 2024 11:29
Operator : MA/JU
Sample : PB158300BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK300

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

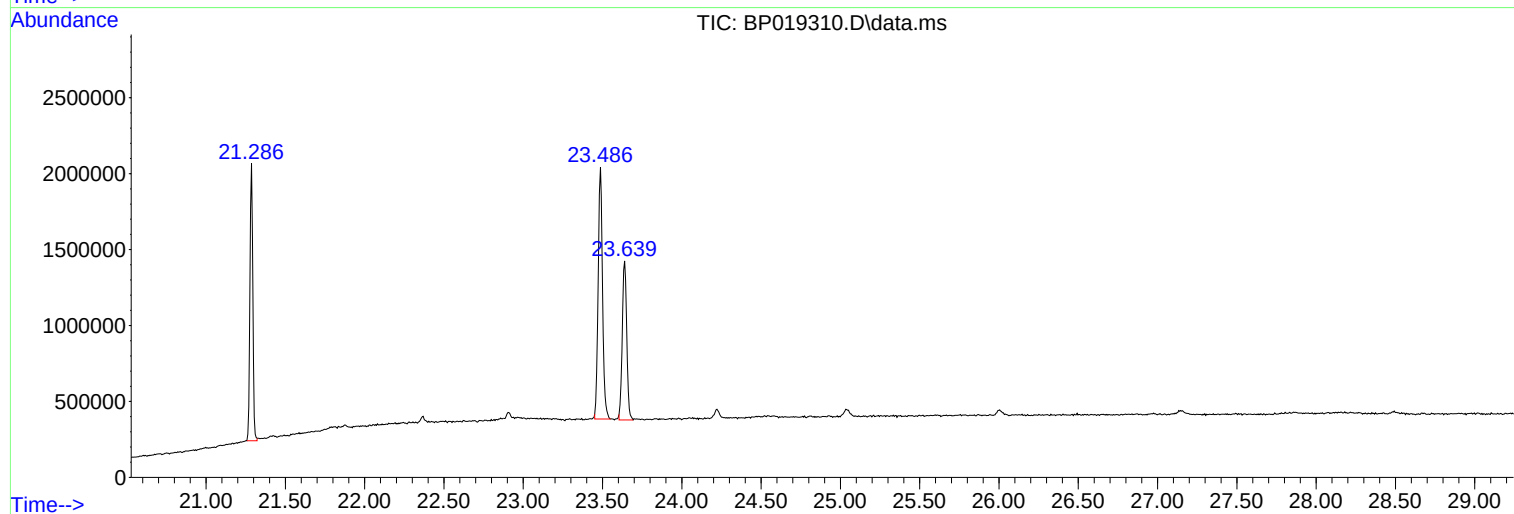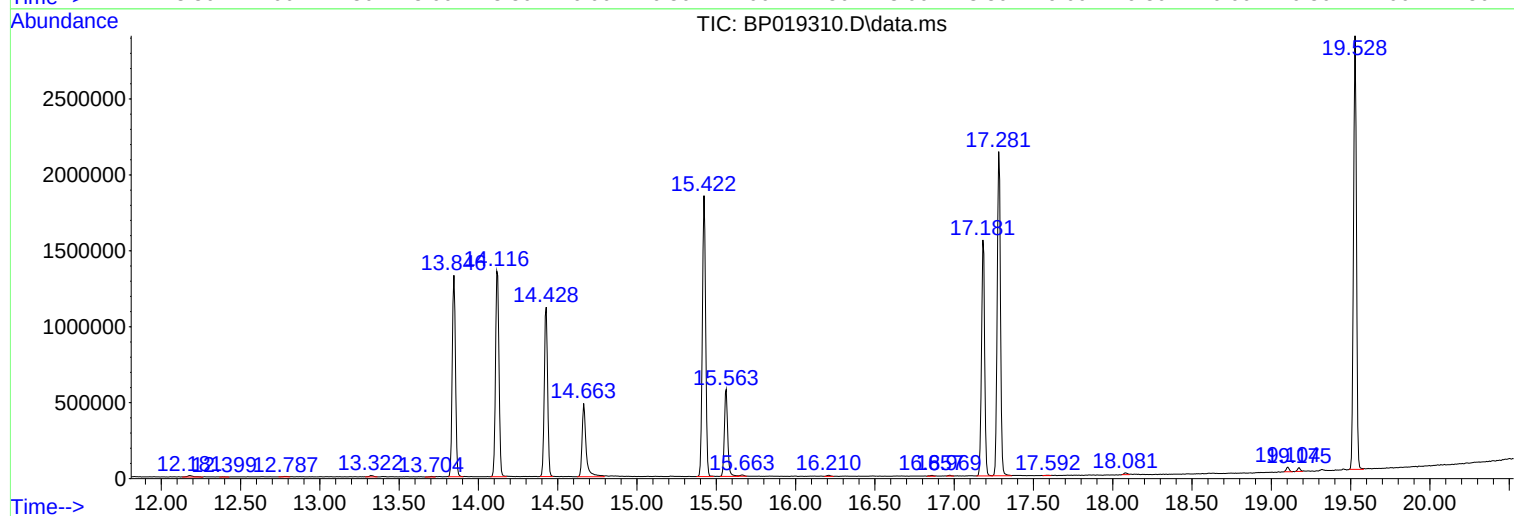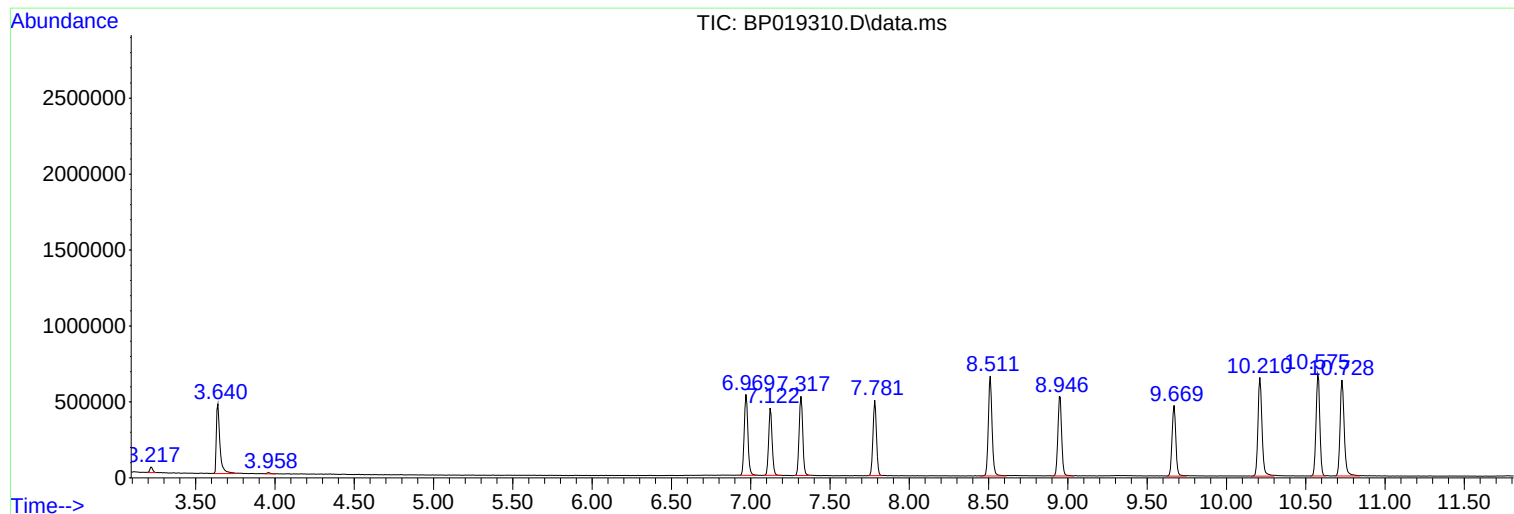

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010924\
Data File : BP019310.D
Acq On : 09 Jan 2024 11:29
Operator : MA/JU
Sample : PB158300BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK300

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010924\
Data File : BP019310.D
Acq On : 09 Jan 2024 11:29
Operator : MA/JU
Sample : PB158300BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK300

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc