

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010924\
 Data File : BP019316.D
 Acq On : 09 Jan 2024 14:55
 Operator : MA/JU
 Sample : 05953-07MEDL 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCFA9MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019316.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.664	94	98	106	rBV4	9069	16482	0.62%	0.104%
2	3.958	144	148	152	rVB2	8355	12051	0.45%	0.076%
3	4.417	224	226	230	rVB2	2911	2921	0.11%	0.018%
4	5.252	365	368	373	rBV6	2179	3150	0.12%	0.020%
5	6.764	623	625	629	rVB5	2348	2983	0.11%	0.019%
6	6.905	647	649	655	rVB7	2518	3087	0.12%	0.020%
7	6.975	655	661	672	rVB	33093	63850	2.39%	0.404%
8	7.122	681	686	694	rVB	28427	46628	1.74%	0.295%
9	7.317	714	719	730	rVB	33574	58370	2.18%	0.369%
10	7.781	788	798	808	rBV	504606	789971	29.56%	4.998%
11	8.022	835	839	842	rVB6	1876	2890	0.11%	0.018%
12	8.516	918	923	935	rBV2	38707	77392	2.90%	0.490%
13	8.628	938	942	946	rVB6	2686	5282	0.20%	0.033%
14	8.952	989	997	1007	rBV2	32749	65222	2.44%	0.413%
15	9.311	1055	1058	1061	rBV5	2022	3220	0.12%	0.020%
16	9.675	1113	1120	1127	rBV2	26014	49610	1.86%	0.314%
17	10.228	1204	1214	1224	rBV3	31746	81726	3.06%	0.517%
18	10.575	1263	1273	1285	rBV	672775	1132892	42.39%	7.167%
19	10.746	1292	1302	1314	rBV4	17928	51648	1.93%	0.327%
20	12.775	1644	1647	1648	rBV3	3141	3041	0.11%	0.019%
21	13.328	1735	1741	1747	rBV	15085	24267	0.91%	0.154%
22	13.687	1797	1802	1807	rBV8	11242	20232	0.76%	0.128%
23	13.846	1823	1829	1835	rBV	95094	148718	5.56%	0.941%
24	13.904	1835	1839	1842	rVB5	5544	8005	0.30%	0.051%
25	14.122	1870	1876	1884	rBV	101555	156290	5.85%	0.989%
26	14.246	1894	1897	1899	rBV4	3476	3985	0.15%	0.025%
27	14.310	1905	1908	1914	rVB8	4642	8445	0.32%	0.053%
28	14.363	1914	1917	1918	rBV3	2327	2747	0.10%	0.017%
29	14.428	1921	1928	1940	rVV	1185180	1779451	66.58%	11.258%
30	14.687	1963	1972	1981	rBV4	16556	52488	1.96%	0.332%
31	14.940	2012	2015	2018	rVB4	5962	6453	0.24%	0.041%
32	15.069	2033	2037	2044	rVB2	21906	34712	1.30%	0.220%
33	15.128	2044	2047	2050	rBV5	4108	5188	0.19%	0.033%
34	15.251	2066	2068	2073	rBV6	3107	5177	0.19%	0.033%
35	15.422	2092	2097	2106	rBV	151903	229520	8.59%	1.452%
36	15.534	2111	2116	2119	rVV	54716	77689	2.91%	0.491%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010924\
 Data File : BP019316.D
 Acq On : 09 Jan 2024 14:55
 Operator : MA/JU
 Sample : 05953-07MEDL 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GCFA9MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

37	15.563	2119	2121	2127	rVB2	30925	41954	1.57%	0.265%
38	15.681	2137	2141	2152	rVB2	24248	51534	1.93%	0.326%
39	16.016	2194	2198	2203	rBV8	7588	12229	0.46%	0.077%
40	16.163	2216	2223	2228	rBV2	77676	124536	4.66%	0.788%
41	16.257	2237	2239	2242	rBV3	6098	7706	0.29%	0.049%
42	16.834	2332	2337	2353	rBV	1557097	2213498	82.83%	14.004%
43	16.987	2358	2363	2373	rVB	95910	164056	6.14%	1.038%
44	17.181	2390	2396	2405	rBV	1722168	2382690	89.16%	15.074%
45	17.281	2408	2413	2419	rBV	181596	265016	9.92%	1.677%
46	17.598	2463	2467	2471	rBV	32260	46373	1.74%	0.293%
47	17.798	2498	2501	2505	rVB4	37958	43116	1.61%	0.273%
48	18.075	2544	2548	2554	rBV2	62486	98276	3.68%	0.622%
49	19.528	2790	2795	2799	rBV	271979	360658	13.50%	2.282%
50	21.286	3089	3094	3103	rBV	2172835	2672474	100.00%	16.907%
51	23.645	3488	3495	3504	rVB	1181569	2286837	85.57%	14.467%




Sum of corrected areas: 15806736

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010924\
Data File : BP019316.D
Acq On : 09 Jan 2024 14:55
Operator : MA/JU
Sample : 05953-07MEDL 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCFA9MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

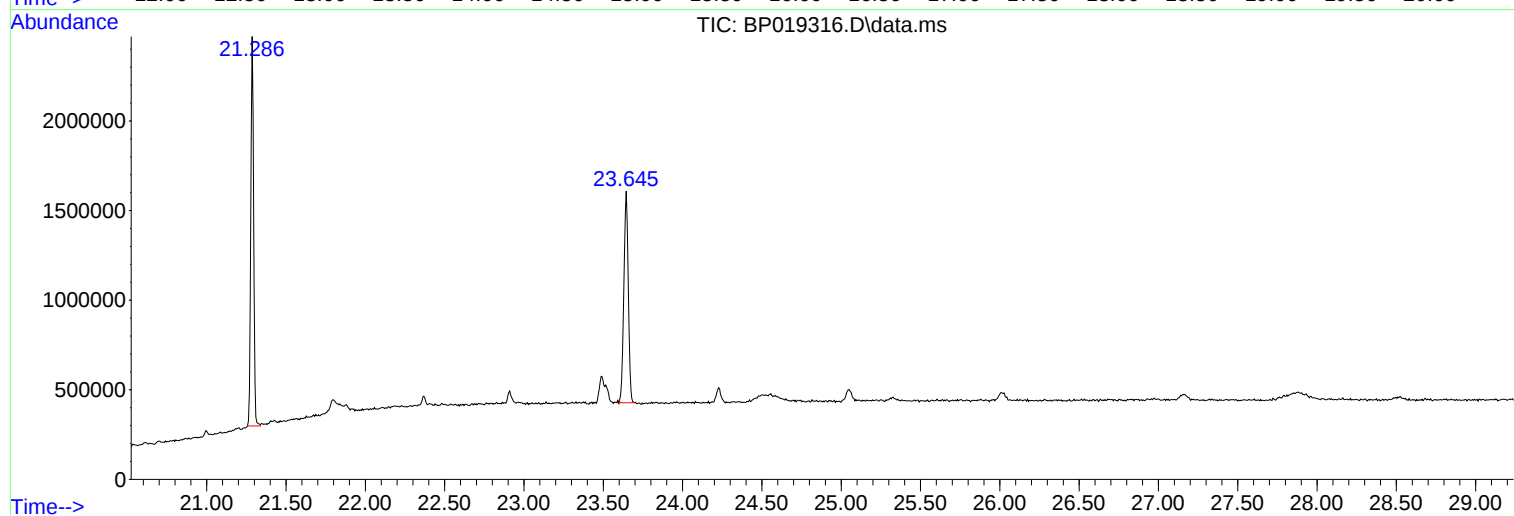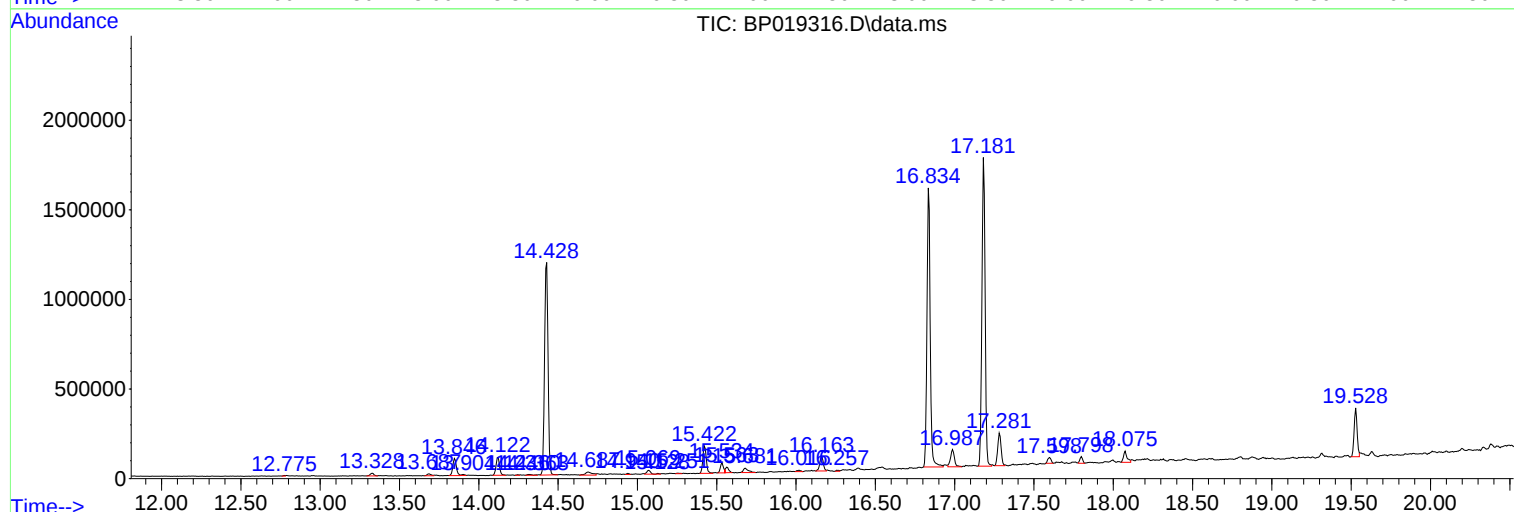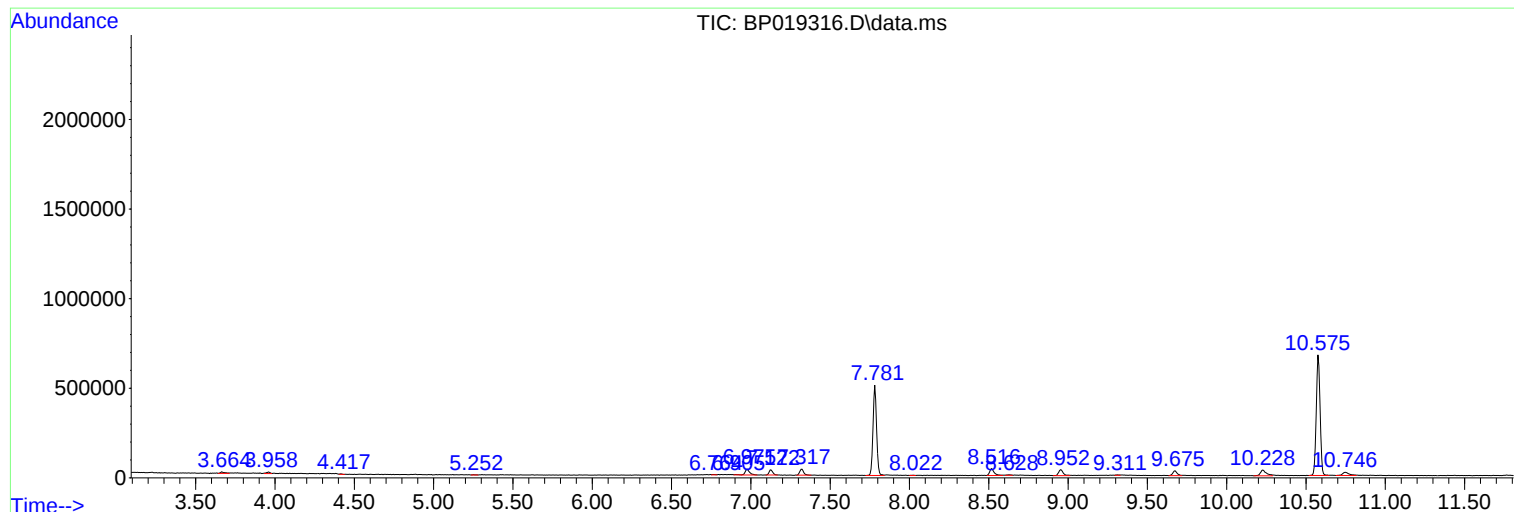

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010924\
Data File : BP019316.D
Acq On : 09 Jan 2024 14:55
Operator : MA/JU
Sample : 05953-07MEDL 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCFA9MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP010924\
Data File : BP019316.D
Acq On : 09 Jan 2024 14:55
Operator : MA/JU
Sample : 05953-07MEDL 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GCFA9MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc