

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011322\
 Data File : BP008787.D
 Acq On : 13 Jan 2022 11:37
 Operator : CG/JU
 Sample : PB141983BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB141983BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008787.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.064	9	13	27	rVB	226614	334243	1.42%	0.361%
2	5.452	412	419	440	rBV	5404134	8214366	34.84%	8.873%
3	7.046	682	690	709	rBV	4825124	8138160	34.52%	8.790%
4	7.863	822	829	838	rBV	1157413	1871357	7.94%	2.021%
5	9.022	1016	1026	1047	rBV	3102823	5392094	22.87%	5.824%
6	10.663	1296	1305	1319	rBV	1355527	2522228	10.70%	2.724%
7	13.128	1716	1724	1746	rBV	9336981	14043589	59.57%	15.169%
8	14.504	1951	1958	1975	rBV	2313148	3602046	15.28%	3.891%
9	15.998	2204	2212	2242	rBV	6771957	11211595	47.56%	12.110%
10	17.257	2419	2426	2440	rBV	3071276	4614760	19.57%	4.985%
11	19.821	2855	2862	2875	rBV	18205709	23574966	100.00%	25.464%
12	21.345	3116	3121	3131	rBV	3710802	4854676	20.59%	5.244%
13	23.774	3527	3534	3548	rVB2	1930400	4206265	17.84%	4.543%


Sum of corrected areas: 92580345

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011322\
Data File : BP008787.D
Acq On : 13 Jan 2022 11:37
Operator : CG/JU
Sample : PB141983BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141983BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

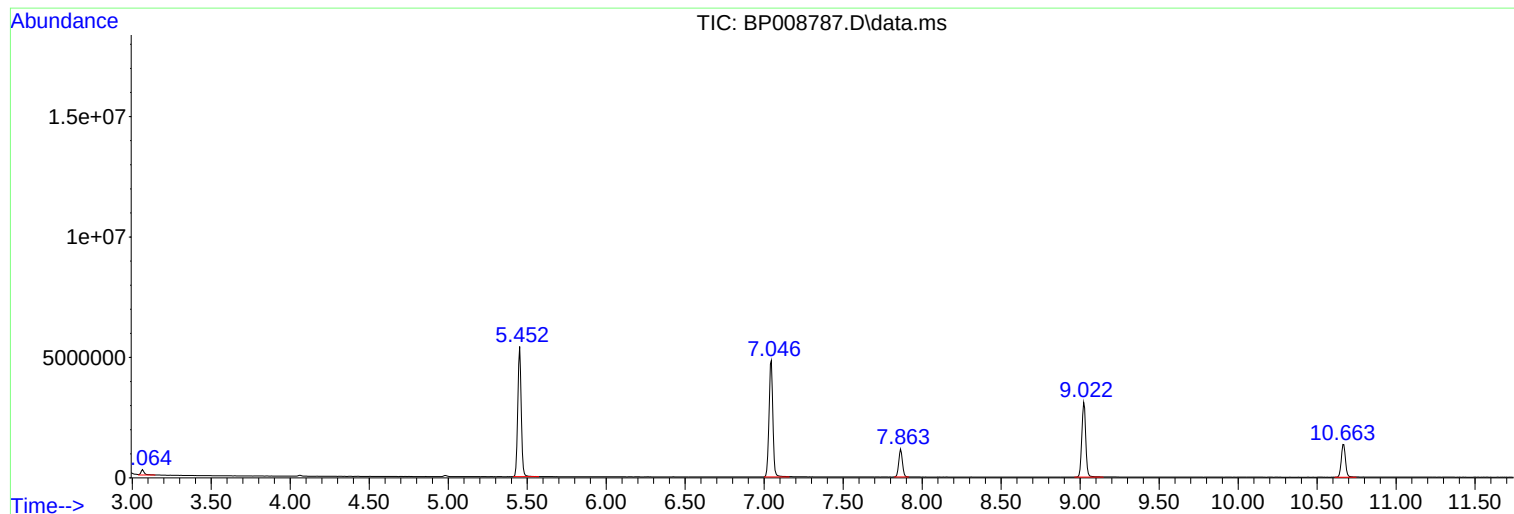

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011322\
Data File : BP008787.D
Acq On : 13 Jan 2022 11:37
Operator : CG/JU
Sample : PB141983BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141983BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.064	3.57 ng	334243	1,4-Dichlorobenzene-d4	7.863

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	86
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	37
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	16

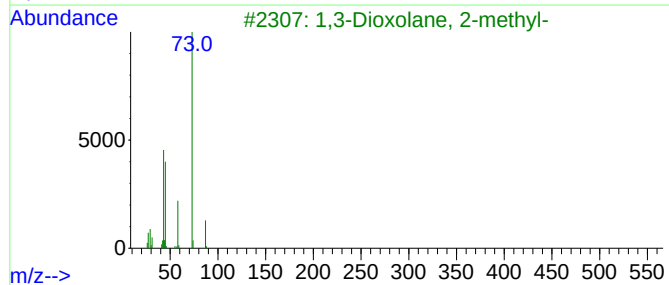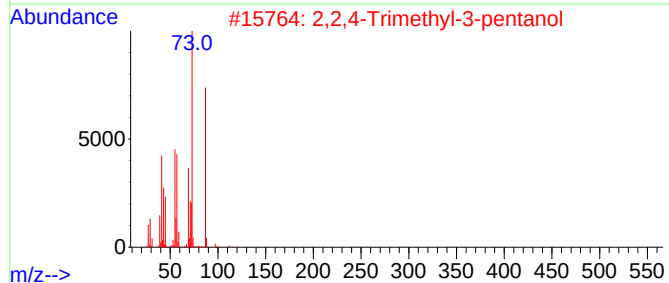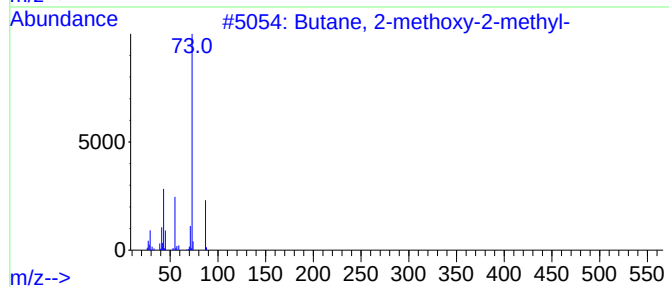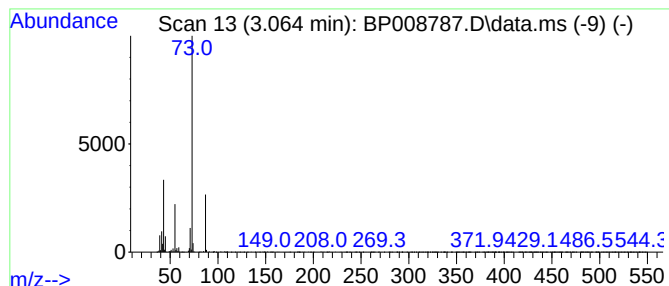

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011322\
Data File : BP008787.D
Acq On : 13 Jan 2022 11:37
Operator : CG/JU
Sample : PB141983BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141983BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.064	3.6	ng	334243	1	7.863	1871360	20.0