
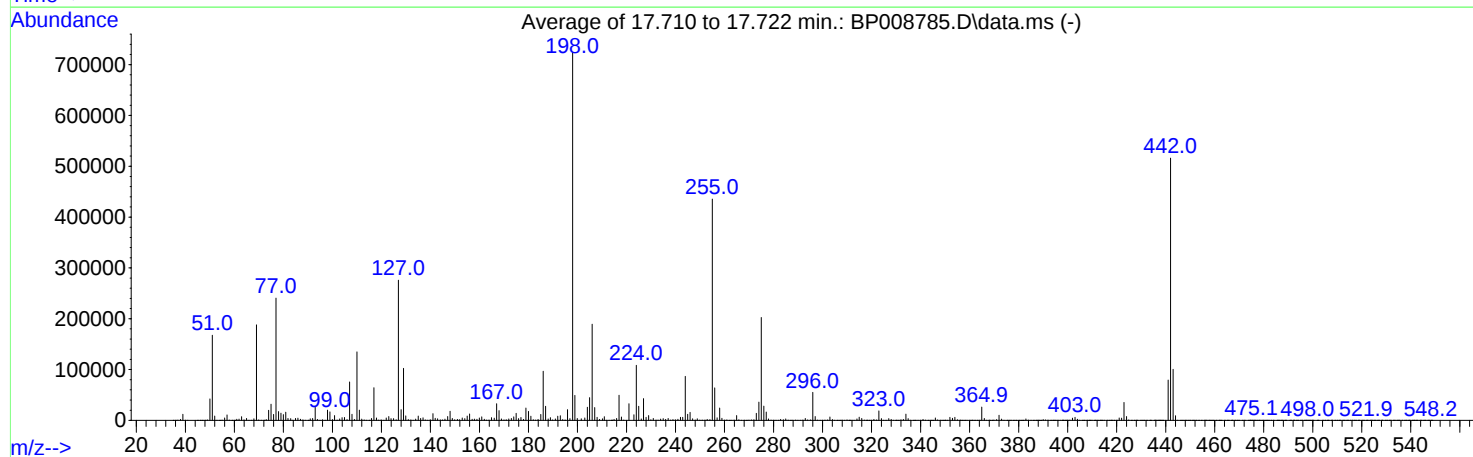


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011322\
 Data File : BP008785.D
 Acq On : 13 Jan 2022 10:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 12 00:18:56 2022

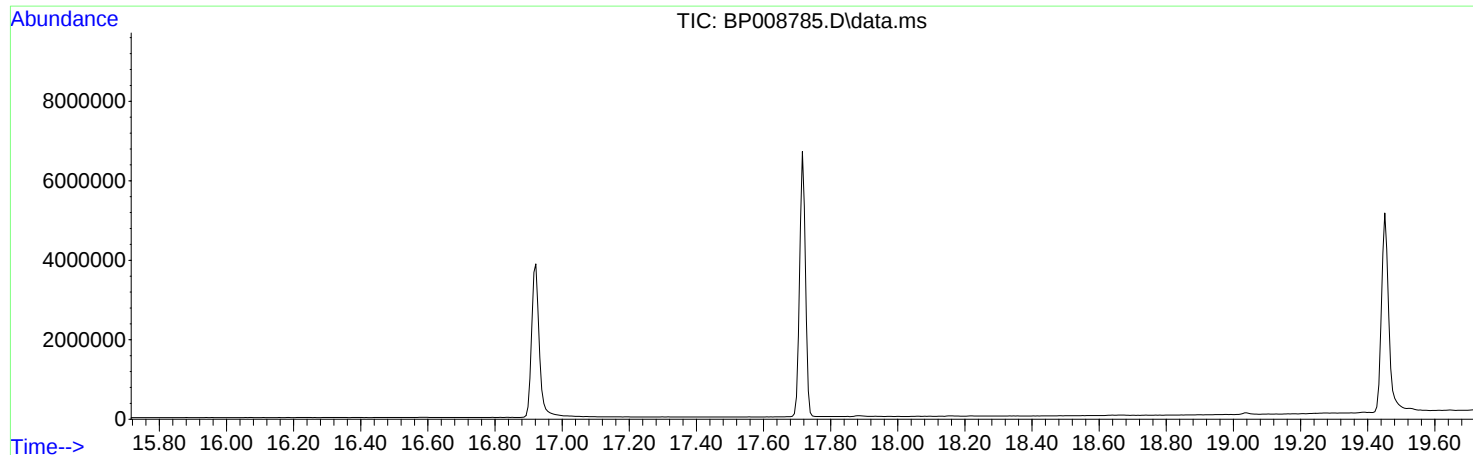




AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.1	167572	PASS
68	69	0.00	2	1.7	3123	PASS
69	198	0.00	100	26.0	187961	PASS
70	69	0.00	2	0.5	1004	PASS
127	198	10	80	38.1	275828	PASS
197	198	0.00	2	0.5	3483	PASS
198	198	100	100	100.0	723882	PASS
199	198	5	9	6.8	49005	PASS
275	198	10	60	28.0	202603	PASS
365	198	1	100	3.6	26080	PASS
441	198	0.01	100	11.0	79271	PASS
442	442	100	100	100.0	515989	PASS
443	442	15	24	19.5	100528	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011322\
 Data File : BP008785.D
 Acq On : 13 Jan 2022 10:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jan 14 01:00:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 12 00:18:56 2022
 Response via : Initial Calibration

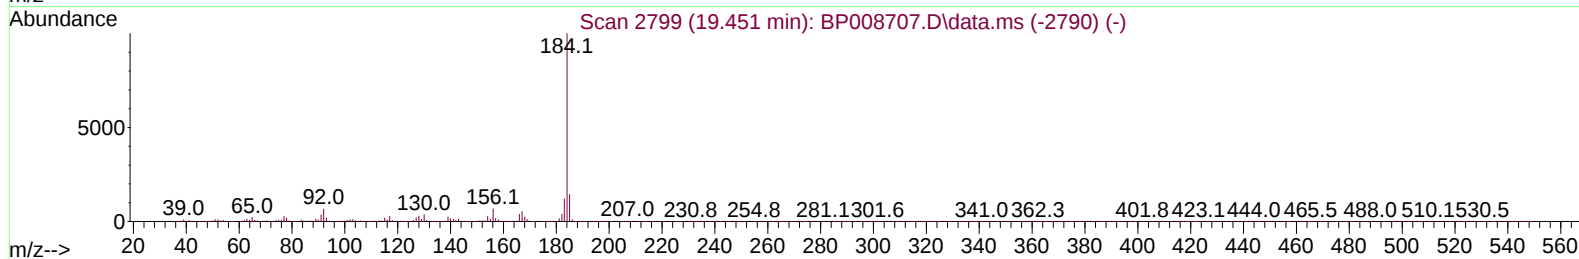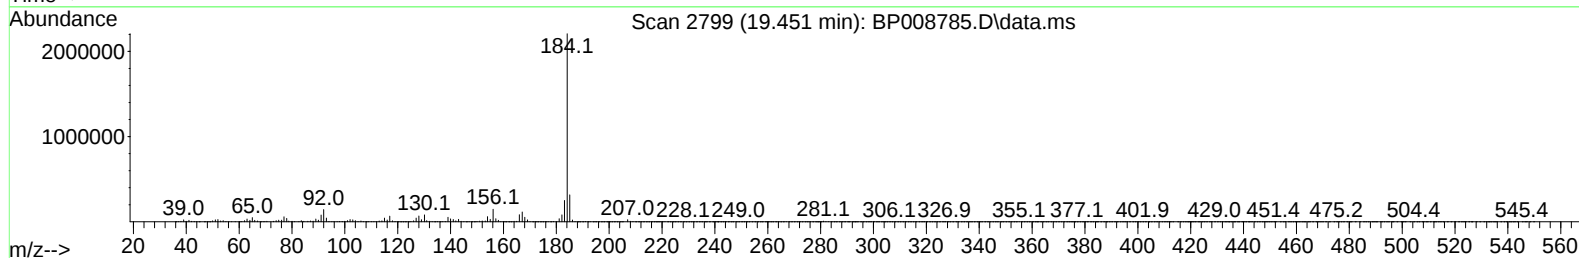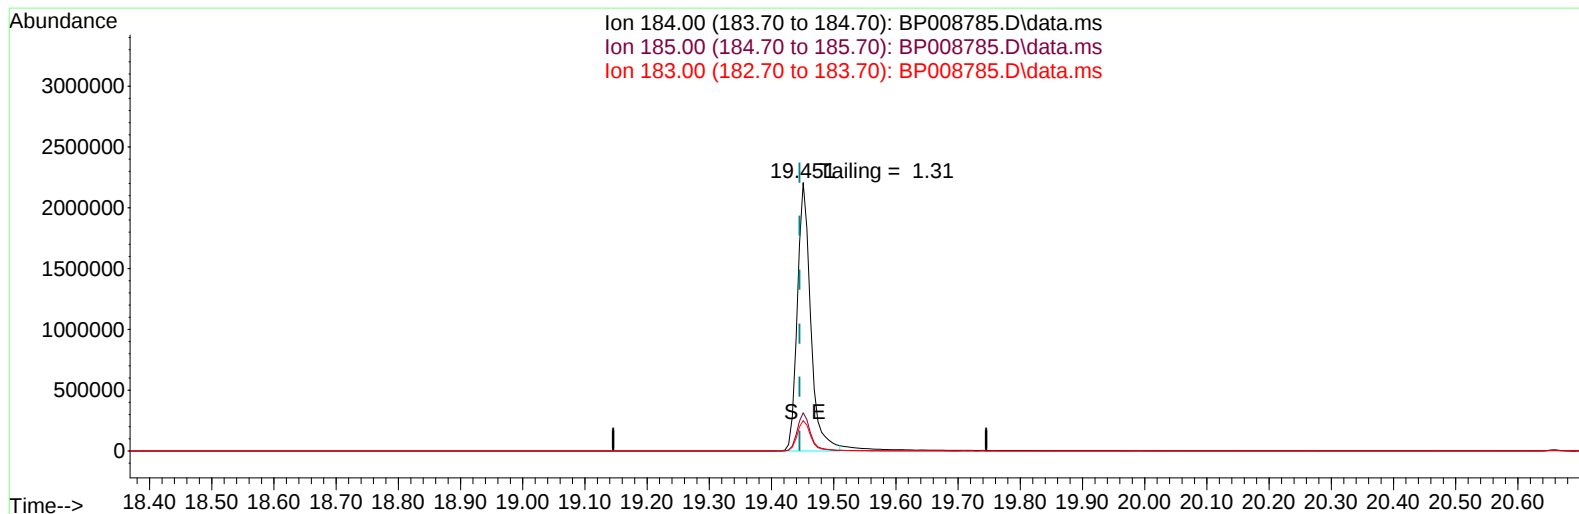

TIC: BP008785.D\data.ms

(77) Benzidine

19.451min (+ 0.006) 211021.07 ng




response 3449198

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.26
183.00	11.90	11.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011322\
Data File : BP008785.D
Acq On : 13 Jan 2022 10:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 14 01:00:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP010622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 12 00:18:56 2022
Response via : Initial Calibration

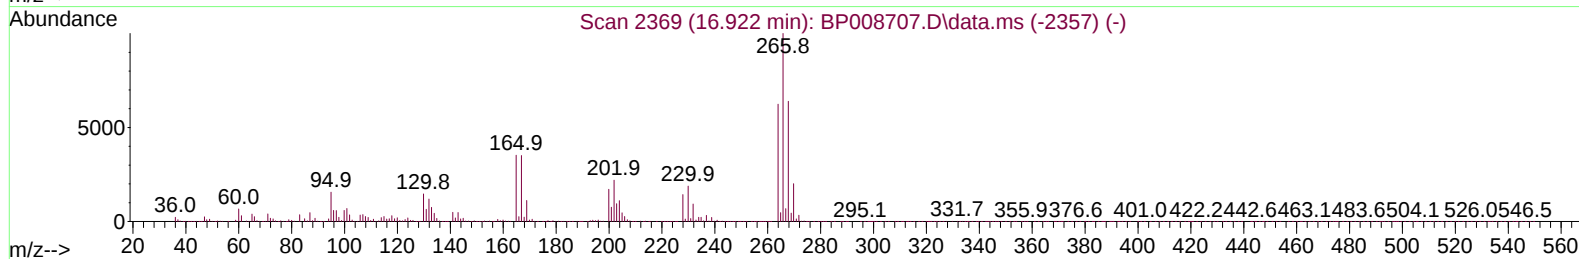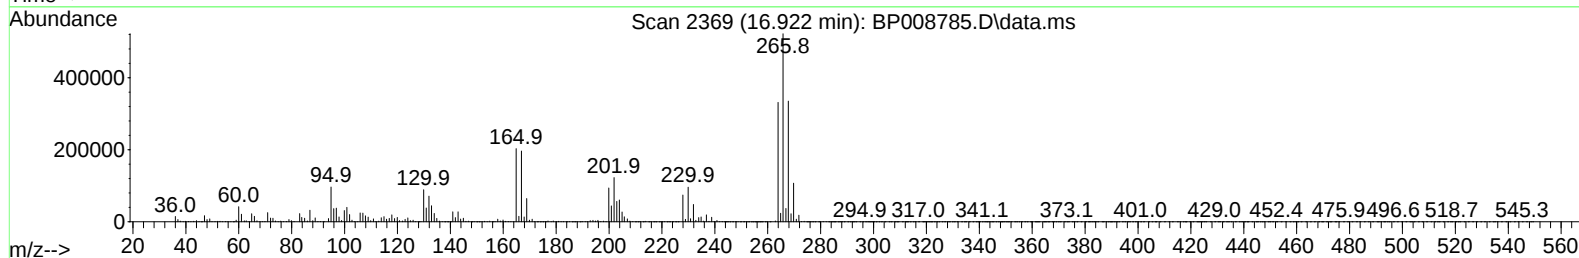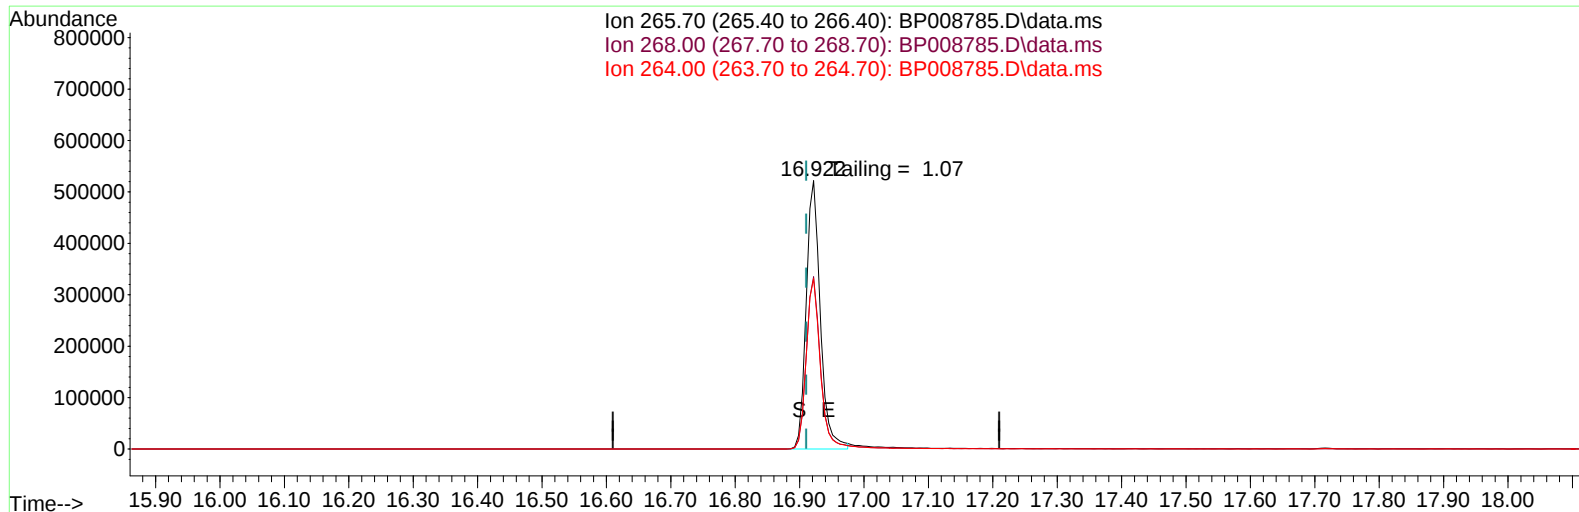

TIC: BP008785.D\data.ms

(70) Pentachlorophenol (C)

16.922min (+ 0.012) 2285960.37 ng

response 825090

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.19
264.00	62.90	63.47
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/13/2022	BNA_P	<u>BP008785.D</u>
Compound Name	Response	Retention Time
DDT	2330153	20.657
DDD	63647	20.227
DDE	3509	19.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
67156	2397309	2.80

Instrument :
BNA_P
ClientSampleId :
DFTPP