

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP011420\
 Data File : BP001592.D
 Acq On : 14 Jan 2020 17:51
 Operator : JU
 Sample : PB126085BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB126085BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.876	10	15	24	rBV	58698	113630	4.00%	0.782%
2	2.952	24	28	49	rVB	721074	989660	34.87%	6.812%
3	4.805	338	343	357	rVB	76890	112201	3.95%	0.772%
4	5.264	415	421	433	rBV	311633	472548	16.65%	3.253%
5	6.828	681	687	698	rBV	186331	304254	10.72%	2.094%
6	7.181	739	747	761	rBV	570993	945906	33.33%	6.511%
7	7.634	818	824	833	rBV	129267	210035	7.40%	1.446%
8	7.958	871	879	889	rVB	562985	912305	32.15%	6.280%
9	8.787	1011	1020	1036	rBV	459446	802129	28.26%	5.521%
10	10.410	1289	1296	1314	rVB	140296	248231	8.75%	1.709%
11	12.904	1712	1720	1732	rBV	1102353	1615854	56.94%	11.123%
12	14.287	1947	1955	1968	rBV	226460	347519	12.24%	2.392%
13	15.787	2203	2210	2230	rBV	955664	1379291	48.60%	9.494%
14	17.045	2418	2424	2438	rBV	299835	435022	15.33%	2.994%
15	19.639	2859	2865	2880	rBV	2360098	2838050	100.00%	19.535%
16	20.910	3077	3081	3085	rBV	60198	71464	2.52%	0.492%
17	21.151	3117	3122	3132	rBV	340869	480066	16.92%	3.304%
18	21.339	3150	3154	3162	rBV	183010	206324	7.27%	1.420%
19	21.775	3224	3228	3237	rBV	290717	369937	13.03%	2.546%
20	22.245	3303	3308	3316	rBV	330715	460095	16.21%	3.167%
21	22.763	3391	3396	3405	rVB	251191	389443	13.72%	2.681%
22	23.345	3489	3495	3498	rBV	160824	279144	9.84%	1.921%
23	23.386	3498	3502	3511	rVB	209900	383689	13.52%	2.641%
24	24.004	3602	3607	3614	rVB	87943	160896	5.67%	1.108%


Sum of corrected areas: 14527693

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP011420\
Data File : BP001592.D
Acq On : 14 Jan 2020 17:51
Operator : JU
Sample : PB126085BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB126085BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP010820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

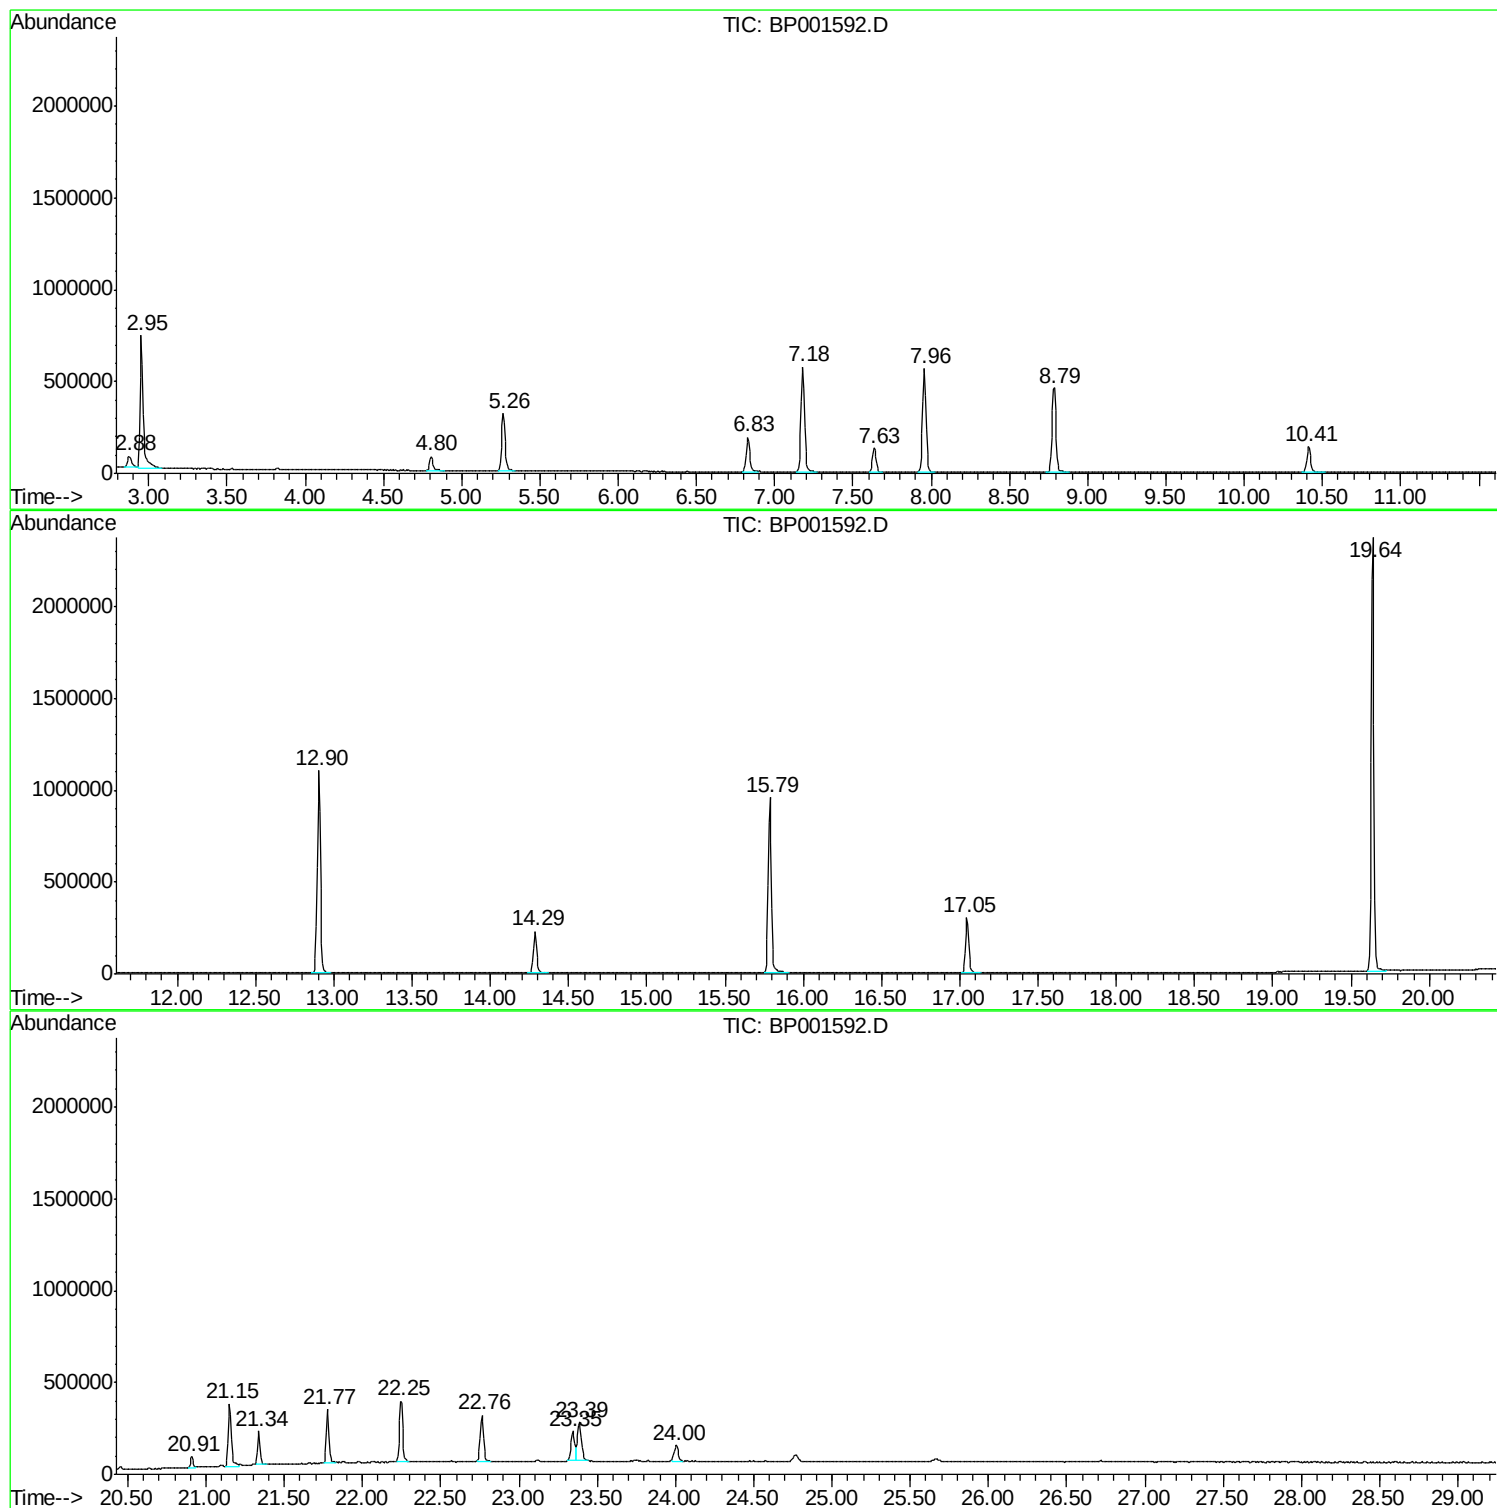

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP011420\\
Data_File : BP001592.D
Acq_On : 14 Jan 2020 17:511
Operator : JUJ
Sample : PB126085BLL
Misc :
ALS_Vial : 4 Sample_Multiplier: 11

Instrument :
BNA_P
ClientSampleId :
PB126085BL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010820.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
