


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP011420\
 Data File : BP001589.D
 Acq On : 14 Jan 2020 16:02
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 14 21:52:04 2020

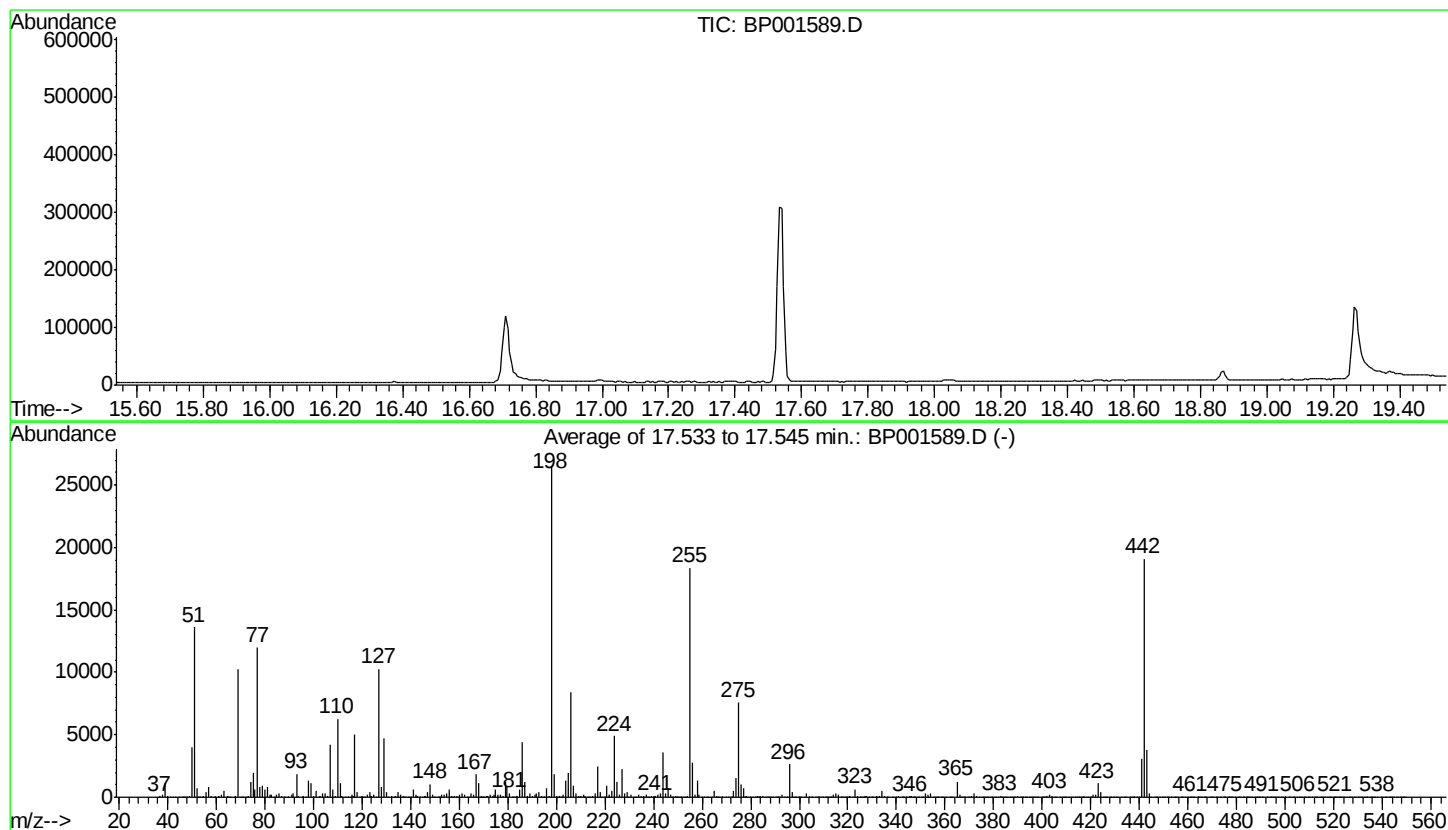

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.2	13584	PASS
68	69	0.00	2	1.4	145	PASS
69	198	0.00	100	38.7	10275	PASS
70	69	0.00	2	0.4	37	PASS
127	198	10	80	38.7	10263	PASS
197	198	0.00	2	0.6	152	PASS
198	198	100	100	100.0	26544	PASS
199	198	5	9	7.1	1883	PASS
275	198	10	60	28.5	7575	PASS
365	198	1	100	4.7	1251	PASS
441	198	0.01	100	11.7	3098	PASS
442	198	50	100	71.8	19068	PASS
443	442	15	24	19.8	3771	PASS