

Data File : BP001617.D
Acq On : 15 Jan 2020 19:40
Operator : JU
Sample : L1114-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RBR-200057-27

Quant Time: Jan 16 06:02:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 14 21:52:04 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	34132	20.00	ng	0.00
21) Naphthalene-d8	10.41	136	123619	20.00	ng	0.00
39) Acenaphthene-d10	14.28	164	85142	20.00	ng	0.00
64) Phenanthrene-d10	17.05	188	186835	20.00	ng	0.00
76) Chrysene-d12	21.14	240	180682	20.00	ng	-0.01
87) Perylene-d12	23.38	264	191624	20.00	ng	-0.01

System Monitoring Compounds						
5) 2-Fluorophenol	5.26	112	168625	96.78	ng	0.00
7) Phenol-d6	6.83	99	238686	85.71	ng	0.00
23) Nitrobenzene-d5	8.78	82	169528	59.93	ng	0.00
42) 2,4,6-Tribromophenol	15.78	330	95157	73.42	ng	-0.01
45) 2-Fluorobiphenyl	12.90	172	350785	60.58	ng	0.00
79) Terphenyl-d14	19.63	244	571132	57.82	ng	0.00


Target Compounds				Qvalue		
10) Phenol	6.85	94	6025	2.092	ng	# 66
32) Benzoic acid	9.71	122	38	4.727	ng	# 36
50) Dimethylphthalate	13.75	163	36622	5.222	ng	99
70) Pentachlorophenol	16.70	266	24609	18.197	ng	96
71) Phenanthrene	17.09	178	42484	4.181	ng	100
75) Fluoranthene	19.07	202	90227	6.749	ng	99
78) Pyrene	19.42	202	71904	5.417	ng	# 96
81) Benzo(a)anthracene	21.13	228	41887	3.329	ng	92
83) Chrysene	21.18	228	37185	3.032	ng	# 93
88) Benzo(b)fluoranthene	22.71	252	47644	3.946	ng	# 90
89) Benzo(k)fluoranthene	22.71	252	47644	4.047	ng	# 91
90) Benzo(a)pyrene	23.28	252	28376	2.475	ng	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BP001617.D
Acq On : 15 Jan 2020 19:40
Operator : JU
Sample : L1114-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RBR-200057-27

Quant Time: Jan 16 06:02:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 14 21:52:04 2020
Response via : Initial Calibration

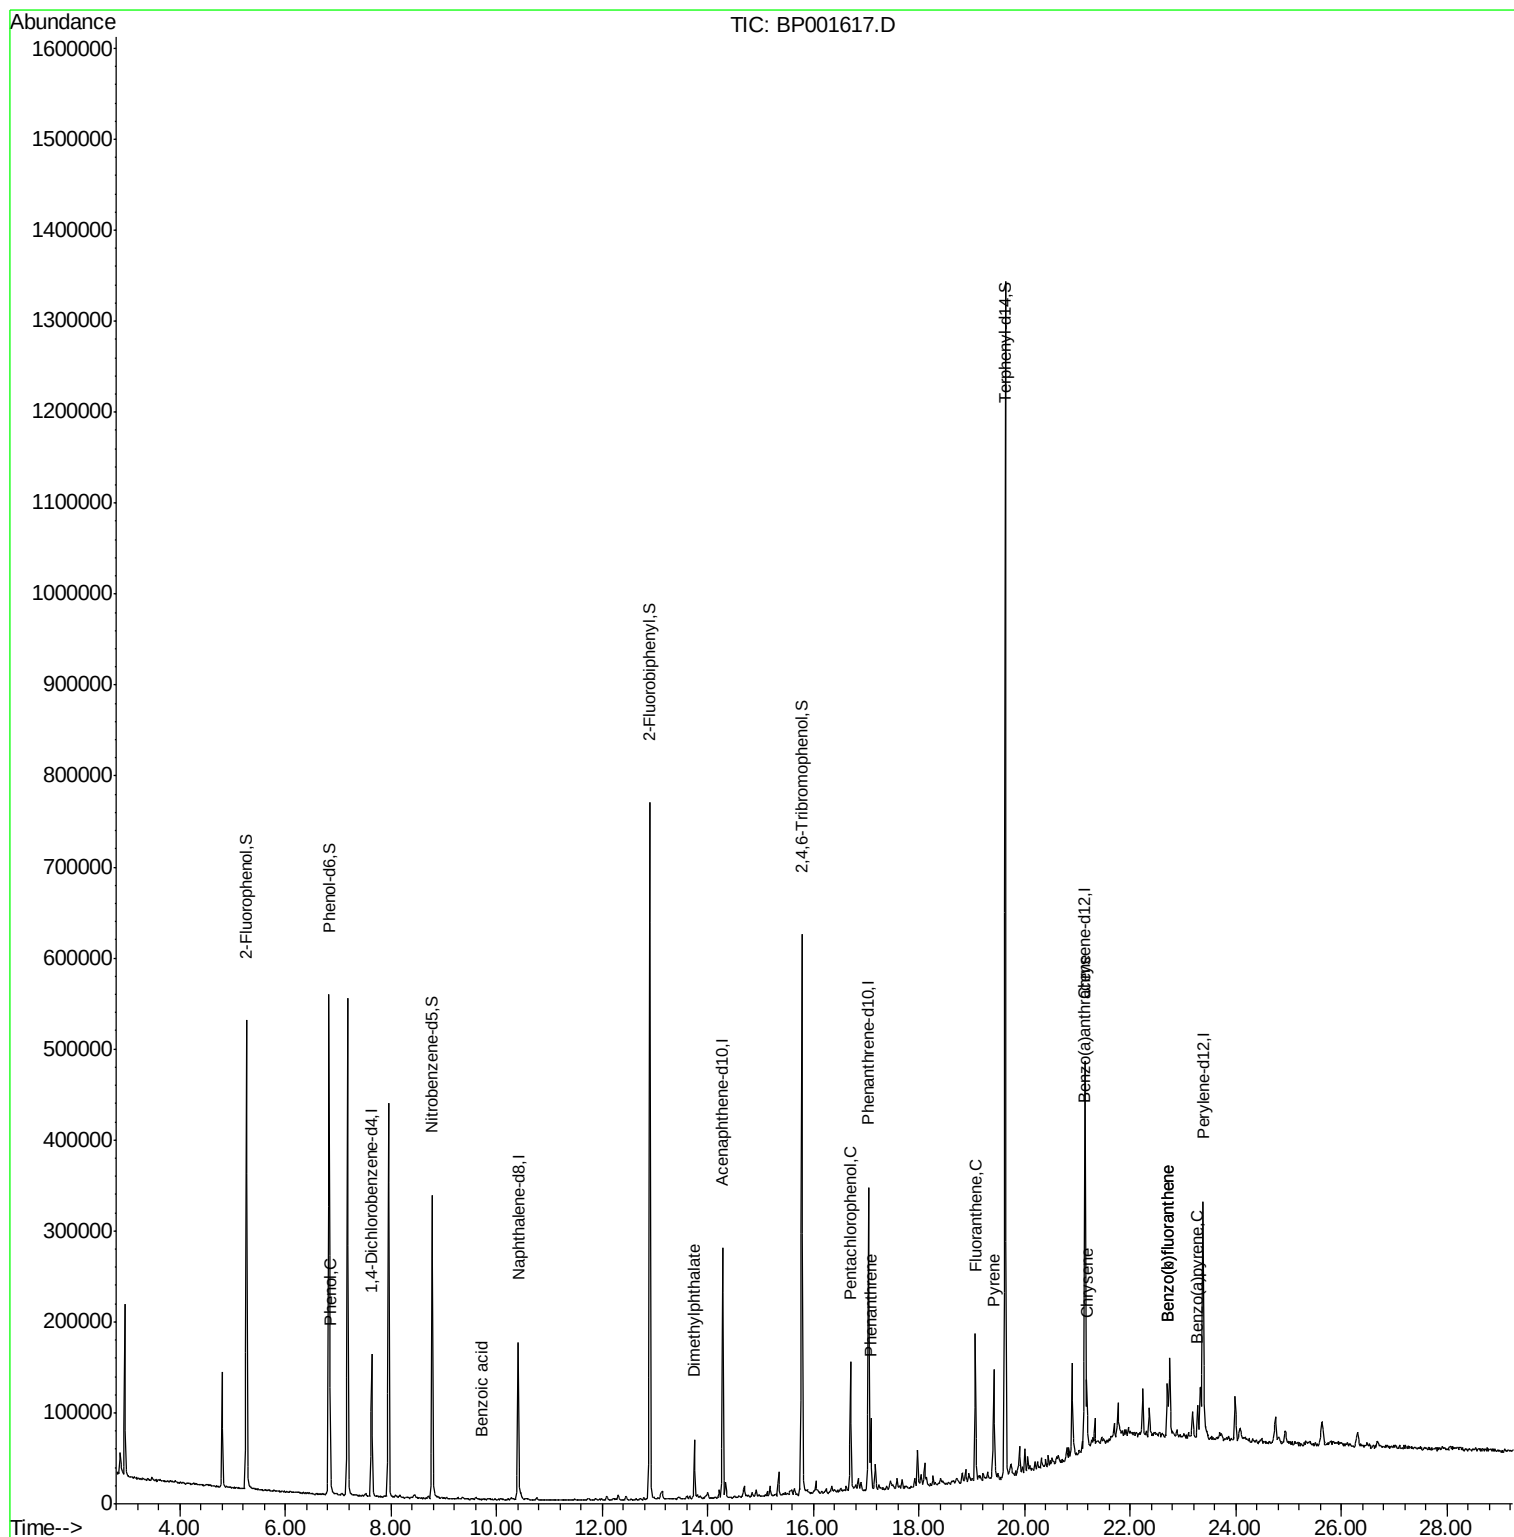

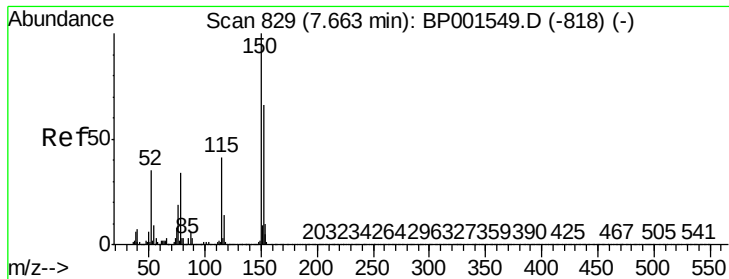


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.63 min Scan# 824
Delta R.T. -0.01 min
Lab File: BP001617.D
Acq: 15 Jan 2020 19:40

Instrument :
BNA_P
ClientSampleId :
RBR-200057-27

Tgt Ion	Ratio	Lower	Upper
152	100		
150	147.9	122.0	183.0
115	60.7	50.7	76.1

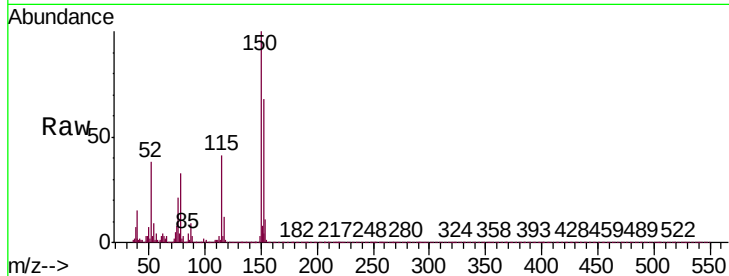


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

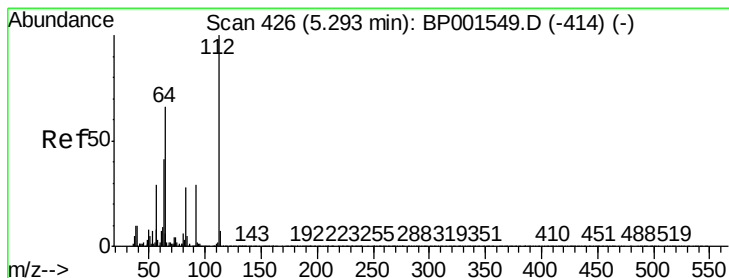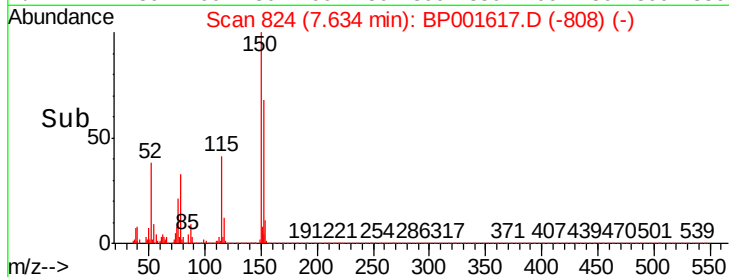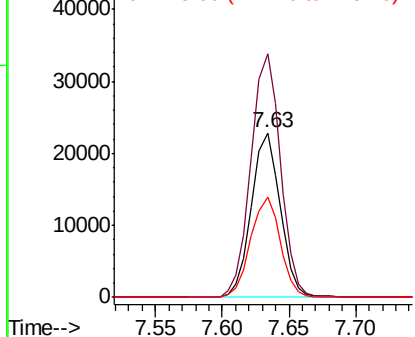



#5


2-Fluorophenol
Concen: 96.777 ng
RT: 5.26 min Scan# 421
Delta R.T. -0.00 min
Lab File: BP001617.D
Acq: 15 Jan 2020 19:40

Tgt Ion	Ratio	Lower	Upper
112	100		
64	71.9	52.8	79.2
63	44.6	33.1	49.7

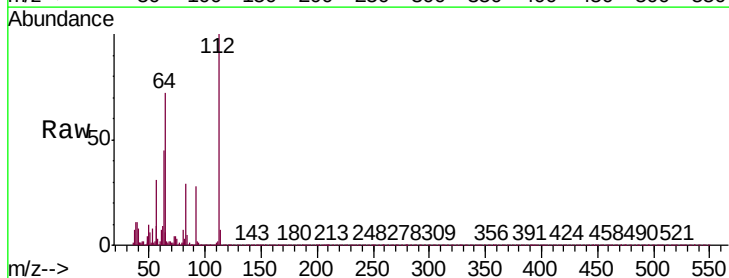

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BP0
Ion 63.00 (62.70 to 63.70): BP0

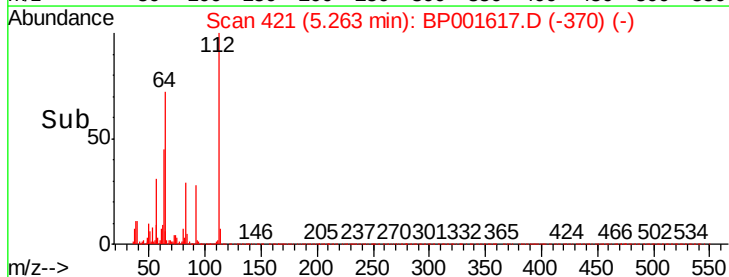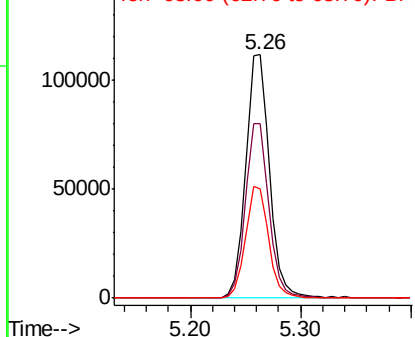

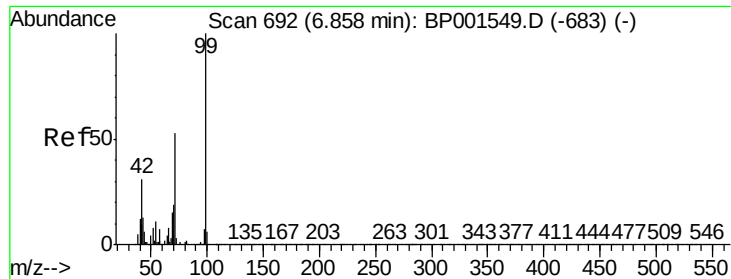

#7

Phenol-d6

Concen: 85.713 ng

RT: 6.83 min Scan# 687

Delta R.T. -0.01 min

Lab File: BP001617.D

Acq: 15 Jan 2020 19:40

Instrument :

BNA_P

ClientSampleId :

RBR-200057-27





Tgt Ion: 99 Resp: 238686

Ion Ratio Lower Upper

99 100

42 33.6 24.5 36.7

71 51.1 42.4 63.6

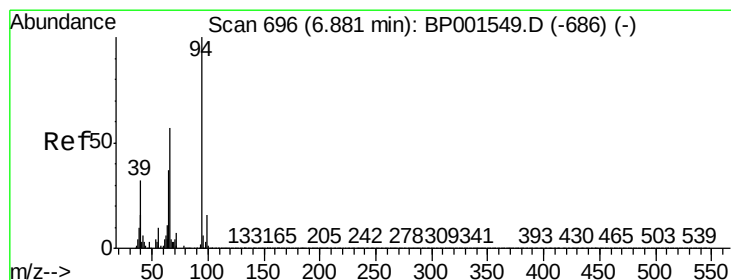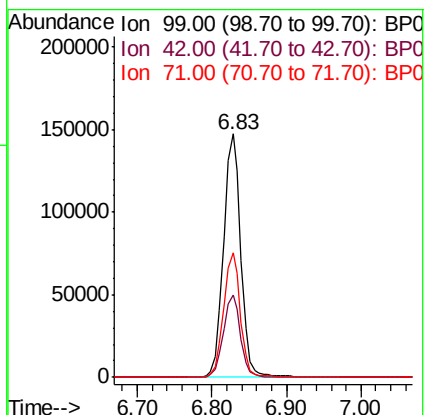

#10

Phenol

Concen: 2.092 ng

RT: 6.85 min Scan# 691

Delta R.T. -0.01 min

Lab File: BP001617.D

Acq: 15 Jan 2020 19:40




Tgt Ion: 94 Resp: 6025


Ion Ratio Lower Upper

94 100

65 50.6 17.5 57.5

66 88.1 36.7 76.7#


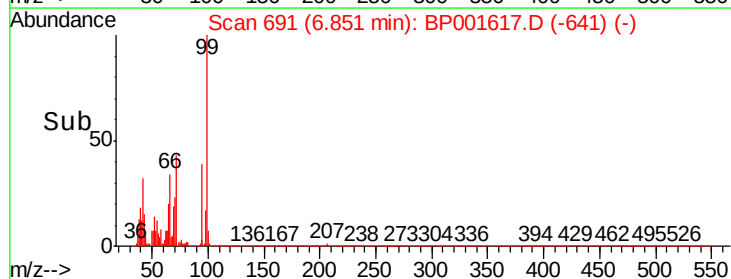
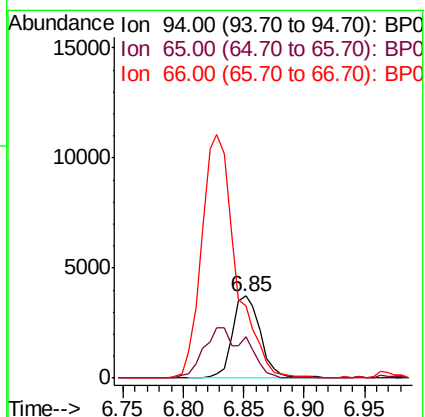
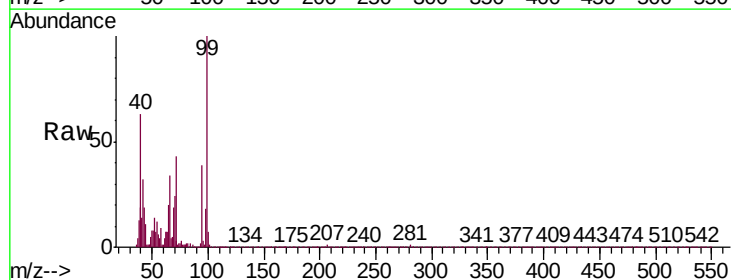




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.41 min Scan# 1296
Delta R.T. -0.01 min
Lab File: BP001617.D
Acq: 15 Jan 2020 19:40




Instrument :
BNA_P
ClientSampleId :
RBR-200057-27


Tgt Ion:	136	Resp:	123619
Ion	Ratio	Lower	Upper
136	100		
137	10.7	8.6	12.8
54	12.3	9.2	13.8
68	6.2	4.1	6.1#

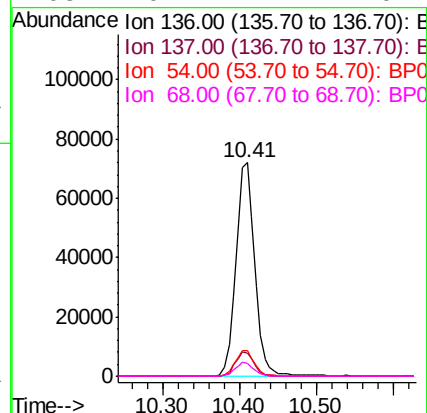

#23
Nitrobenzene-d5
Concen: 59.926 ng
RT: 8.78 min Scan# 1019
Delta R.T. -0.01 min
Lab File: BP001617.D
Acq: 15 Jan 2020 19:40

Tgt Ion:	82	Resp:	169528
Ion	Ratio	Lower	Upper
82	100		
128	35.2	28.4	42.6
54	73.2	53.4	80.2


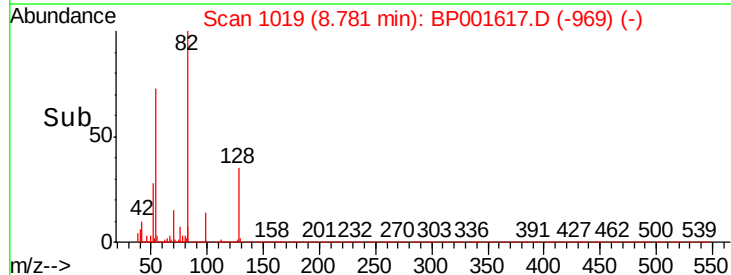
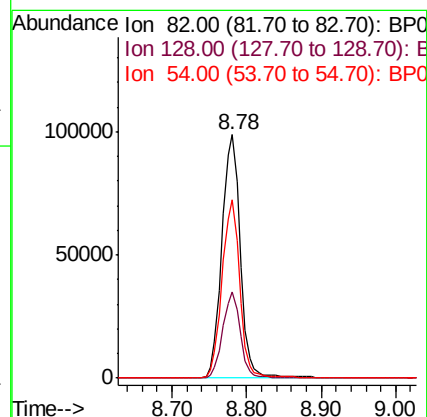



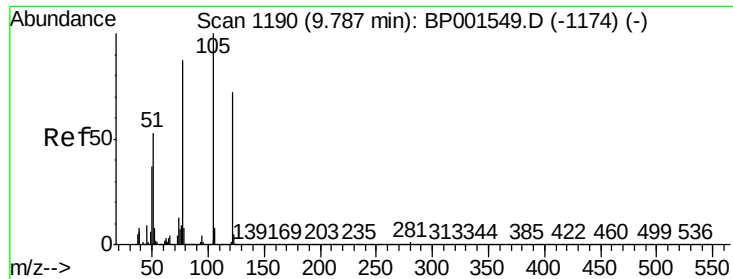

#32
Benzoic acid
Concen: 4.727 ng
RT: 9.71 min Scan# 1177
Delta R.T. -0.04 min
Lab File: BP001617.D
Acq: 15 Jan 2020 19:40




Instrument :
BNA_P
ClientSampleId :
RBR-200057-27


Tgt Ion	Ratio	Lower	Upper
122	100		
105	61.3	119.5	159.5#
77	51.6	102.8	142.8#

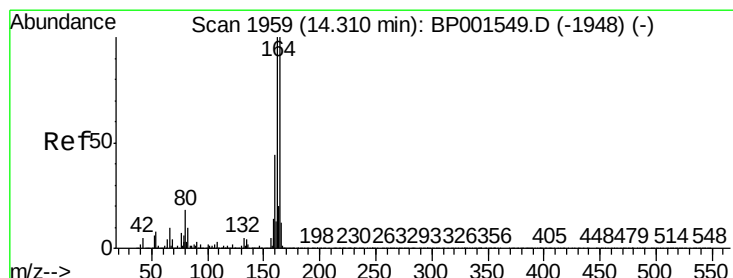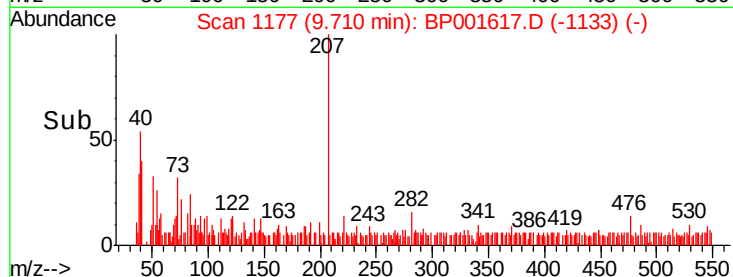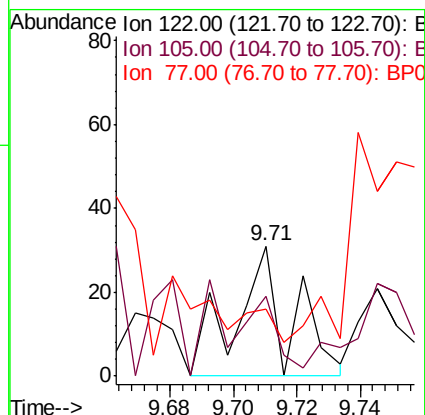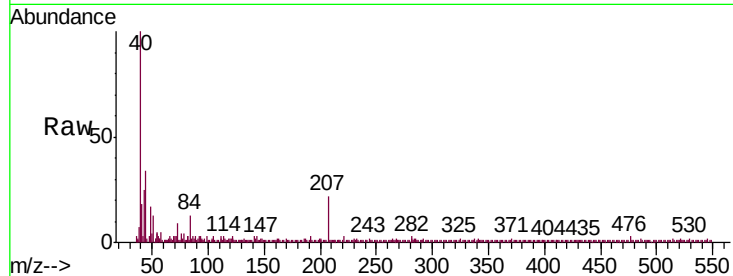

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.28 min Scan# 1954
Delta R.T. -0.01 min
Lab File: BP001617.D
Acq: 15 Jan 2020 19:40

Tgt Ion	Ratio	Lower	Upper
164	100		
162	96.3	79.8	119.6
160	43.2	35.0	52.6


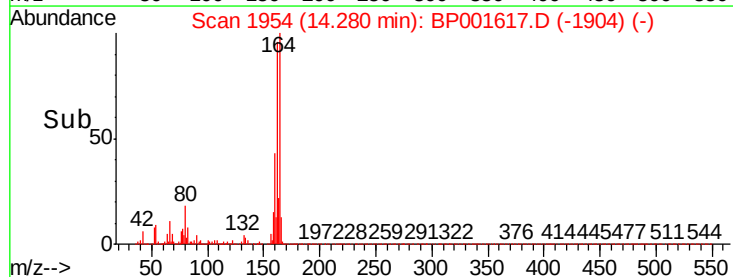
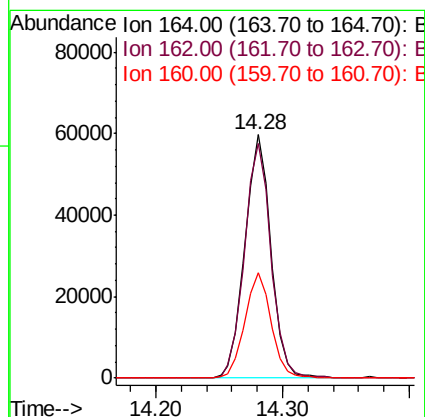
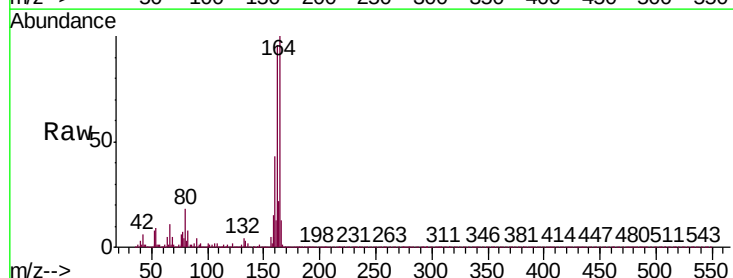


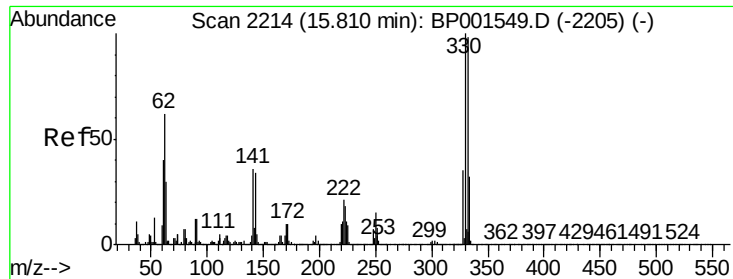

#42
 2,4,6-Tribromophenol
 Concen: 73.422 ng
 RT: 15.78 min Scan# 2209
 Delta R.T. -0.01 min
 Lab File: BP001617.D
 Acq: 15 Jan 2020 19:40




Instrument :
 BNA_P
 ClientSampleId :
 RBR-200057-27


Tgt Ion:330 Resp: 95157
 Ion Ratio Lower Upper
 330 100
 332 95.9 77.8 116.6
 141 38.4 28.7 43.1

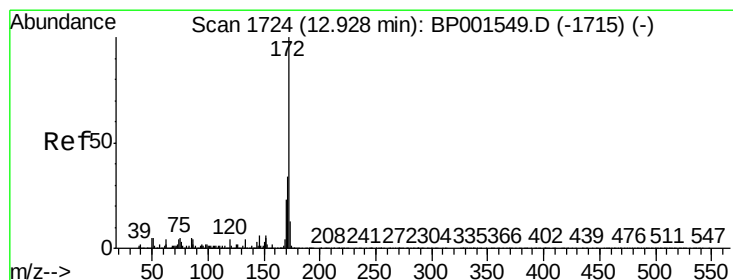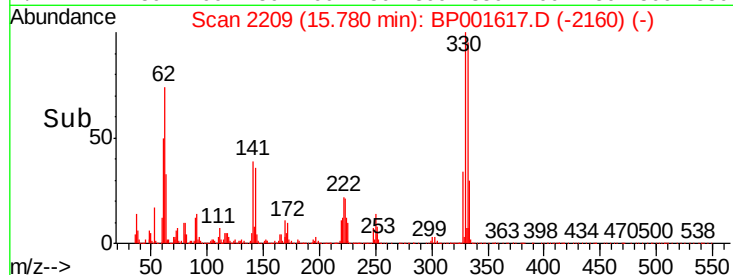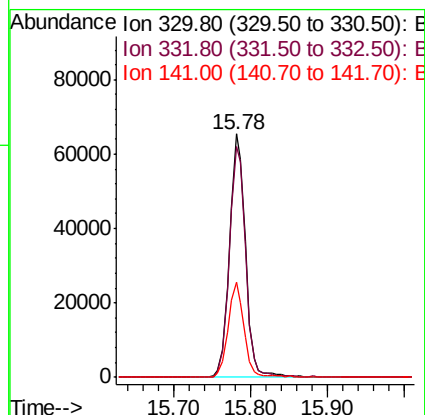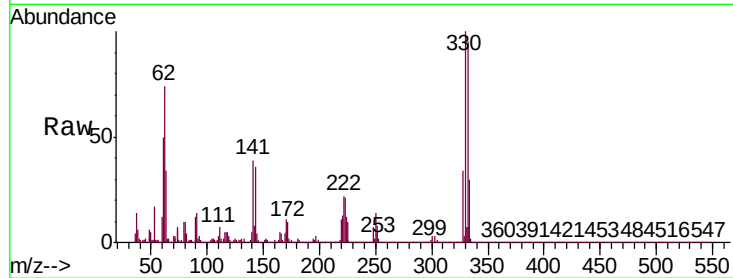

#45
 2-Fluorobiphenyl
 Concen: 60.575 ng
 RT: 12.90 min Scan# 1719
 Delta R.T. -0.01 min
 Lab File: BP001617.D
 Acq: 15 Jan 2020 19:40

Tgt Ion:172 Resp: 350785
 Ion Ratio Lower Upper
 172 100
 171 34.9 27.6 41.4
 170 23.5 18.3 27.5

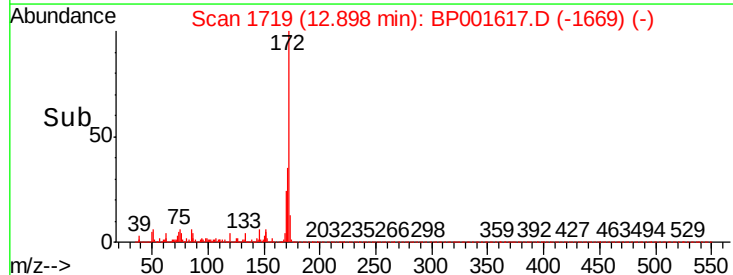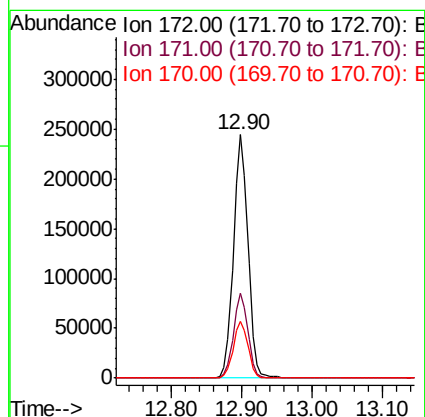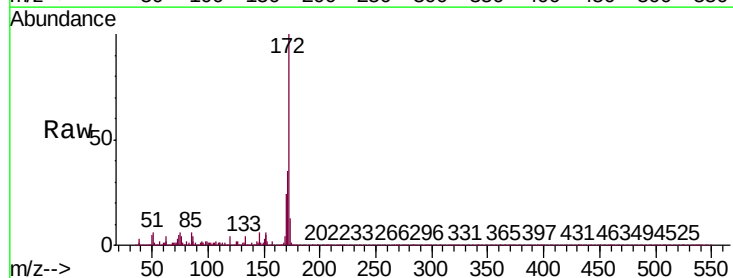

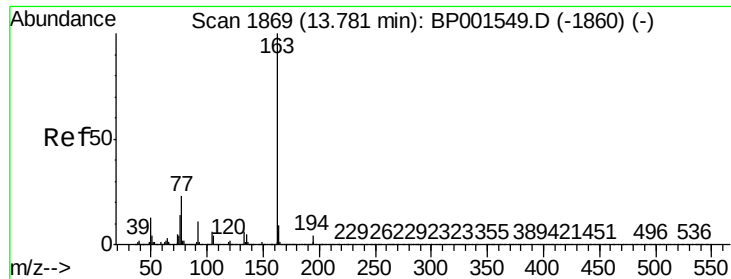

#50

Dimethylphthalate

Concen: 5.222 ng

RT: 13.75 min Scan# 1863

Delta R.T. -0.01 min

Lab File: BP001617.D

Acq: 15 Jan 2020 19:40





Instrument :

BNA_P

ClientSampleId :

RBR-200057-27

Tgt Ion:	163	Resp:	36622
Ion	Ratio	Lower	Upper
163	100		
194	4.3	3.6	5.4
164	9.8	7.5	11.3

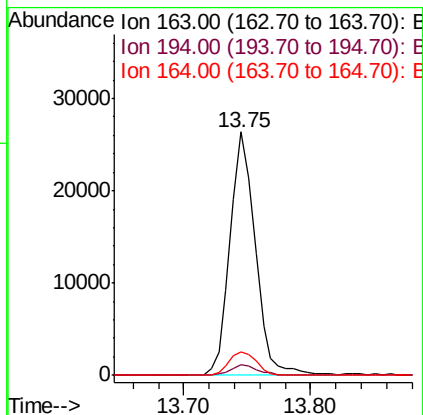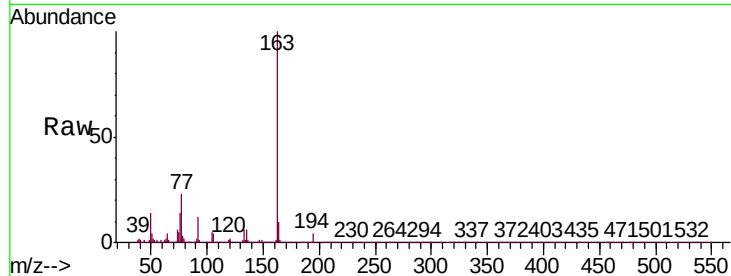

#64

Phenanthrene-d10

Concen: 20.000 ng




RT: 17.05 min Scan# 2424


Delta R.T. -0.01 min

Lab File: BP001617.D

Acq: 15 Jan 2020 19:40

Tgt Ion:	188	Resp:	186835
Ion	Ratio	Lower	Upper
188	100		
94	7.2	5.9	8.9
80	8.5	6.8	10.2

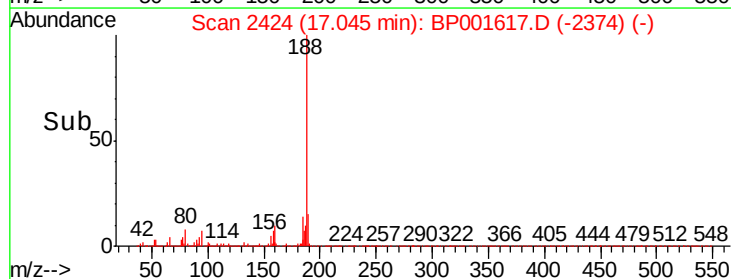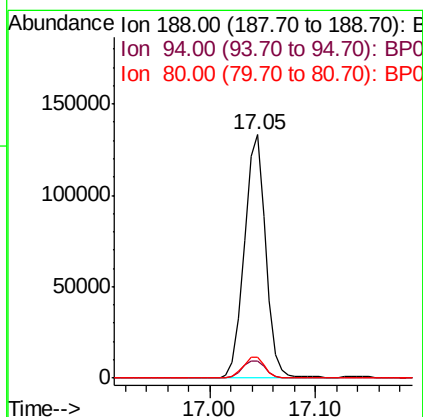

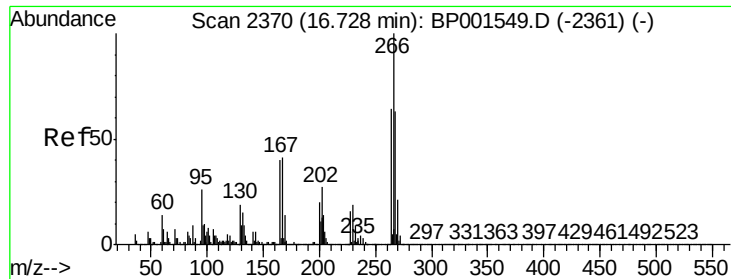

#70

Pentachlorophenol

Concen: 18.197 ng

RT: 16.70 min Scan# 2365

Delta R.T. -0.01 min

Lab File: BP001617.D

Acq: 15 Jan 2020 19:40


Instrument :

BNA_P




ClientSampleId :

RBR-200057-27

Tgt Ion:	266	Resp:	24609
Ion	Ratio	Lower	Upper
266	100		
268	69.1	50.5	75.7
264	64.0	50.9	76.3

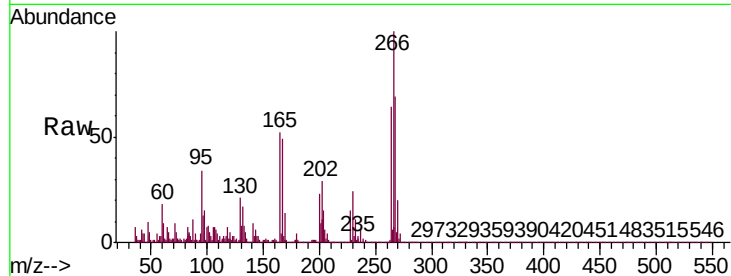

Abundance Ion 265.70 (265.40 to 266.40): E
Ion 268.00 (267.70 to 268.70): E
Ion 264.00 (263.70 to 264.70): E

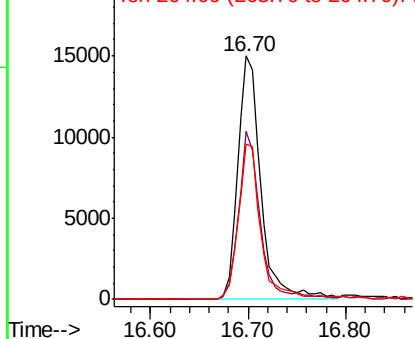

#71

Phenanthrene

Concen: 4.181 ng


RT: 17.09 min Scan# 2431

Delta R.T. -0.01 min



Lab File: BP001617.D


Acq: 15 Jan 2020 19:40

Tgt Ion:	178	Resp:	42484
Ion	Ratio	Lower	Upper
178	100		
176	18.5	14.9	22.3
179	15.5	12.5	18.7



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

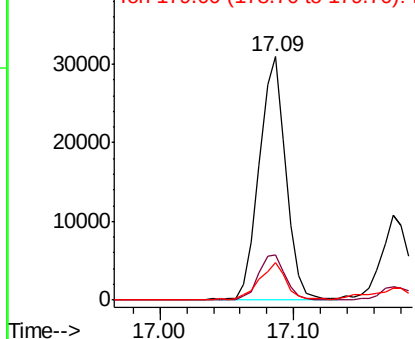



#75

Fluoranthene

Concen: 6.749 ng

RT: 19.07 min Scan# 2768

Delta R.T. -0.01 min

Lab File: BP001617.D

Acq: 15 Jan 2020 19:40





Instrument :

BNA_P

ClientSampleId :

RBR-200057-27

Tgt Ion:	202	Resp:	90227
Ion Ratio	Lower	Upper	
202	100		
101	8.1	0.0	28.4
203	17.0	0.0	37.4

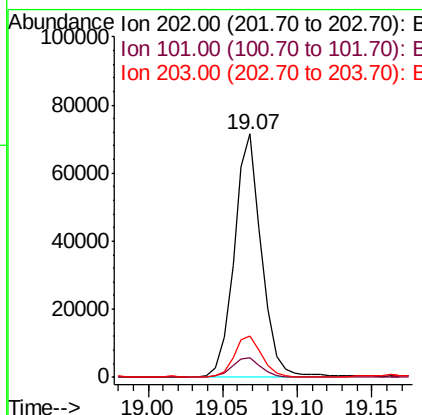

#76

Chrysene-d12

Concen: 20.000 ng




RT: 21.14 min Scan# 3121


Delta R.T. -0.01 min

Lab File: BP001617.D

Acq: 15 Jan 2020 19:40

Tgt Ion:	240	Resp:	180682
Ion Ratio	Lower	Upper	
240	100		
120	8.3	5.7	8.5
236	25.7	20.4	30.6

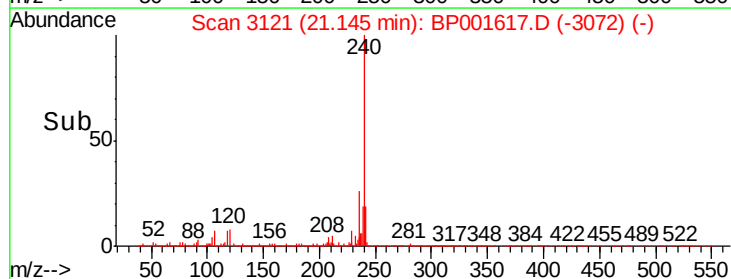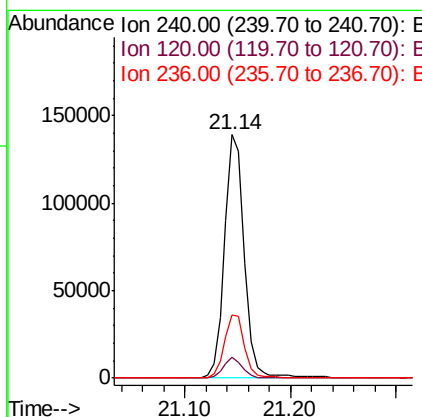

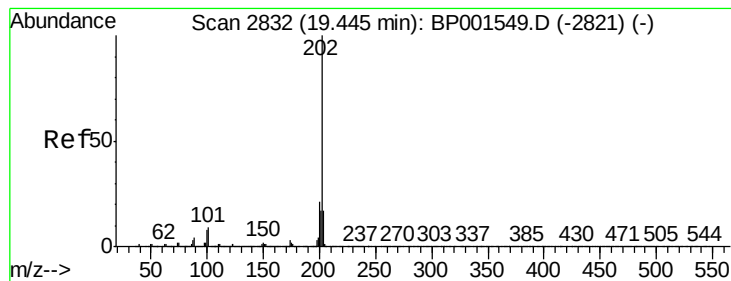

#78

Pyrene

Concen: 5.417 ng

RT: 19.42 min Scan# 2827

Delta R.T. -0.01 min

Lab File: BP001617.D

Acq: 15 Jan 2020 19:40

Instrument :

BNA_P

ClientSampleId :

RBR-200057-27


Tgt Ion: 202 Resp: 71904

Ion Ratio Lower Upper

202 100

200 20.8 17.0 25.6




203 20.8 13.7 20.5#

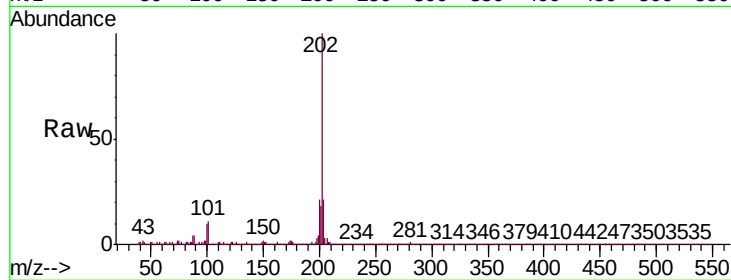

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

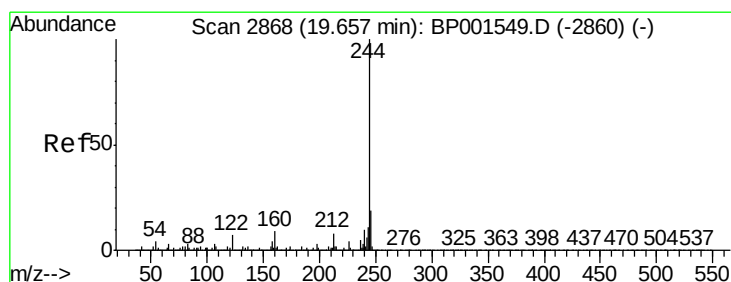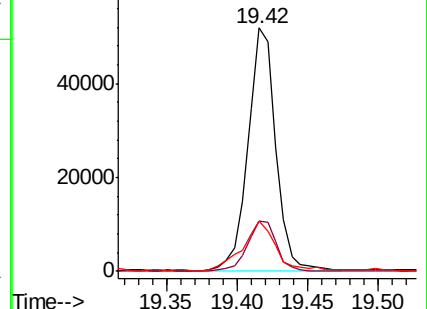

#79

Terphenyl-d14

Concen: 57.815 ng

RT: 19.63 min Scan# 2864

Delta R.T. -0.01 min

Lab File: BP001617.D

Acq: 15 Jan 2020 19:40


Tgt Ion: 244 Resp: 571132

Ion Ratio Lower Upper

244 100

212 7.9 6.3 9.5



122 7.2 5.8 8.6

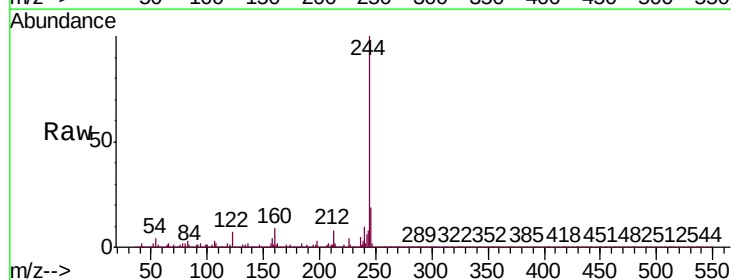


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E




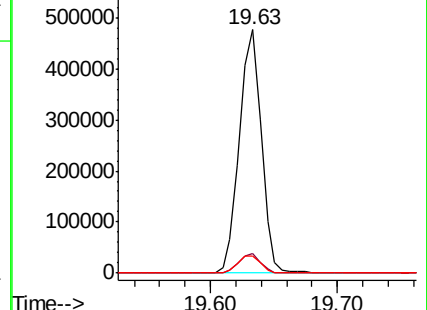


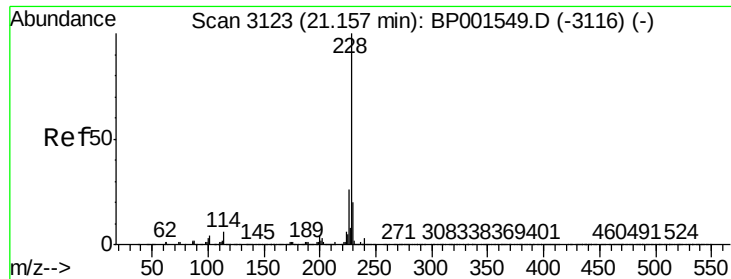

#81
Benzo(a)anthracene
Concen: 3.329 ng
RT: 21.13 min Scan# 3119
Delta R.T. -0.01 min
Lab File: BP001617.D
Acq: 15 Jan 2020 19:40




Instrument :
BNA_P
ClientSampleId :
RBR-200057-27


Tgt Ion:	228	Resp:	41887
Ion Ratio	Lower	Upper	
228	100		
226	30.3	21.2	31.8
229	23.7	16.1	24.1

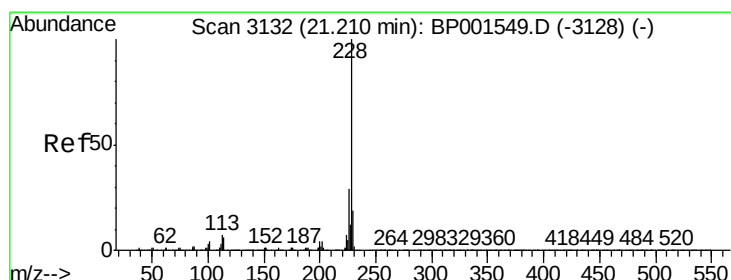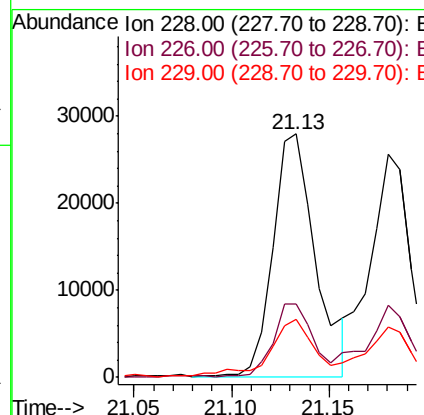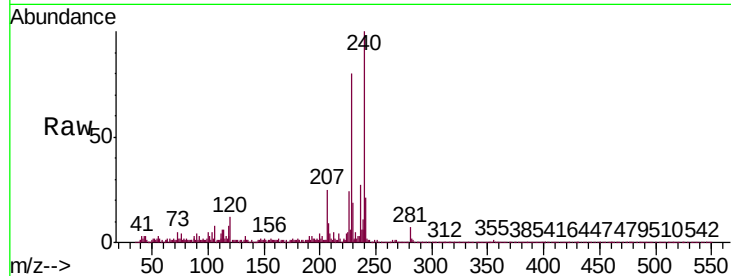

#83
Chrysene
Concen: 3.032 ng
RT: 21.18 min Scan# 3127
Delta R.T. -0.01 min
Lab File: BP001617.D
Acq: 15 Jan 2020 19:40

Tgt Ion:	228	Resp:	37185
Ion Ratio	Lower	Upper	
228	100		
226	32.5	23.2	34.8
229	22.9	15.2	22.8#



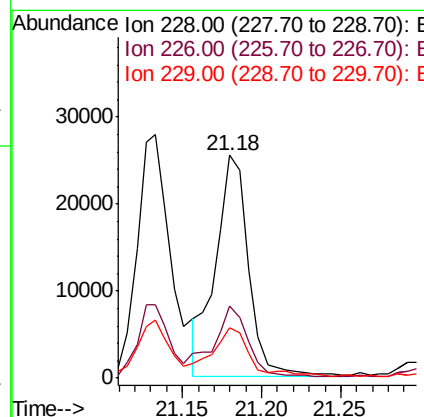



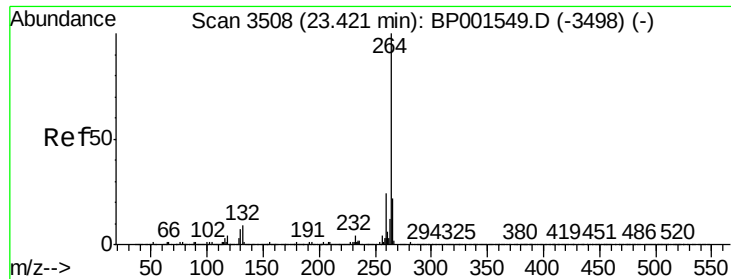

#87
Perylene-d12
Concen: 20.000 ng
RT: 23.38 min Scan# 3501
Delta R.T. -0.01 min
Lab File: BP001617.D
Acq: 15 Jan 2020 19:40




Instrument :
BNA_P
ClientSampleId :
RBR-200057-27


Tgt Ion:	264	Resp:	191624
Ion	Ratio	Lower	Upper
264	100		
260	23.5	19.0	28.6
265	22.0	18.2	27.4

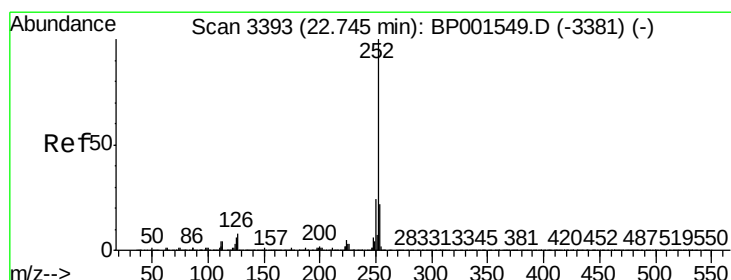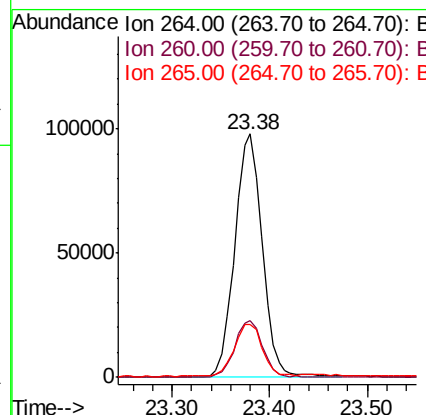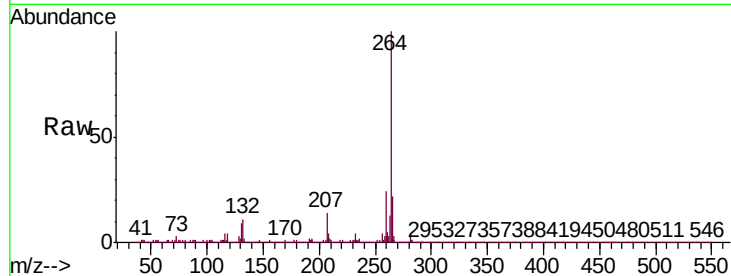

#88
Benzo(b)fluoranthene
Concen: 3.946 ng
RT: 22.71 min Scan# 3387
Delta R.T. -0.01 min
Lab File: BP001617.D
Acq: 15 Jan 2020 19:40

Tgt Ion:	252	Resp:	47644
Ion	Ratio	Lower	Upper
252	100		
253	26.4	17.6	26.4#
125	9.7	4.6	7.0#

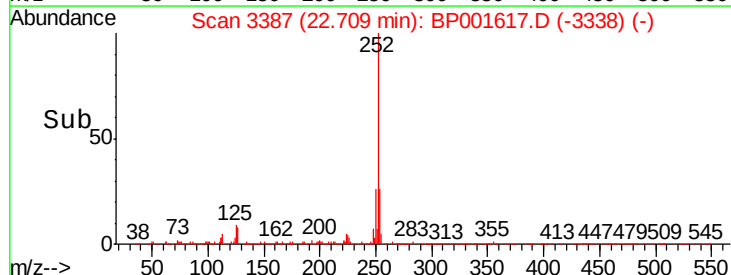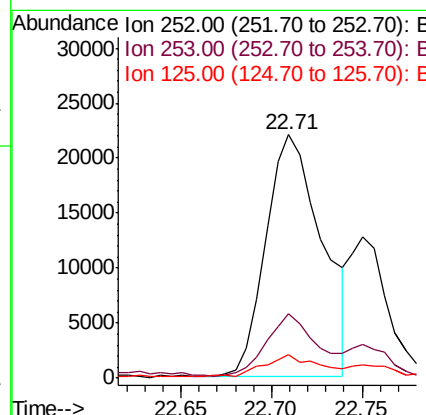



#89

Benzo(k)fluoranthene

Concen: 4.047 ng

RT: 22.71 min Scan# 3387

Delta R.T. -0.06 min

Lab File: BP001617.D

Acq: 15 Jan 2020 19:40

Instrument :

BNA_P

ClientSampleId :

RBR-200057-27


Tgt Ion:252 Resp: 47644

Ion Ratio Lower Upper

252 100

253 26.4 18.2 27.2




125 9.7 4.6 6.8#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

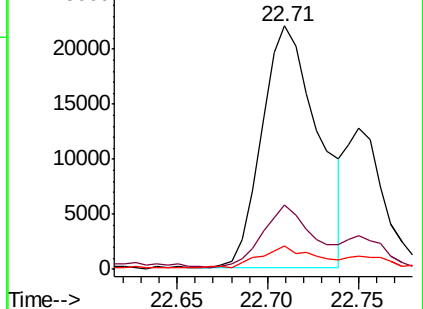

#90

Benzo(a)pyrene

Concen: 2.475 ng

RT: 23.28 min Scan# 3484

Delta R.T. -0.02 min

Lab File: BP001617.D

Acq: 15 Jan 2020 19:40


Tgt Ion:252 Resp: 28376

Ion Ratio Lower Upper

252 100

253 25.2 17.6 26.4

125 7.0 5.0 7.4



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

