
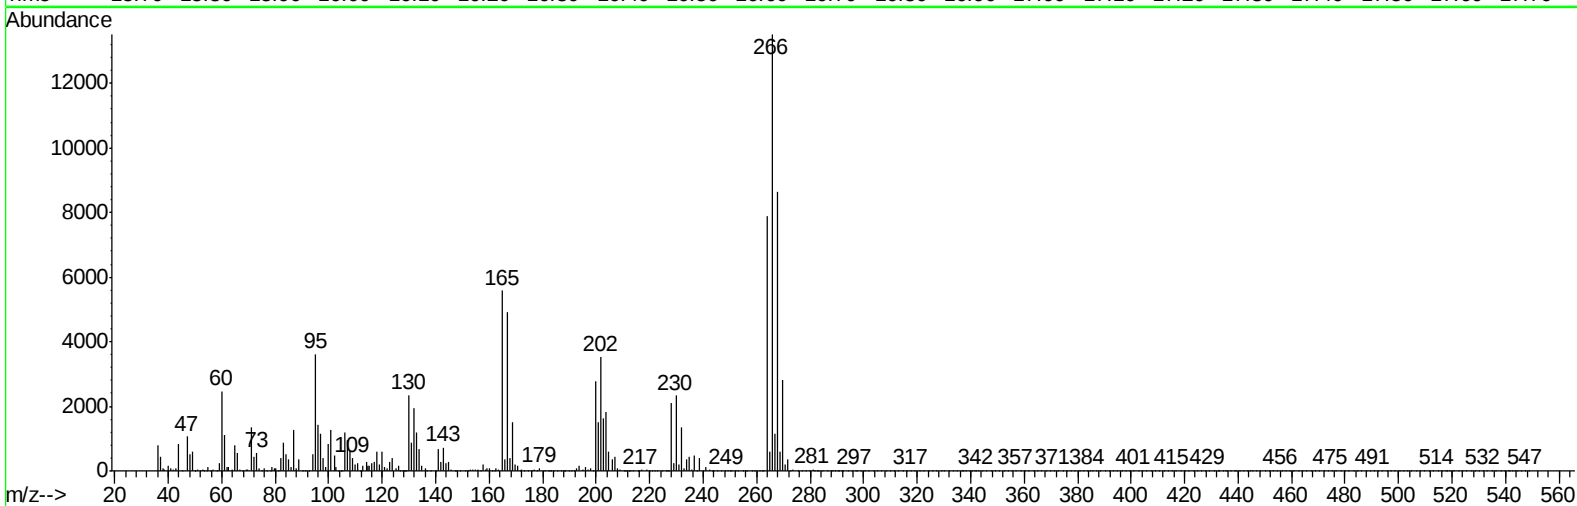


Data File : BP001605.D
Acq On : 15 Jan 2020 12:41
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 08:01:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 14 21:52:04 2020
Response via : Initial Calibration

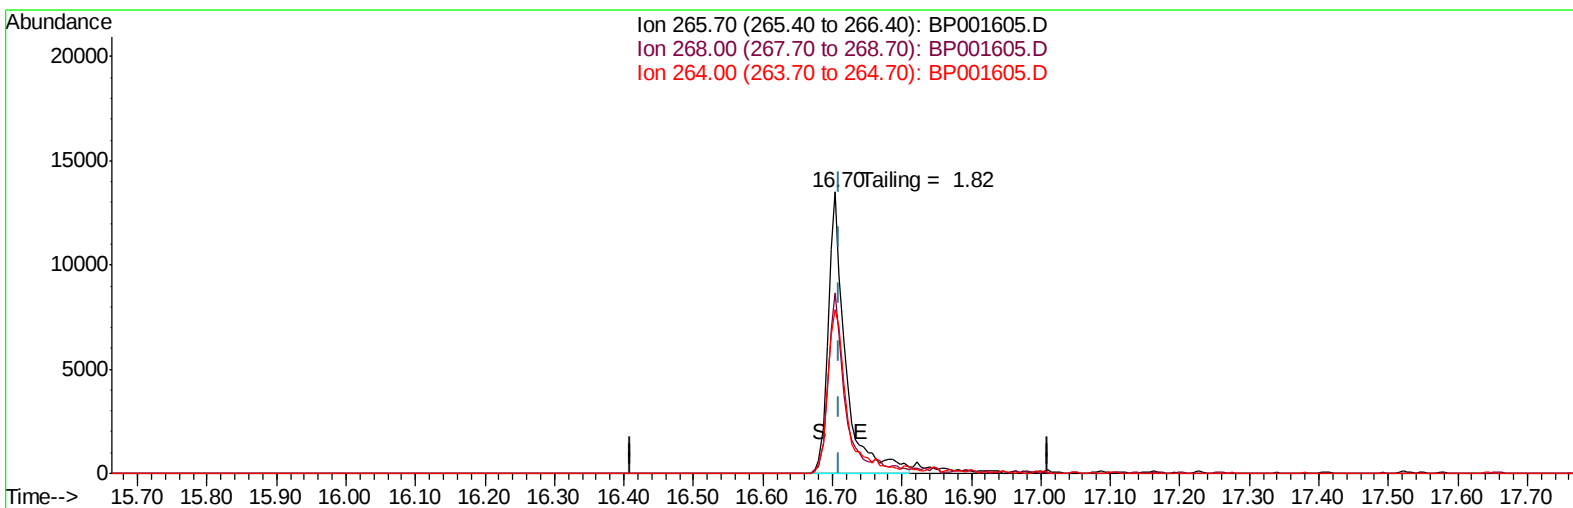

TIC: BP001605.D

(70) Pentachlorophenol (C)



16.704min (-0.006) 280598.96ng

response 22342

Ion	Exp%	Act%
265.70	100	100
268.00	63.10	63.94
264.00	63.60	58.29
0.00	0.00	0.00

Data File : BP001605.D
Acq On : 15 Jan 2020 12:41
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 08:01:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 14 21:52:04 2020
Response via : Initial Calibration

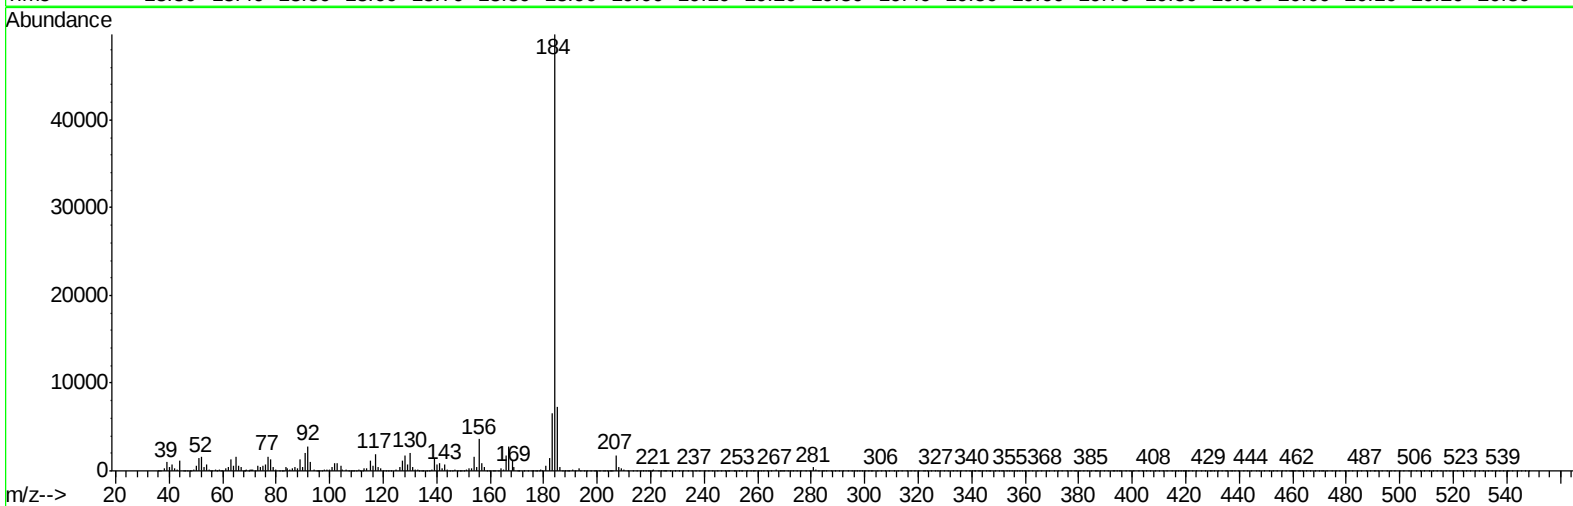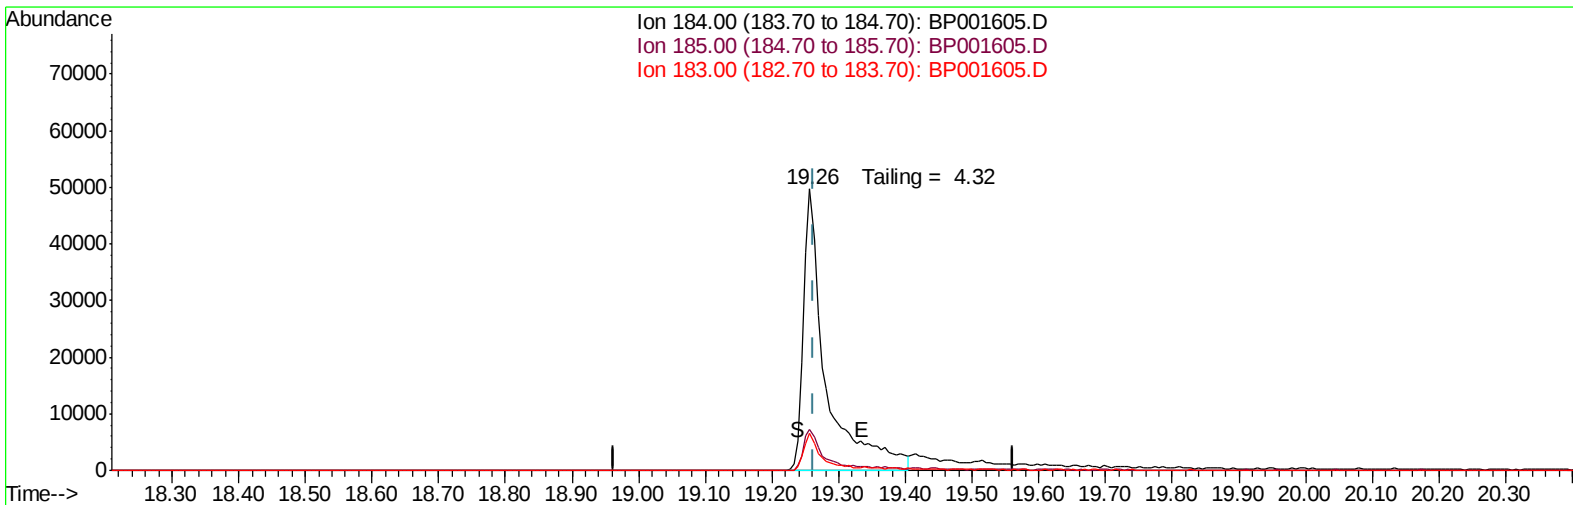

TIC: BP001605.D

(77) Benzidine

19.257min (-0.006) 26311.64ng

response 113549

Ion	Exp%	Act%
184.00	100	100
185.00	13.30	14.76
183.00	11.70	13.25
0.00	0.00	0.00