

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP011520\
 Data File : BP001610.D
 Acq On : 15 Jan 2020 15:43
 Operator : JU
 Sample : L1125-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 FESB-21A-(2.5-3)

Quant Time: Jan 16 06:38:03 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP010820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 14 21:52:04 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	30290	20.00	ng	0.00
21) Naphthalene-d8	10.41	136	106956	20.00	ng	0.00
39) Acenaphthene-d10	14.28	164	76189	20.00	ng	0.00
64) Phenanthrene-d10	17.05	188	177783	20.00	ng	0.00
76) Chrysene-d12	21.15	240	167918	20.00	ng	-0.01
87) Perylene-d12	23.38	264	178982	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.26	112	157977	102.17	ng	0.00
7) Phenol-d6	6.83	99	220465	89.21	ng	0.00
23) Nitrobenzene-d5	8.78	82	156989	64.14	ng	0.00
42) 2,4,6-Tribromophenol	15.78	330	92408	79.68	ng	-0.01
45) 2-Fluorobiphenyl	12.90	172	328449	63.38	ng	0.00
79) Terphenyl-d14	19.63	244	572373	62.35	ng	0.00
Target Compounds						
10) Phenol	6.85	94	5973	2.337	ng	Qvalue # 80
50) Dimethylphthalate	13.75	163	18611	2.966	ng	# 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP011520\
Data File : BP001610.D
Acq On : 15 Jan 2020 15:43
Operator : JU
Sample : L1125-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FESB-21A-(2.5-3)

Quant Time: Jan 16 06:38:03 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP010820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 14 21:52:04 2020
Response via : Initial Calibration

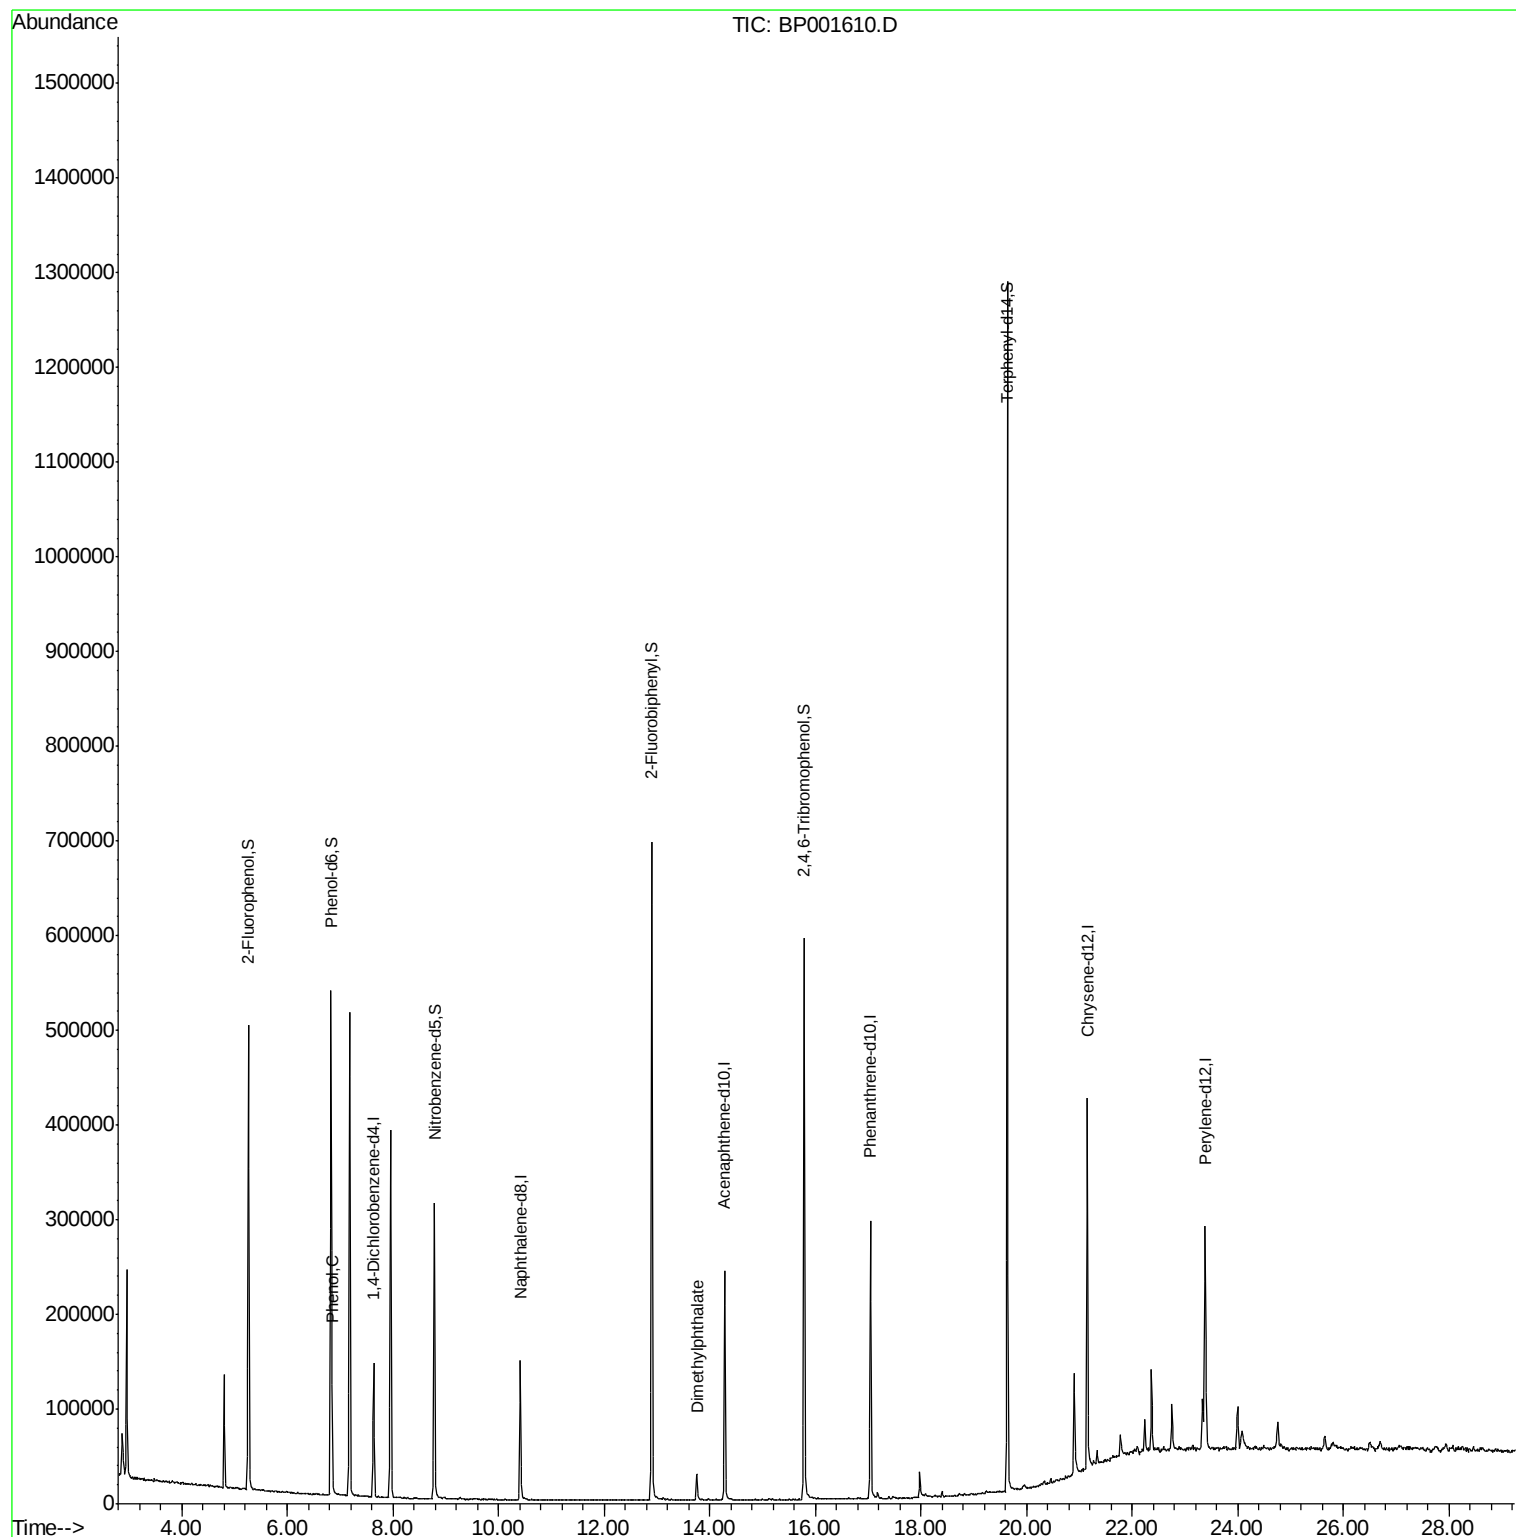


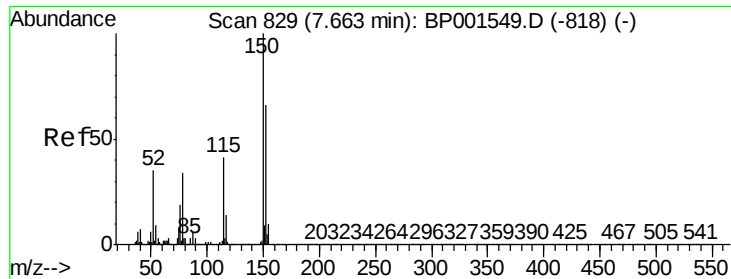

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.63 min Scan# 824
Delta R.T. -0.01 min
Lab File: BP001610.D
Acq: 15 Jan 2020 15:43

Instrument :
BNA_P
ClientSampleId :
FESB-21A-(2.5-3)

Tot Ion	Ratio	Lower	Upper
152	100		
150	157.4	122.0	183.0
115	64.7	50.7	76.1






Abundance

Ion 152.00 (151.70 to 152.70): E


Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

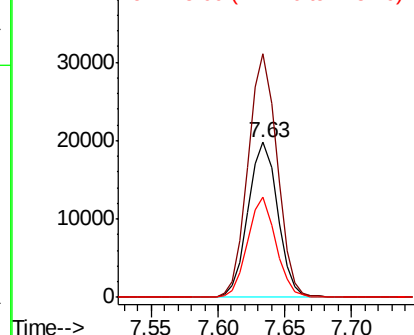

#5
2-Fluorophenol
Concen: 102.166 ng
RT: 5.26 min Scan# 421
Delta R.T. -0.00 min
Lab File: BP001610.D
Acq: 15 Jan 2020 15:43

Tgt Ion	Ratio	Lower	Upper
112	100		
64	70.1	52.8	79.2
63	44.6	33.1	49.7






Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BP0

Ion 63.00 (62.70 to 63.70): BP0

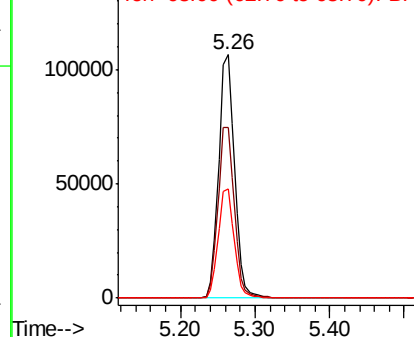

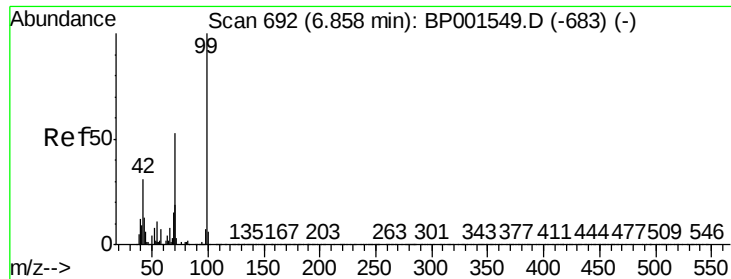

#7

Phenol-d6

Concen: 89.212 ng

RT: 6.83 min Scan# 687

Delta R.T. -0.01 min

Lab File: BP001610.D

Acq: 15 Jan 2020 15:43

Instrument :

BNA_P

ClientSampleId :

FESB-21A-(2.5-3)


Tot Ion: 99 Resp: 220465

Ion Ratio Lower Upper

99 100

42 33.5 24.5 36.7

71 49.4 42.4 63.6



Abundance Ion 99.00 (98.70 to 99.70): BP0

Ion 42.00 (41.70 to 42.70): BP0

Ion 71.00 (70.70 to 71.70): BP0

200000

150000

100000



50000

0

6.83

6.70 6.80 6.90

Time-->



#10

Phenol

Concen: 2.337 ng

RT: 6.85 min Scan# 691

Delta R.T. -0.01 min

Lab File: BP001610.D

Acq: 15 Jan 2020 15:43


Tgt Ion: 94 Resp: 5973

Ion Ratio Lower Upper

94 100

65 41.4 17.5 57.5

66 78.3 36.7 76.7#



Abundance Ion 94.00 (93.70 to 94.70): BP0

Ion 65.00 (64.70 to 65.70): BP0

Ion 66.00 (65.70 to 66.70): BP0

15000

10000


5000


0

6.85

6.80 6.90

Time-->







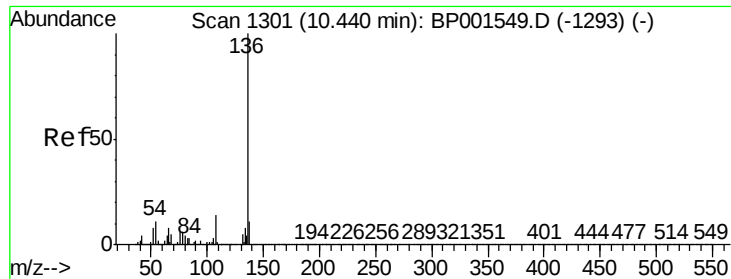

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.41 min Scan# 1296
Delta R.T. -0.01 min
Lab File: BP001610.D
Acq: 15 Jan 2020 15:43




Instrument :
BNA_P
ClientSampleId :
FESB-21A-(2.5-3)


Tot Ion:136	Resp:	106956
Ion	Ratio	Lower Upper
136	100	
137	10.9	8.6 12.8
54	12.8	9.2 13.8
68	5.5	4.1 6.1

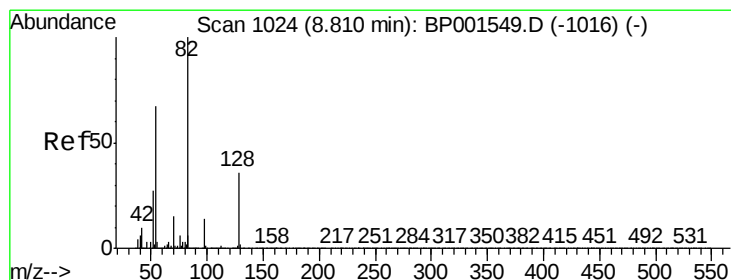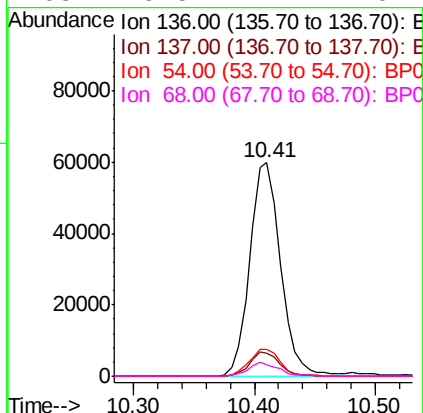

#23
Nitrobenzene-d5
Concen: 64.139 ng
RT: 8.78 min Scan# 1019
Delta R.T. -0.01 min
Lab File: BP001610.D
Acq: 15 Jan 2020 15:43

Tgt Ion: 82	Resp:	156989
Ion	Ratio	Lower Upper
82	100	
128	33.6	28.4 42.6
54	71.1	53.4 80.2


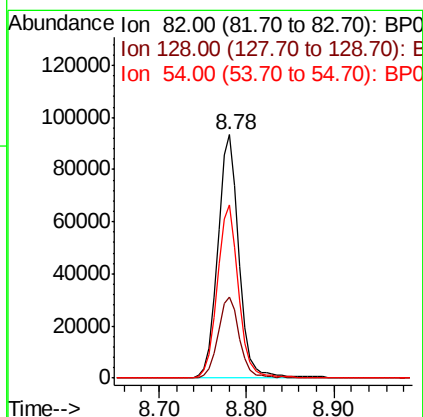
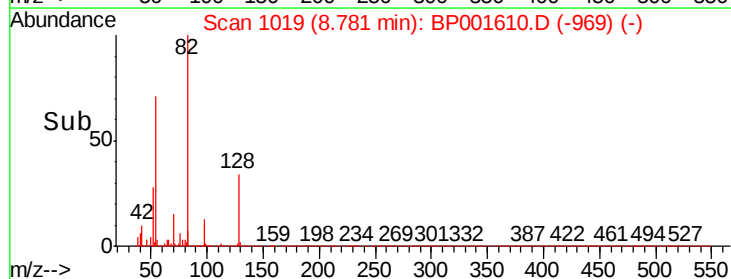
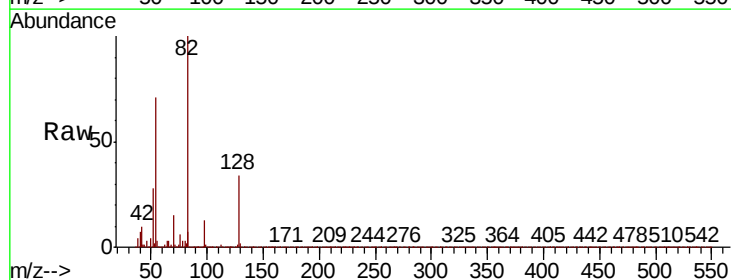




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.28 min Scan# 1954
Delta R.T. -0.01 min
Lab File: BP001610.D
Acq: 15 Jan 2020 15:43




Instrument :
BNA_P
ClientSampleId :
FESB-21A-(2.5-3)


Tot Ion:164 Resp: 76189
Ion Ratio Lower Upper
164 100
162 101.4 79.8 119.6
160 43.3 35.0 52.6

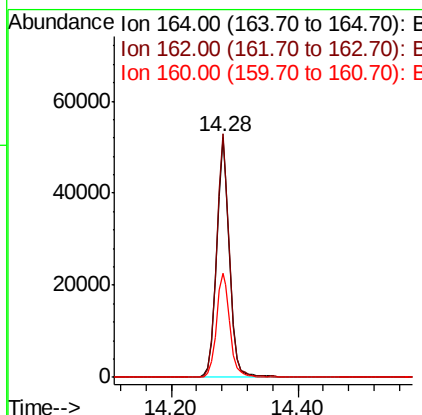

#42
2,4,6-Tribromophenol
Concen: 79.679 ng
RT: 15.78 min Scan# 2209
Delta R.T. -0.01 min
Lab File: BP001610.D
Acq: 15 Jan 2020 15:43

Tgt Ion:330 Resp: 92408
Ion Ratio Lower Upper
330 100
332 94.2 77.8 116.6
141 37.4 28.7 43.1



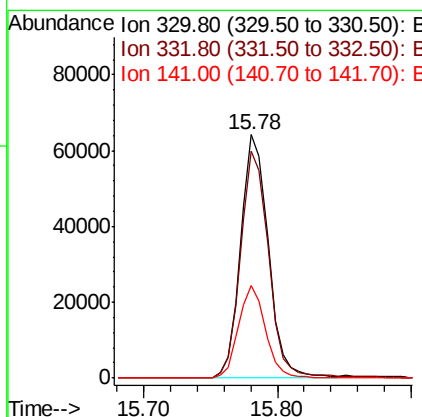



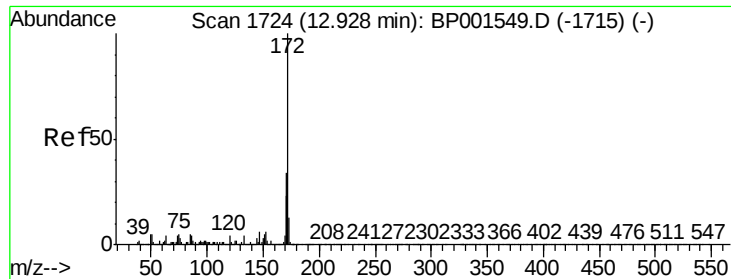

#45
2-Fluorobiphenyl
Concen: 63.383 ng
RT: 12.90 min Scan# 1719
Delta R.T. -0.01 min
Lab File: BP001610.D
Acq: 15 Jan 2020 15:43




Instrument :
BNA_P
ClientSampleId :
FESB-21A-(2.5-3)


Tot Ion	Ratio	Lower	Upper
172	100		
171	35.4	27.6	41.4
170	23.5	18.3	27.5

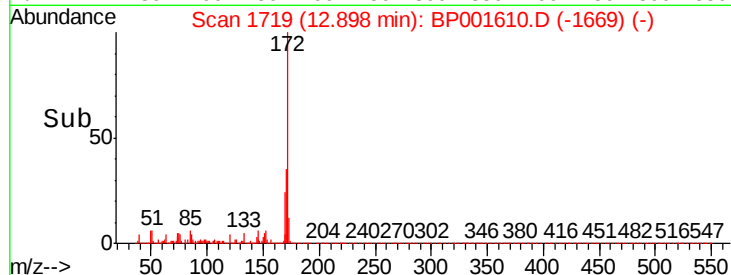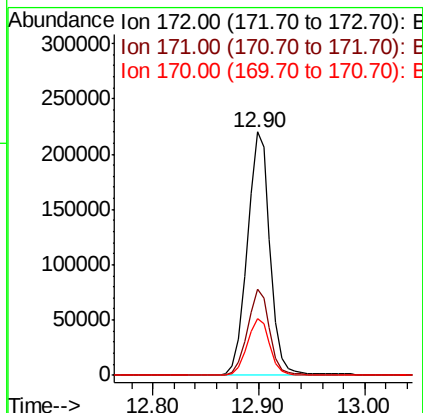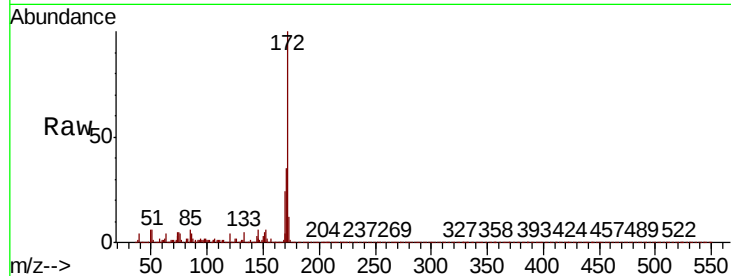

#50
Dimethylphthalate
Concen: 2.966 ng
RT: 13.75 min Scan# 1864
Delta R.T. -0.01 min
Lab File: BP001610.D
Acq: 15 Jan 2020 15:43

Tgt Ion	Ratio	Lower	Upper
163	100		
194	3.7	3.6	5.4
164	12.9	7.5	11.3#

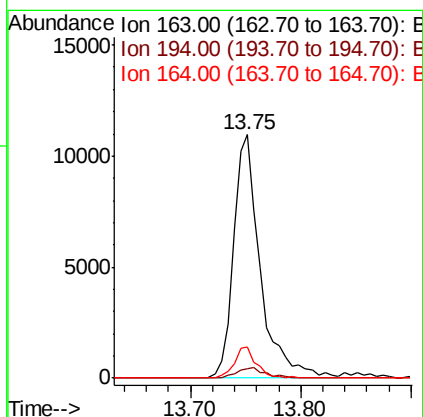



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.05 min Scan# 2424

Delta R.T. -0.01 min

Lab File: BP001610.D

Acq: 15 Jan 2020 15:43

Instrument :

BNA_P

ClientSampleId :

FESB-21A-(2.5-3)


Tot Ion:188 Resp: 177783

Ion Ratio Lower Upper

188 100

94 7.2 5.9 8.9

80 8.1 6.8 10.2



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BP0

Ion 80.00 (79.70 to 80.70): BP0

150000

100000



50000

0

17.05

17.00 17.10

Time-->

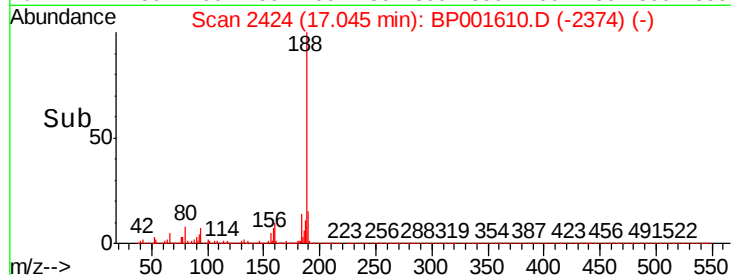

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.15 min Scan# 3121

Delta R.T. -0.01 min

Lab File: BP001610.D

Acq: 15 Jan 2020 15:43


Tgt Ion:240 Resp: 167918

Ion Ratio Lower Upper

240 100

120 7.0 5.7 8.5

236 25.4 20.4 30.6



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

150000

100000


50000


0

21.15

21.10 21.20

Time-->





#79

Terphenyl-d14

Concen: 62.345 ng

RT: 19.63 min Scan# 2864

Delta R.T. -0.01 min

Lab File: BP001610.D

Acq: 15 Jan 2020 15:43

Instrument :

BNA_P

ClientSampleId :

FESB-21A-(2.5-3)


Tot Ion:244 Resp: 572373

Ion Ratio Lower Upper




244 100

212 8.2 6.3 9.5

122 7.1 5.8 8.6



Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

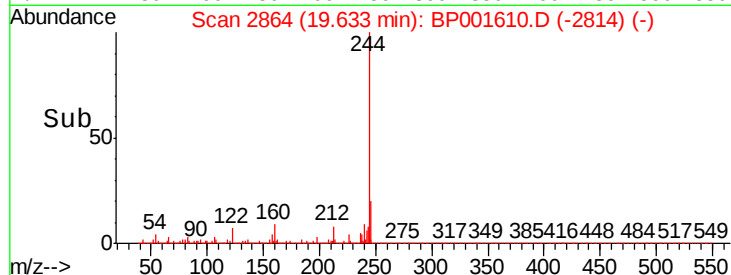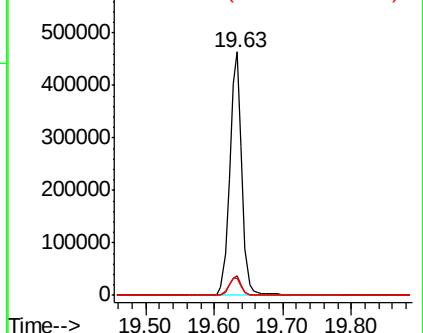

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.38 min Scan# 3501

Delta R.T. -0.01 min

Lab File: BP001610.D

Acq: 15 Jan 2020 15:43


Tgt Ion:264 Resp: 178982

Ion Ratio Lower Upper

264 100

260 22.9 19.0 28.6

265 20.8 18.2 27.4



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

