


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP011520\
 Data File : BP001605.D
 Acq On : 15 Jan 2020 12:41
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 14 21:52:04 2020

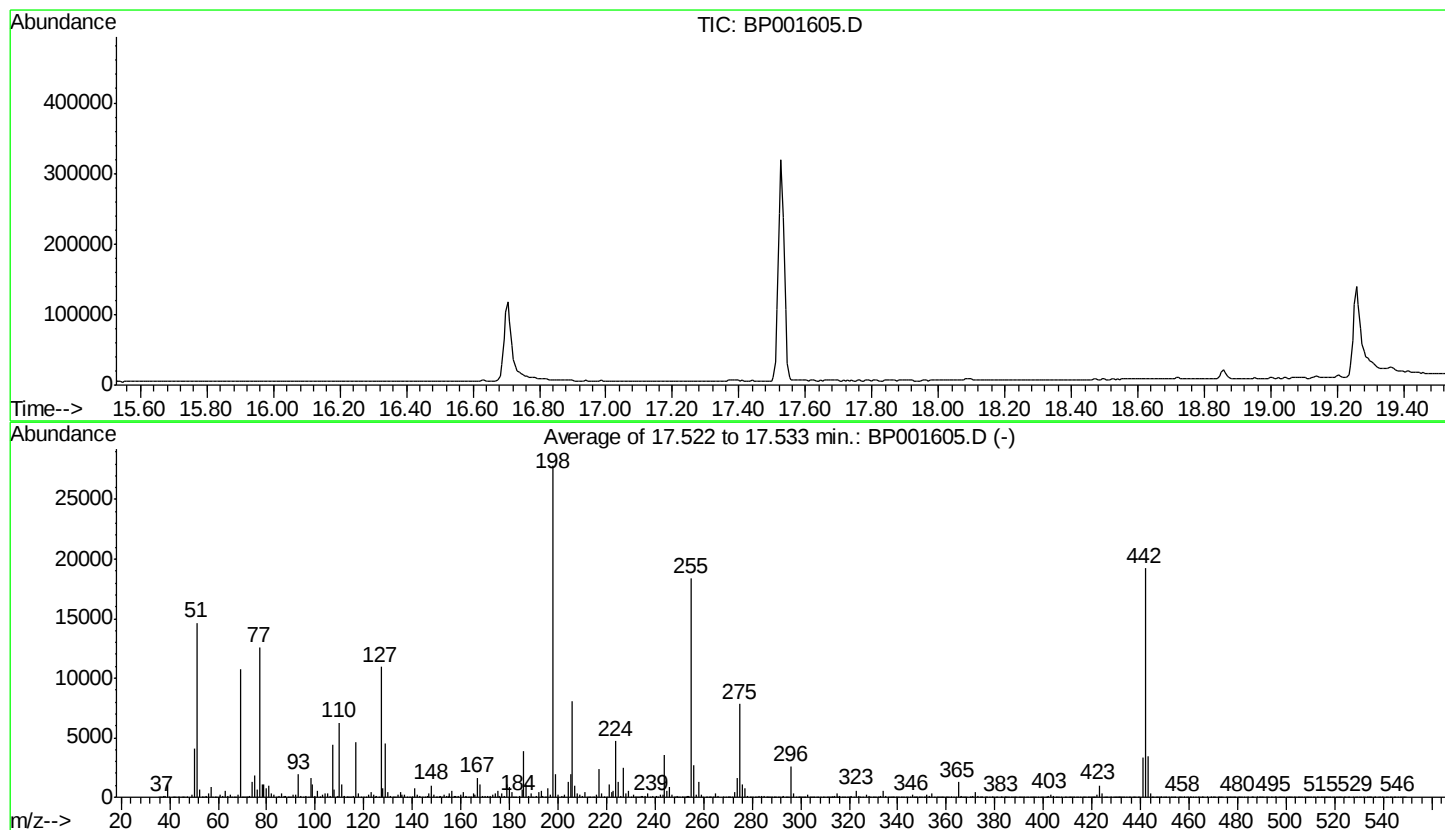

AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2497

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.6	14654	PASS
68	69	0.00	2	1.8	194	PASS
69	198	0.00	100	38.5	10716	PASS
70	69	0.00	2	0.3	32	PASS
127	198	10	80	39.3	10944	PASS
197	198	0.00	2	0.9	241	PASS
198	198	100	100	100.0	27850	PASS
199	198	5	9	7.0	1937	PASS
275	198	10	60	28.0	7808	PASS
365	198	1	100	4.6	1282	PASS
441	198	0.01	100	11.8	3294	PASS
442	198	50	100	68.9	19198	PASS
443	442	15	24	17.8	3410	PASS