
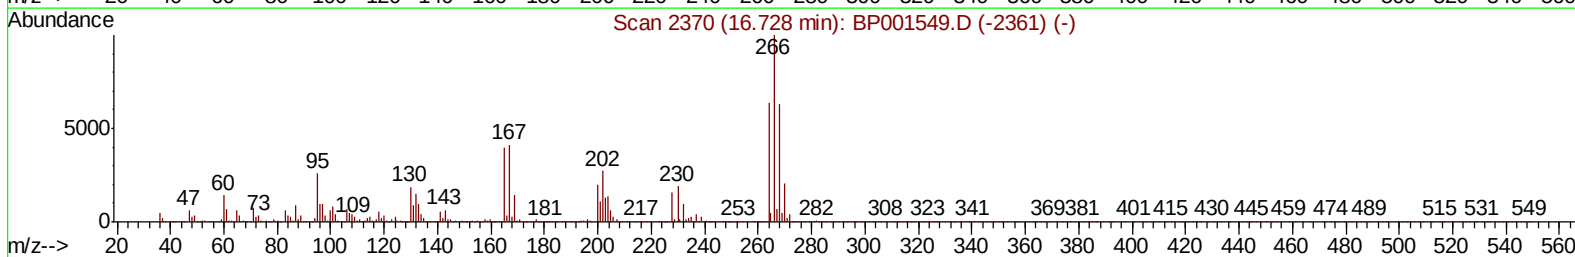
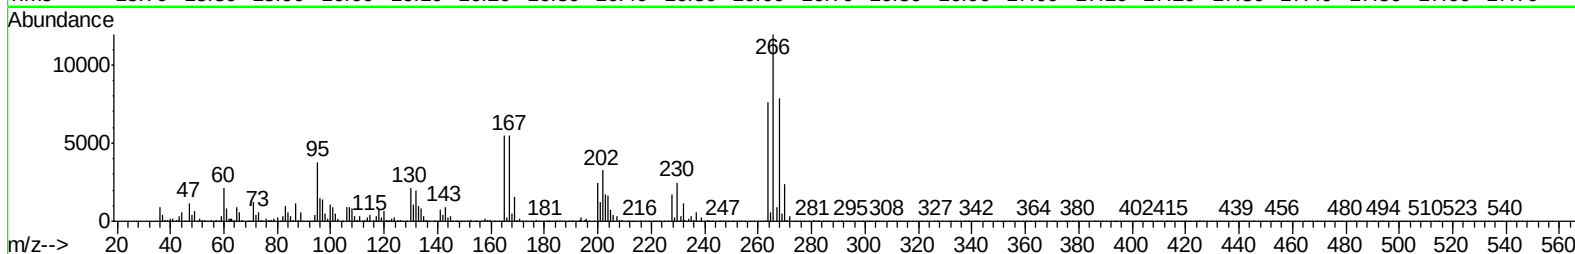


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP011720\  
Data File : BP001650.D  
Acq On : 17 Jan 2020 10:07  
Operator : JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 20 07:38:44 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP010820.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jan 14 21:52:04 2020  
Response via : Initial Calibration

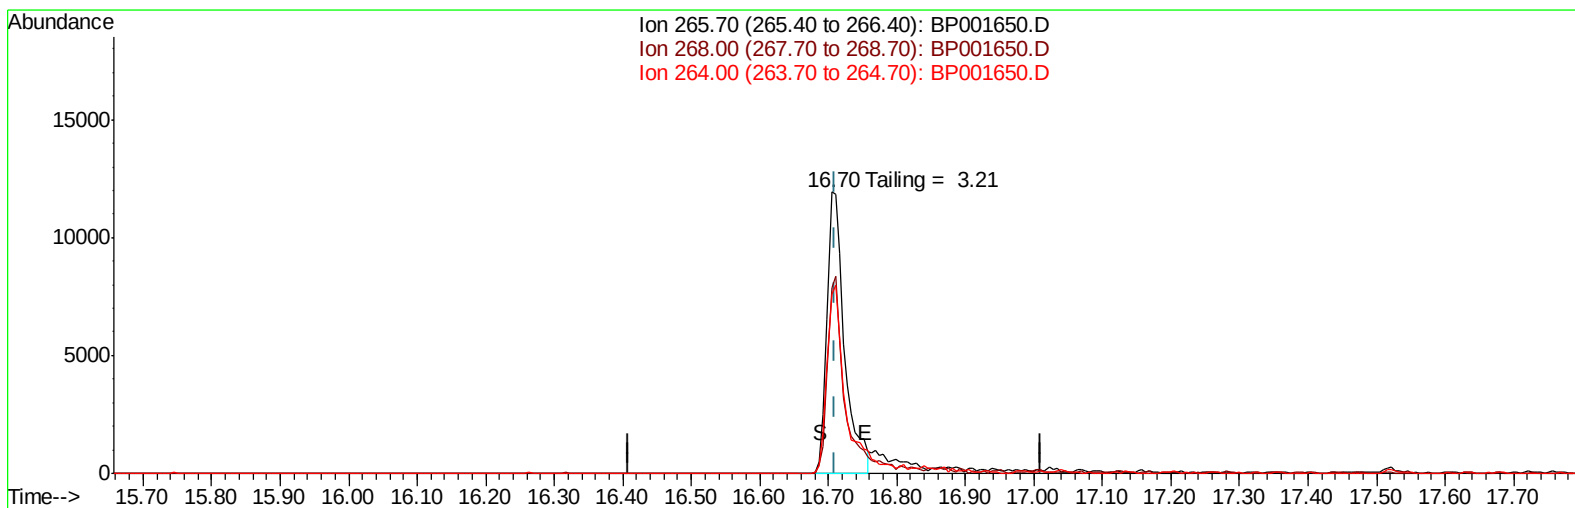

TIC: BP001650.D

(70) Pentachlorophenol (C)




16.704min (-0.006) 242105.79ng

response 22782

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.10 | 69.57 |
| 264.00 | 63.60 | 63.76 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP011720\  
Data File : BP001650.D  
Acq On : 17 Jan 2020 10:07  
Operator : JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 20 07:38:44 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP010820.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jan 14 21:52:04 2020  
Response via : Initial Calibration

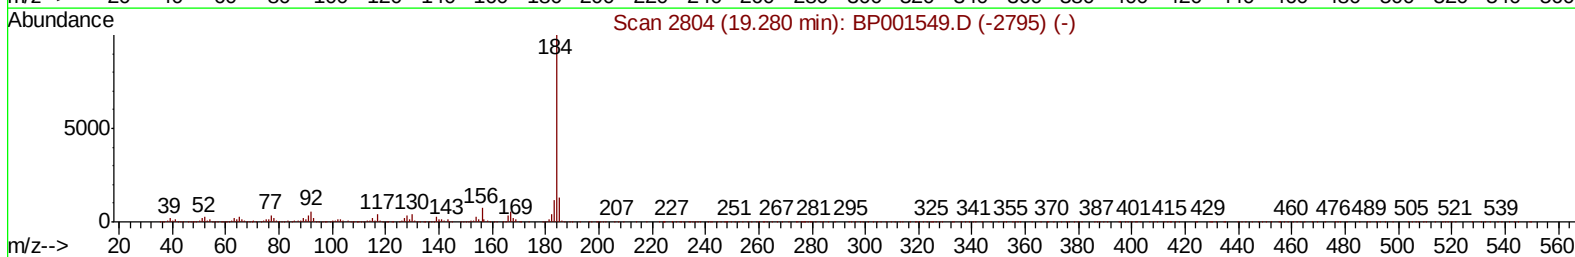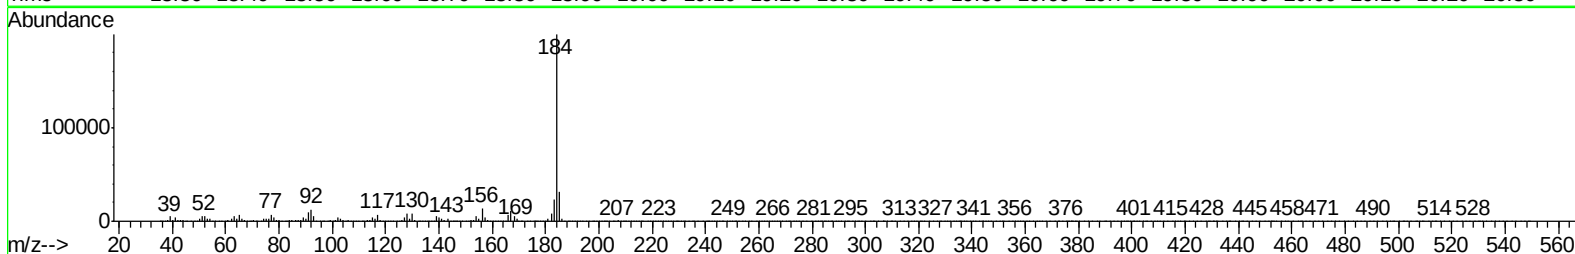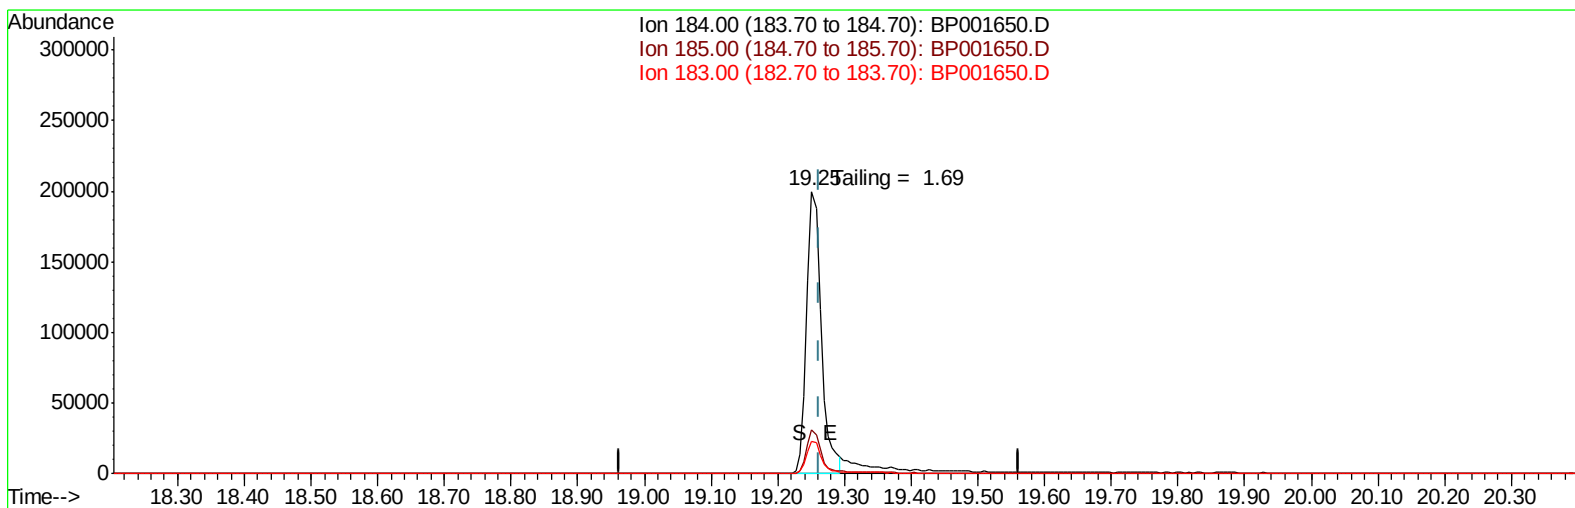

TIC: BP001650.D

(77) Benzidine

19.251min (-0.012) 620128.46ng

response 325674

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 13.30 | 15.48 |
| 183.00 | 11.70 | 11.47 |
| 0.00   | 0.00  | 0.00  |