


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP011720\
 Data File : BP001650.D
 Acq On : 17 Jan 2020 10:07
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 14 21:52:04 2020

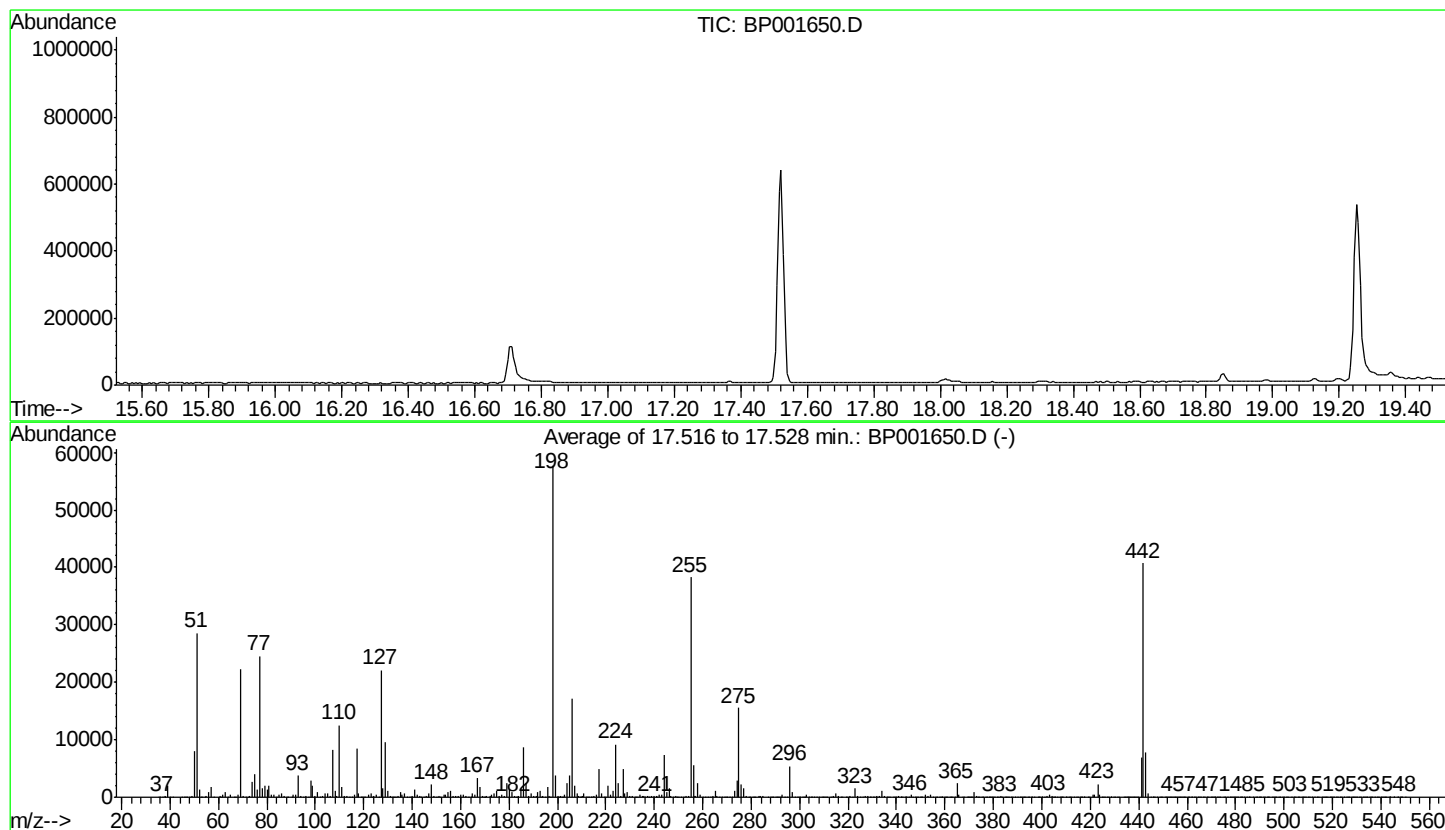

AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2493

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.6	28614	PASS
68	69	0.00	2	1.8	401	PASS
69	198	0.00	100	38.7	22320	PASS
70	69	0.00	2	0.6	131	PASS
127	198	10	80	38.3	22097	PASS
197	198	0.00	2	0.1	67	PASS
198	198	100	100	100.0	57707	PASS
199	198	5	9	6.7	3888	PASS
275	198	10	60	26.9	15526	PASS
365	198	1	100	4.2	2407	PASS
441	198	0.01	100	12.0	6951	PASS
442	198	50	100	70.6	40748	PASS
443	442	15	24	19.3	7866	PASS