

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011924\
 Data File : BP019397.D
 Acq On : 19 Jan 2024 09:54
 Operator : MA/JU
 Sample : PB158500BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK500

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019397.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.205	17	20	29	rVB	28303	39226	1.54%	0.155%
2	3.628	88	92	111	rBV	336289	530082	20.82%	2.091%
3	3.940	143	145	149	rVB	4595	6362	0.25%	0.025%
4	6.957	651	658	671	rBV	393452	643674	25.28%	2.539%
5	7.110	678	684	698	rVB	316468	496085	19.49%	1.957%
6	7.299	710	716	728	rVB	378413	614248	24.13%	2.423%
7	7.469	743	745	749	rBV5	1820	2752	0.11%	0.011%
8	7.769	788	796	806	rBV	345164	534279	20.99%	2.108%
9	8.499	912	920	936	rBV	459315	767302	30.14%	3.027%
10	8.934	987	994	1004	rBV	380381	627472	24.65%	2.475%
11	9.657	1110	1117	1131	rBV	321191	541024	21.25%	2.134%
12	10.198	1202	1209	1230	rBV	450587	832645	32.71%	3.285%
13	10.563	1263	1271	1284	rVB	476437	774951	30.44%	3.057%
14	10.716	1290	1297	1315	rBV	416147	799645	31.41%	3.154%
15	11.728	1464	1469	1470	rBV5	2963	4154	0.16%	0.016%
16	11.745	1470	1472	1478	rVV7	3369	6227	0.24%	0.025%
17	11.798	1478	1481	1488	rVB7	2309	5177	0.20%	0.020%
18	12.181	1541	1546	1555	rBV6	5853	11429	0.45%	0.045%
19	13.316	1734	1739	1746	rVB4	7664	12234	0.48%	0.048%
20	13.698	1799	1804	1806	rBV6	1942	3153	0.12%	0.012%
21	13.839	1819	1828	1838	rBV	1000773	1400931	55.03%	5.526%
22	14.110	1867	1874	1888	rBV2	1038063	1518271	59.64%	5.989%
23	14.416	1919	1926	1936	rBV	820488	1199749	47.13%	4.733%
24	14.669	1963	1969	1990	rBV	210382	485136	19.06%	1.914%
25	15.416	2084	2096	2107	rBV	1377866	2008240	78.89%	7.922%
26	15.557	2114	2120	2133	rBV	385252	559977	22.00%	2.209%
27	15.663	2134	2138	2144	rVB5	7188	11677	0.46%	0.046%
28	16.204	2226	2230	2236	rVB8	5647	7881	0.31%	0.031%
29	16.633	2300	2303	2308	rBV7	4383	6670	0.26%	0.026%
30	16.857	2337	2341	2344	rBV6	4058	6212	0.24%	0.025%
31	16.975	2355	2361	2364	rBV4	3053	5745	0.23%	0.023%
32	17.180	2389	2396	2405	rBV	1081050	1539484	60.47%	6.073%
33	17.280	2406	2413	2425	rVV	1468201	2172085	85.32%	8.568%
34	17.769	2493	2496	2498	rBV4	2033	2784	0.11%	0.011%
35	19.104	2718	2723	2729	rBV2	22885	36360	1.43%	0.143%
36	19.174	2732	2735	2740	rBV	18443	23896	0.94%	0.094%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011924\
Data File : BP019397.D
Acq On : 19 Jan 2024 09:54
Operator : MA/JU
Sample : PB158500BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK500

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Title : SVOA CALIBRATION

37	19.527	2789	2795	2804	rBV	1929132	2545730	100.00%	10.042%
38	21.286	3089	3094	3102	rBV	1125384	1406853	55.26%	5.550%
39	23.492	3462	3469	3482	rVB	962619	1923317	75.55%	7.587%
40	23.639	3488	3494	3504	rVB	609494	1237512	48.61%	4.882%




Sum of corrected areas: 25350631

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011924\
Data File : BP019397.D
Acq On : 19 Jan 2024 09:54
Operator : MA/JU
Sample : PB158500BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK500

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

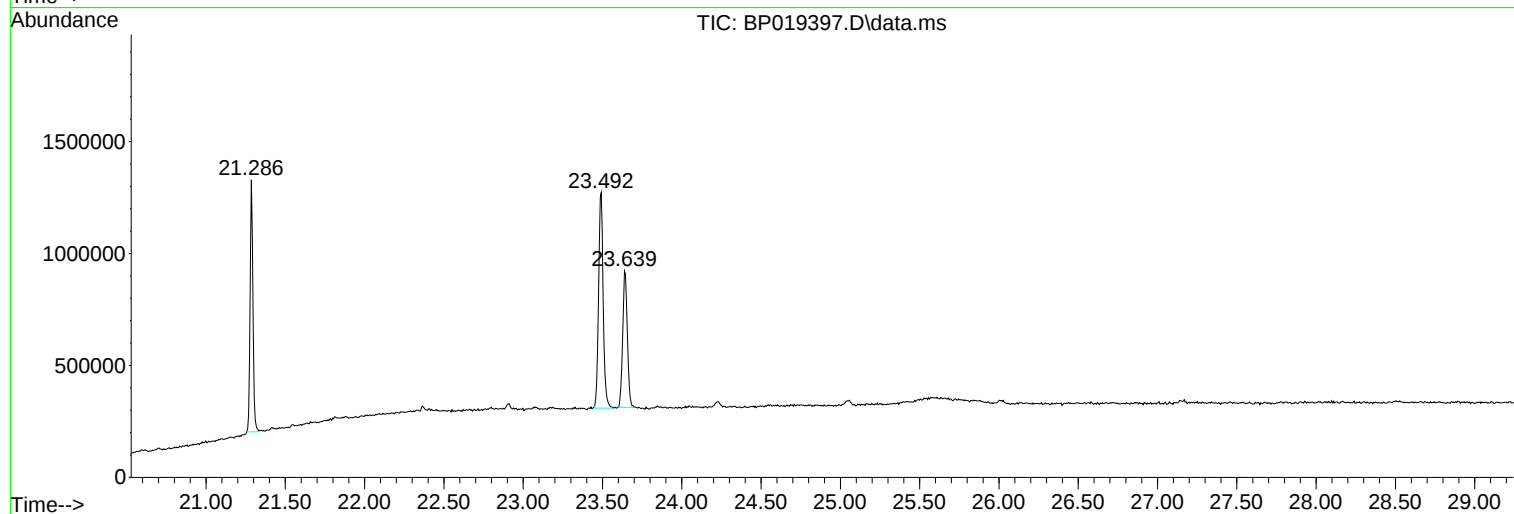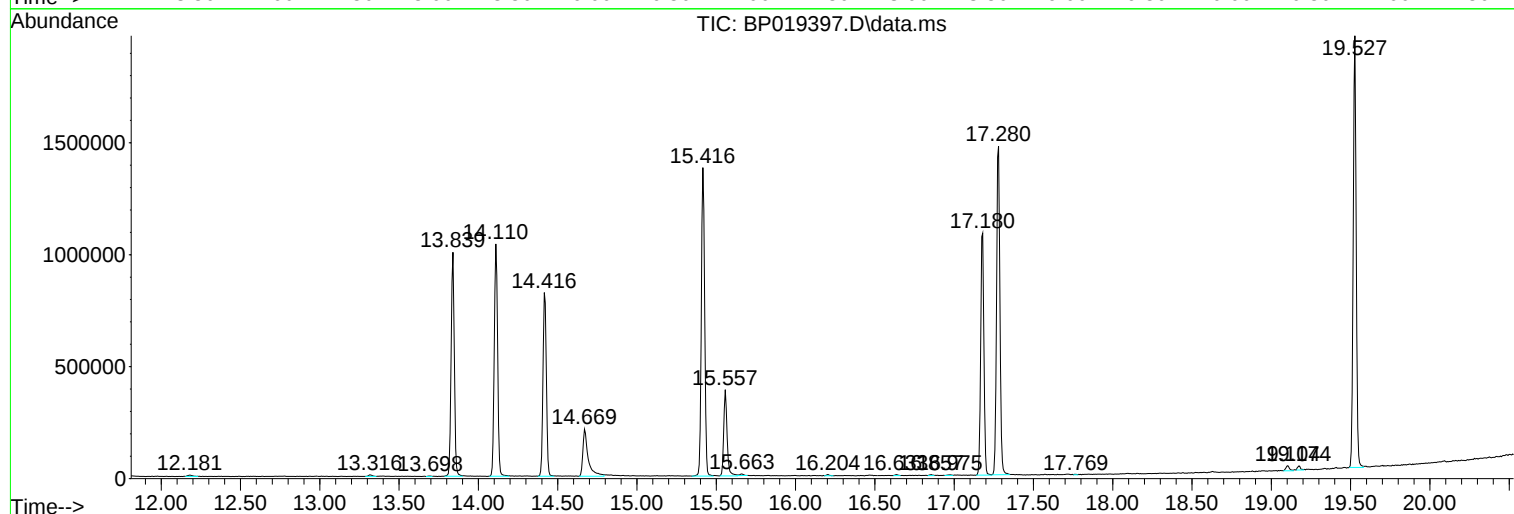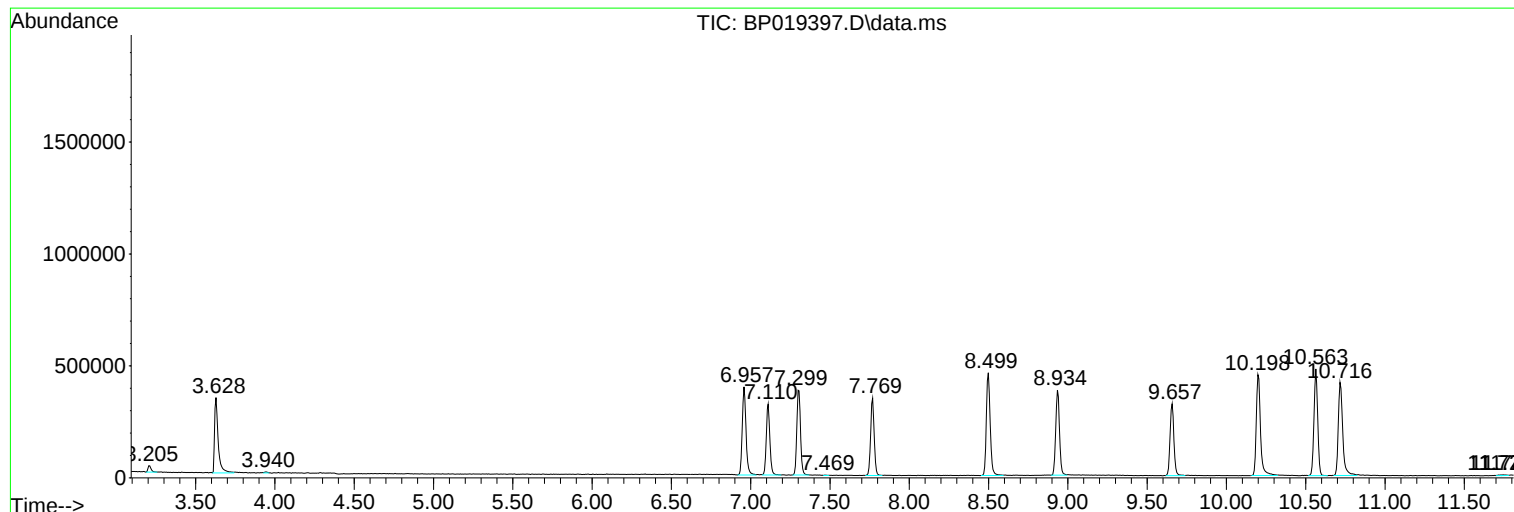

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011924\
Data File : BP019397.D
Acq On : 19 Jan 2024 09:54
Operator : MA/JU
Sample : PB158500BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK500

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011924\
Data File : BP019397.D
Acq On : 19 Jan 2024 09:54
Operator : MA/JU
Sample : PB158500BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK500

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc