
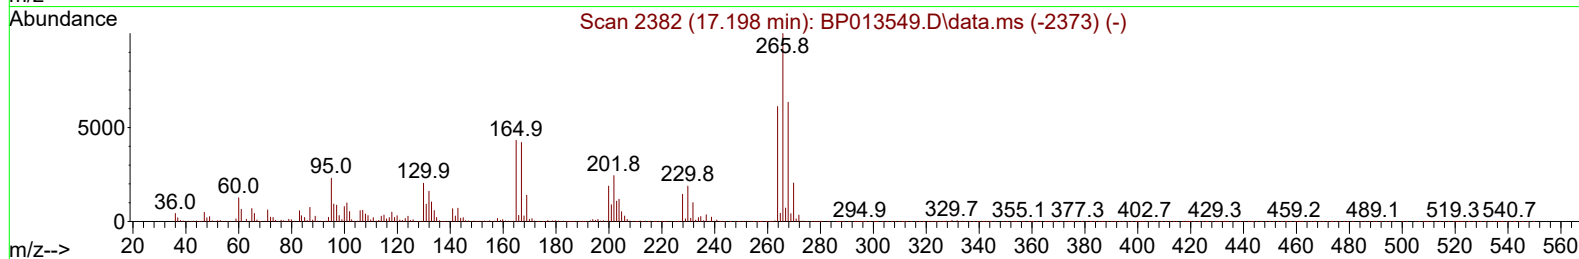
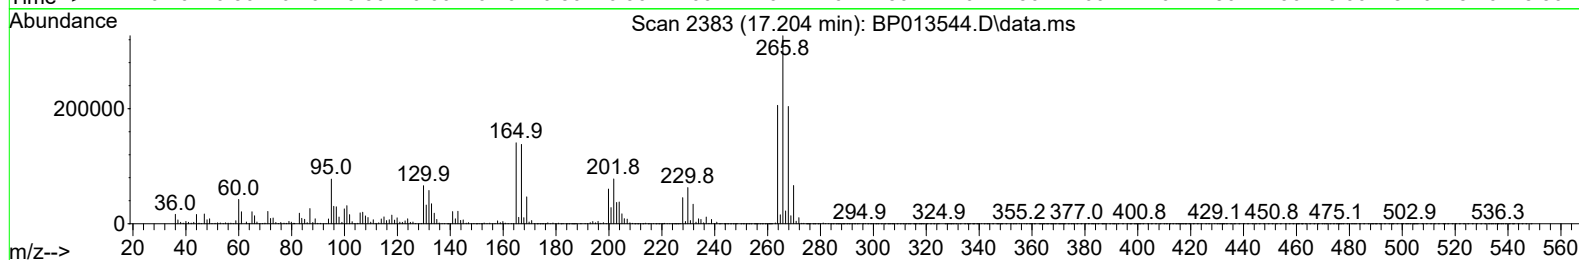


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012323\
Data File : BP013544.D
Acq On : 23 Jan 2023 10:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 06:33:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 24 04:44:15 2023
Response via : Initial Calibration

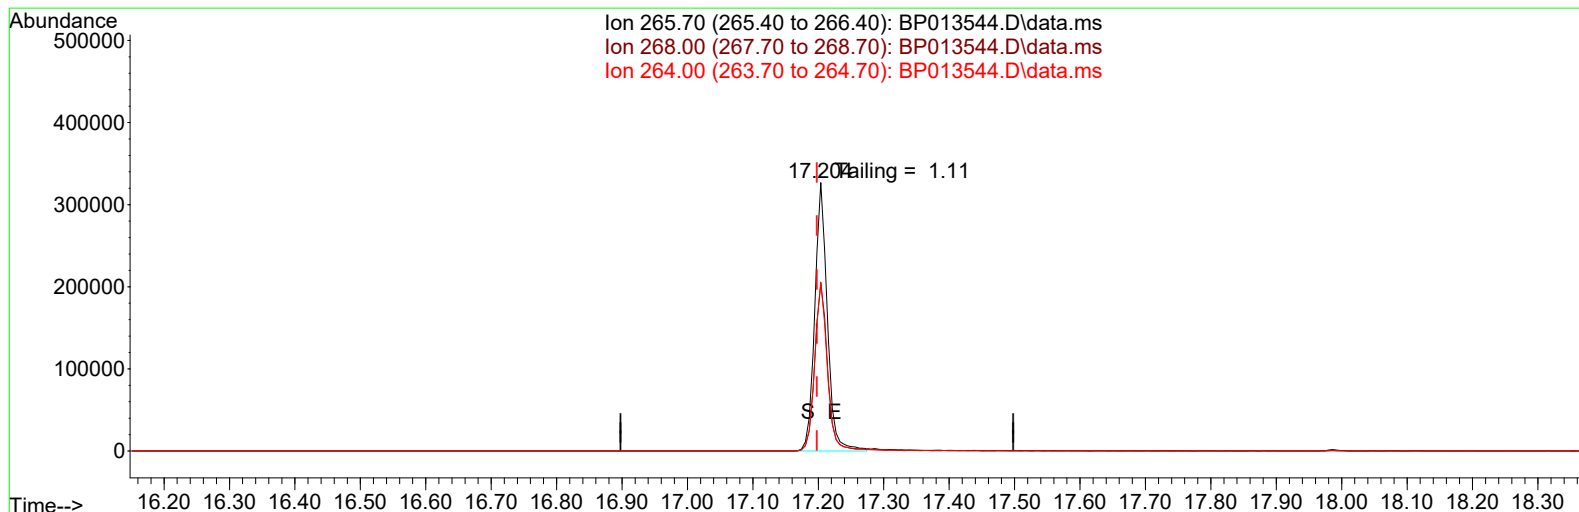

TIC: BP013544.D\data.ms

(70) Pentachlorophenol (C)




17.204min (+ 0.006) 143380.43 ng

response 446504

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.40	62.40
264.00	61.10	62.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012323\
 Data File : BP013544.D
 Acq On : 23 Jan 2023 10:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 06:33:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 24 04:44:15 2023
 Response via : Initial Calibration

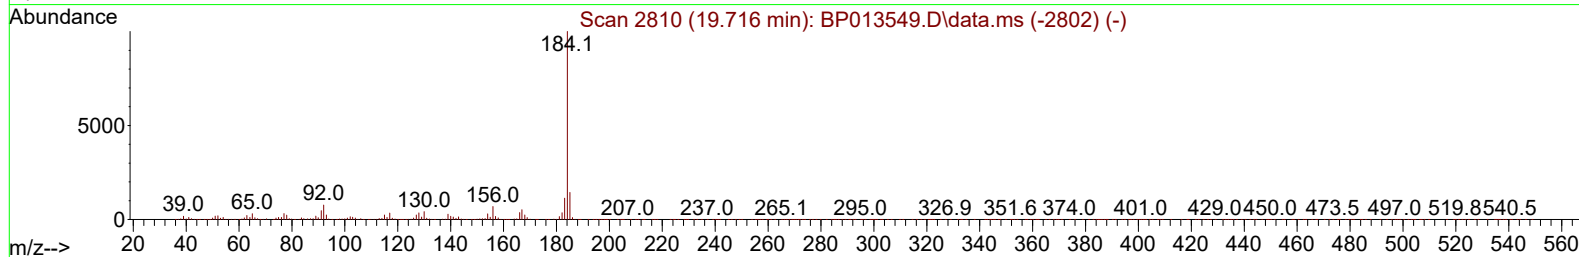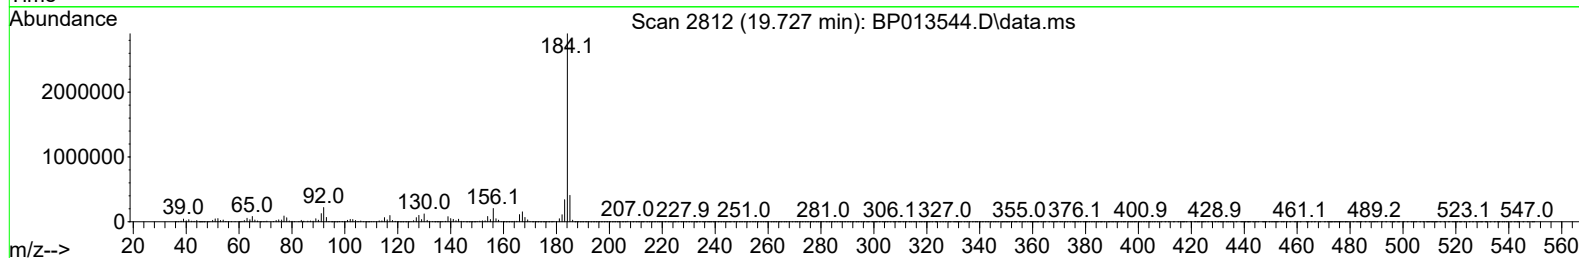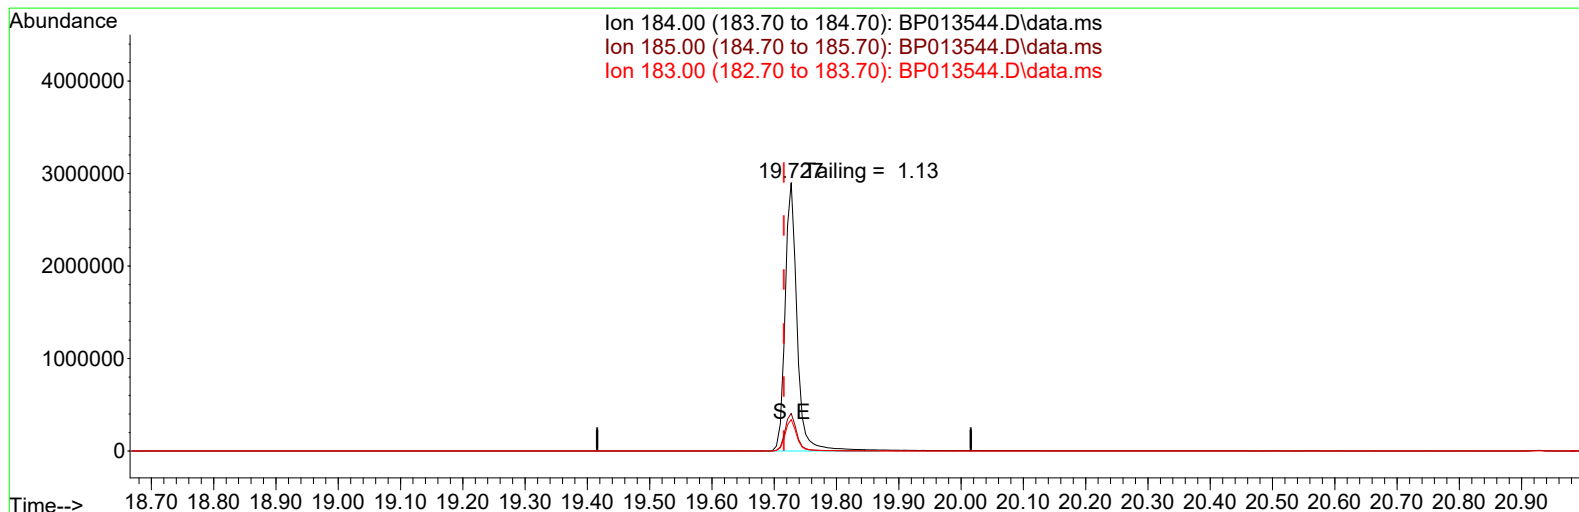

TIC: BP013544.D\data.ms

(77) Benzidine**19.727min (+ 0.011) 235734.26 ng****response 3930835**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.04
183.00	11.30	11.74
0.00	0.00	0.00