

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012323\
 Data File : BP013554.D
 Acq On : 23 Jan 2023 19:14
 Operator : CG/JU
 Sample : PB150389BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB150389BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012323.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP013554.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	3	7	12	rVB	149264	163598	1.09%	0.194%
2	5.222	339	346	359	rBV	2586102	3680646	24.47%	4.367%
3	5.693	416	426	441	rBV	6762631	9924655	65.98%	11.776%
4	7.305	692	700	712	rBV	6177223	10035570	66.71%	11.908%
5	8.163	838	846	854	rVB	1193159	1875667	12.47%	2.226%
6	9.334	1036	1045	1056	rBV	3723756	6166474	40.99%	7.317%
7	10.993	1318	1327	1337	rBV	1621896	2689912	17.88%	3.192%
8	13.428	1733	1741	1748	rBV	9439018	14084677	93.63%	16.713%
9	14.798	1967	1974	1981	rBV	2236106	3268572	21.73%	3.878%
10	16.281	2219	2226	2246	rBV	5957050	8524602	56.67%	10.115%
11	17.551	2435	2442	2453	rBV	2539514	3469478	23.06%	4.117%
12	20.080	2867	2872	2878	rBV	12252025	15042769	100.00%	17.849%
13	21.627	3129	3135	3145	rVB	2111528	2791860	18.56%	3.313%
14	24.216	3568	3575	3589	rVB2	1211651	2557325	17.00%	3.034%




Sum of corrected areas: 84275805

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012323\
Data File : BP013554.D
Acq On : 23 Jan 2023 19:14
Operator : CG/JU
Sample : PB150389BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB150389BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

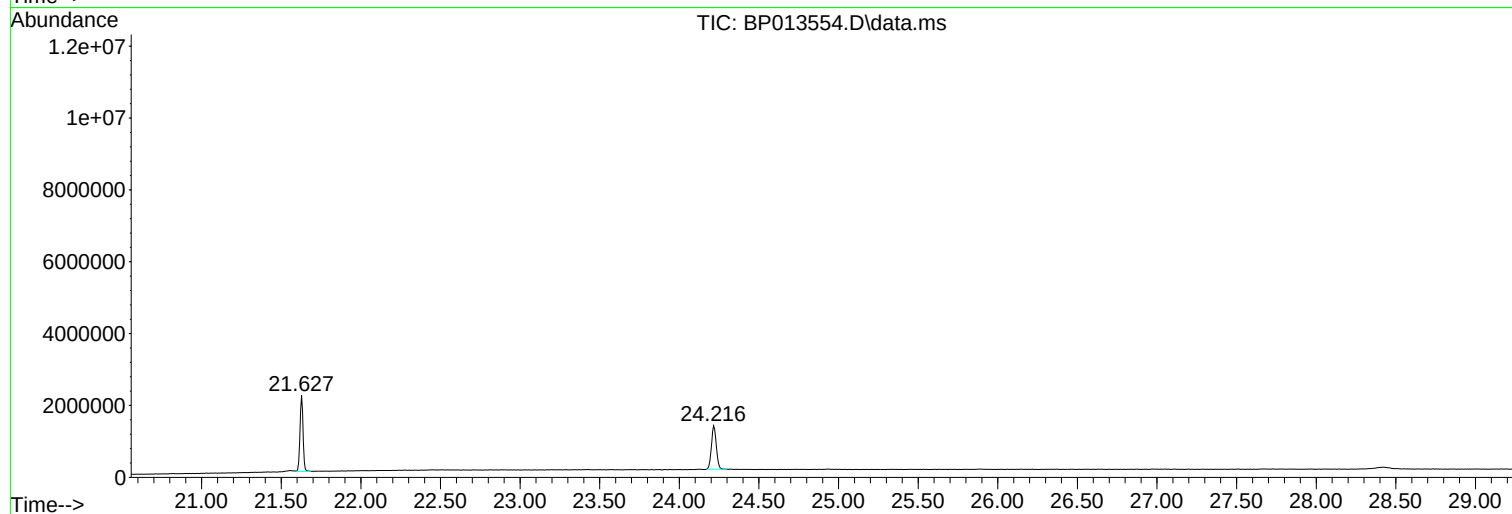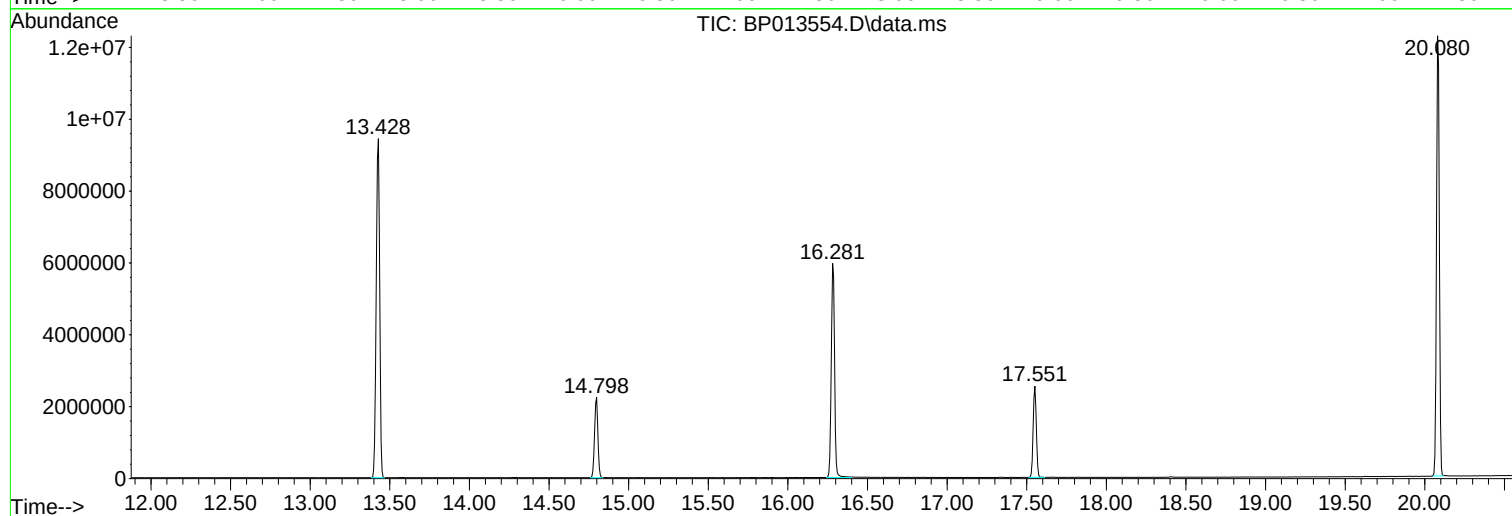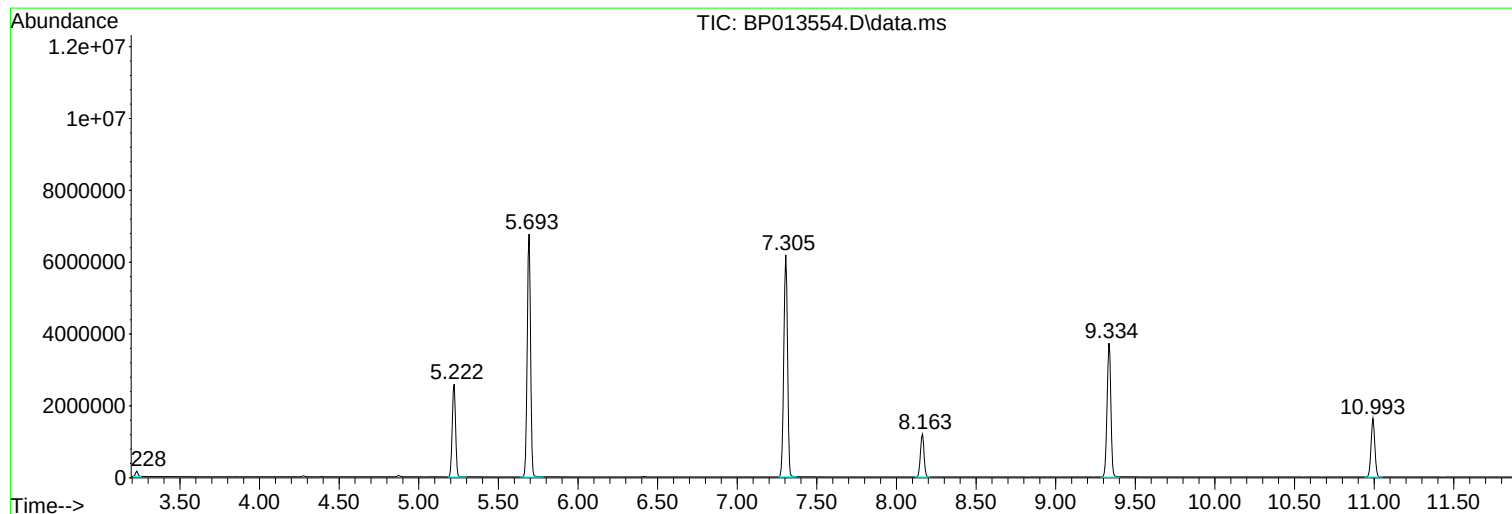

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012323\
Data File : BP013554.D
Acq On : 23 Jan 2023 19:14
Operator : CG/JU
Sample : PB150389BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB150389BL









Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.222	39.25 ng	3680650	1,4-Dichlorobenzene-d4	8.163

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	83		
2	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	36		
3	t-Butyl nitrite	103	C4H9NO2	000540-80-7	36		
4	Acetone	58	C3H6O	000067-64-1	27		
5	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	12		

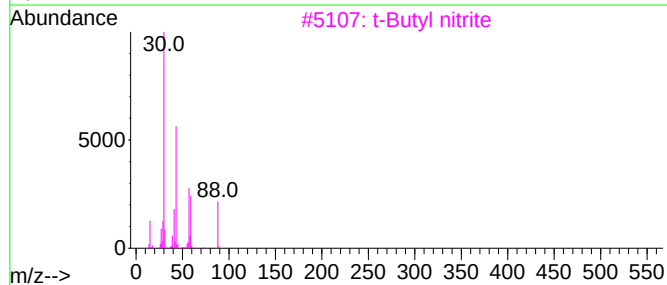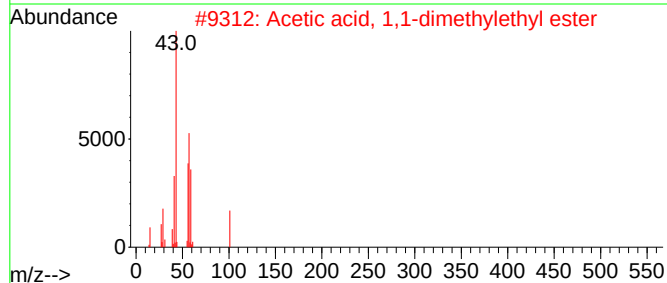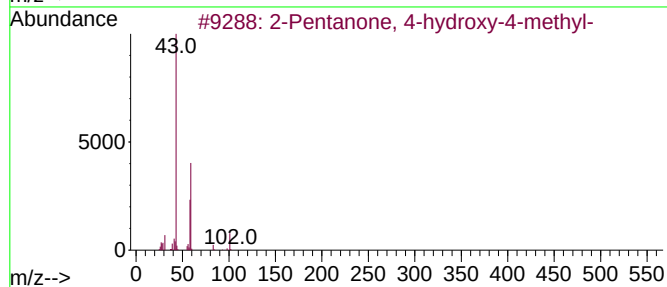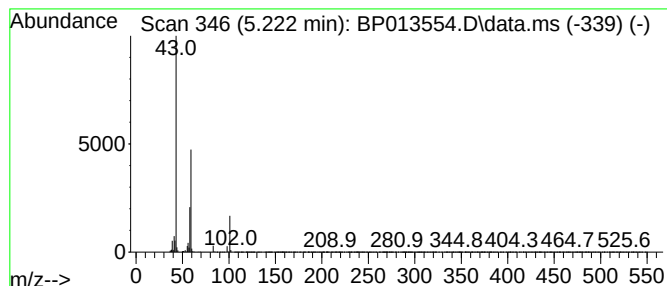

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012323\
Data File : BP013554.D
Acq On : 23 Jan 2023 19:14
Operator : CG/JU
Sample : PB150389BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB150389BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.222	39.3	ng	3680650	1	8.163	1875670	20.0