

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012323\
 Data File : BP013555.D
 Acq On : 23 Jan 2023 19:48
 Operator : CG/JU
 Sample : PB150341BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB150341BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012323.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP013555.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.222	339	346	354	rBV	2257057	3182194	22.57%	4.239%
2	5.693	417	426	444	rBV	5934638	8650481	61.34%	11.523%
3	7.305	688	700	711	rBV	5495729	8807818	62.46%	11.733%
4	8.163	835	846	854	rBV	1083683	1719490	12.19%	2.290%
5	9.334	1036	1045	1061	rBV	3258958	5311258	37.66%	7.075%
6	10.993	1318	1327	1335	rBV	1401104	2342058	16.61%	3.120%
7	13.428	1733	1741	1749	rBV	8343582	12403770	87.96%	16.523%
8	14.798	1967	1974	1981	rBV	1913497	2850221	20.21%	3.797%
9	16.281	2219	2226	2250	rBV	5387020	7607841	53.95%	10.134%
10	17.551	2435	2442	2452	rBV	2218242	3112637	22.07%	4.146%
11	20.080	2867	2872	2878	rBV	11487964	14101989	100.00%	18.785%
12	21.627	3129	3135	3144	rBV	1931547	2589908	18.37%	3.450%
13	24.221	3568	3576	3585	rBV2	1111584	2391379	16.96%	3.185%




Sum of corrected areas: 75071044

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012323\
Data File : BP013555.D
Acq On : 23 Jan 2023 19:48
Operator : CG/JU
Sample : PB150341BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB150341BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

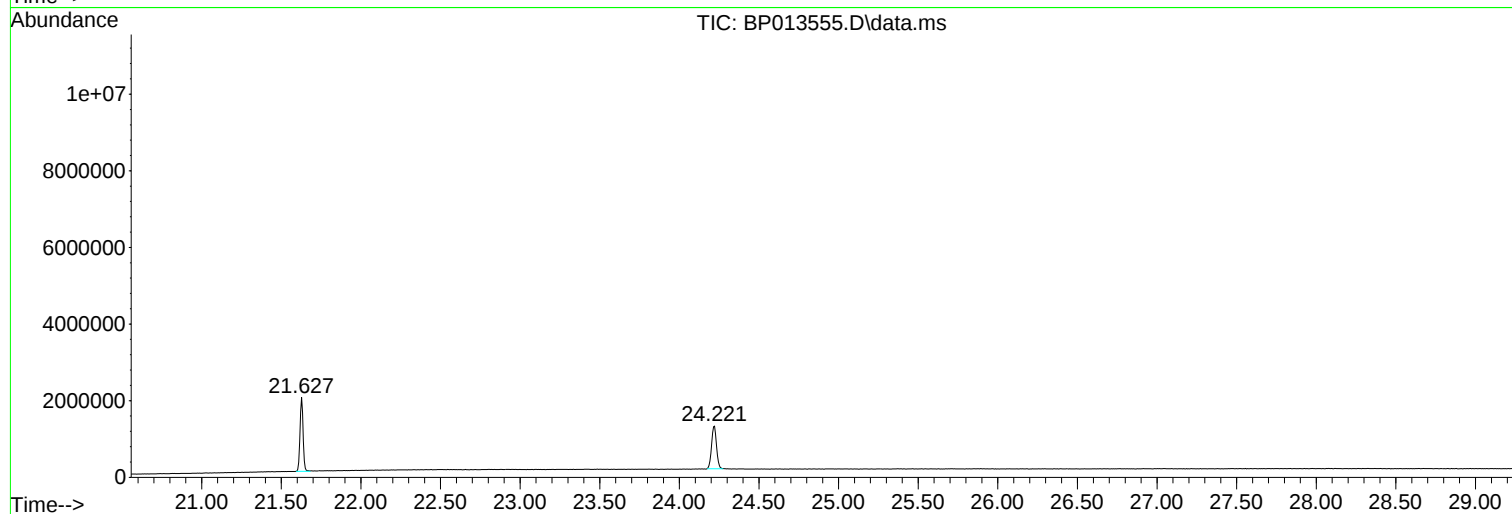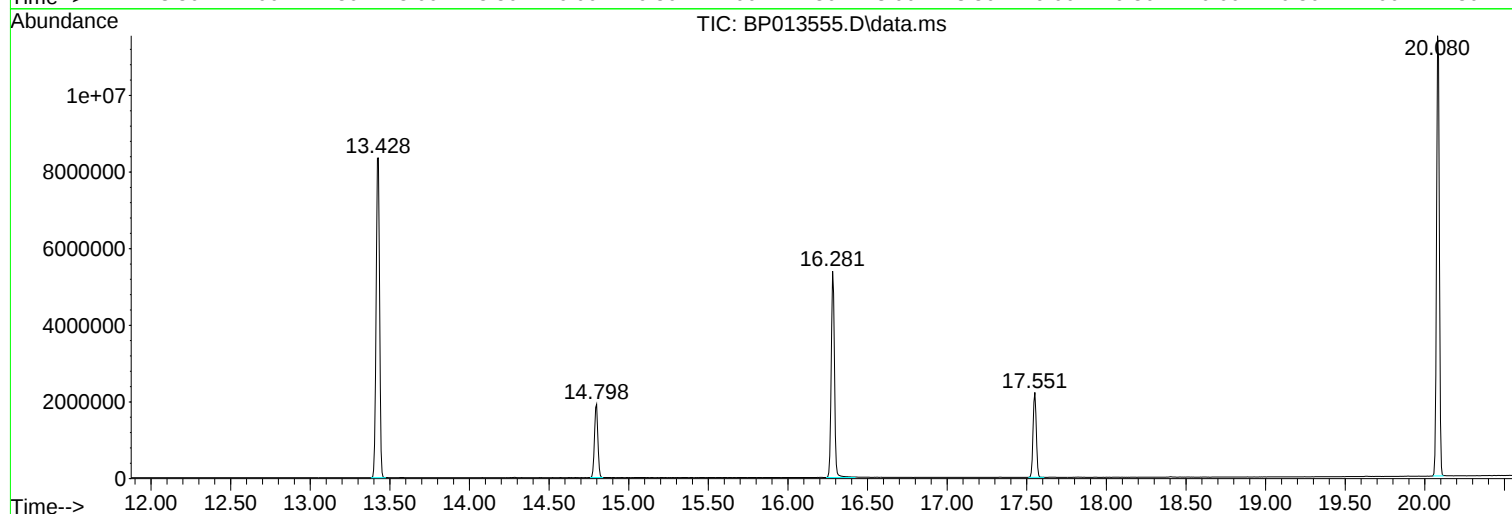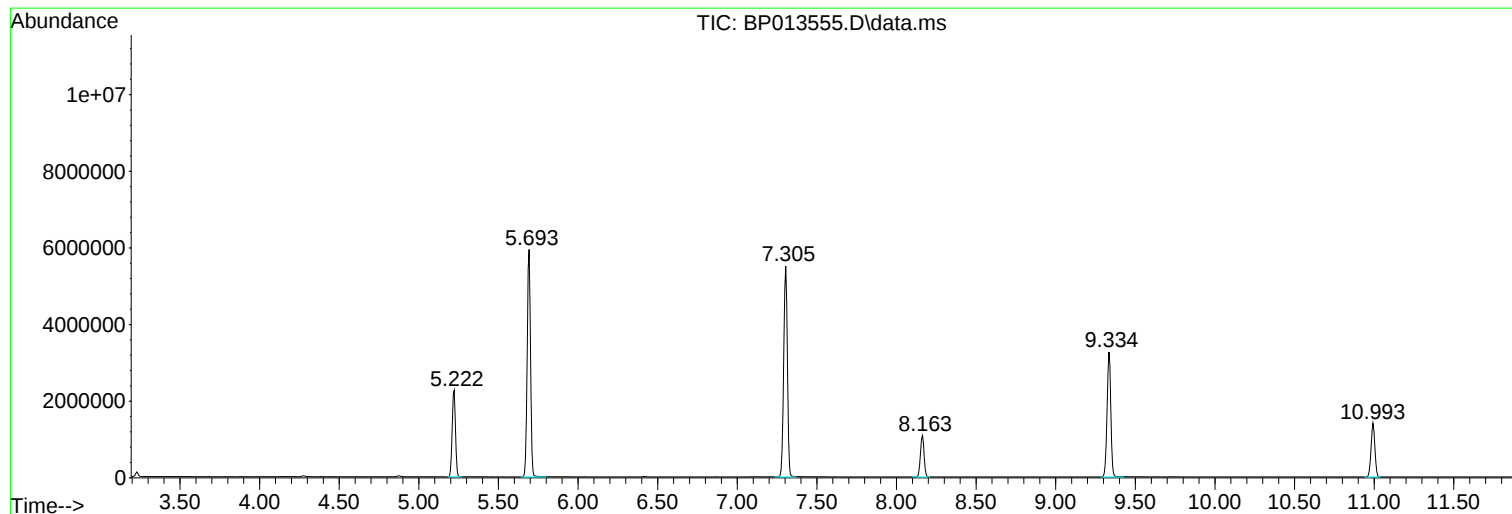

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012323\
Data File : BP013555.D
Acq On : 23 Jan 2023 19:48
Operator : CG/JU
Sample : PB150341BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB150341BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.222	37.01 ng	3182190	1,4-Dichlorobenzene-d4	8.163

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	83		
2	t-Butyl nitrite	103	C4H9NO2	000540-80-7	36		
3	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	36		
4	Acetone	58	C3H6O	000067-64-1	27		
5	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	12		

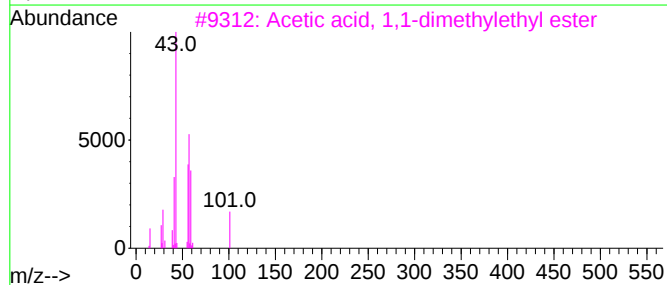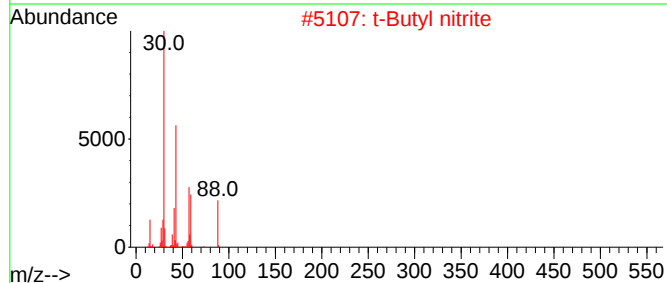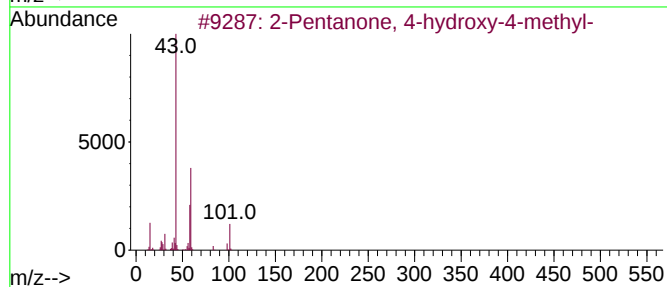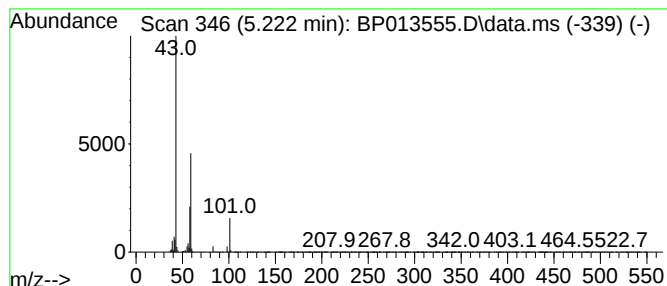

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012323\
Data File : BP013555.D
Acq On : 23 Jan 2023 19:48
Operator : CG/JU
Sample : PB150341BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB150341BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.222	37.0	ng	3182190	1	8.163	1719490	20.0