

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012323\
 Data File : BP013558.D
 Acq On : 23 Jan 2023 21:30
 Operator : CG/JU
 Sample : PB150338BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB150338BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012323.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP013558.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	3	7	12	rVB	115446	129475	1.05%	0.180%
2	5.217	339	345	355	rBV	2328407	3388154	27.38%	4.719%
3	5.693	419	426	439	rBV	6206617	9041418	73.05%	12.592%
4	7.305	691	700	720	rBV	5587143	8971683	72.49%	12.494%
5	8.163	838	846	854	rBV	1173510	1862292	15.05%	2.594%
6	9.334	1036	1045	1057	rBV	3462592	5574852	45.04%	7.764%
7	10.993	1319	1327	1337	rVB	1458232	2446738	19.77%	3.407%
8	13.422	1732	1740	1750	rBV	8518490	12376750	100.00%	17.236%
9	14.793	1967	1973	1981	rBV	1872697	2789367	22.54%	3.885%
10	16.281	2218	2226	2245	rBV	4861840	6941413	56.08%	9.667%
11	17.551	2435	2442	2451	rBV	1924695	2765952	22.35%	3.852%
12	20.081	2866	2872	2883	rBV	9646682	11220638	90.66%	15.626%
13	21.627	3130	3135	3144	rBV	1629884	2102260	16.99%	2.928%
14	24.216	3568	3575	3587	rVB2	1036744	2194720	17.73%	3.056%




Sum of corrected areas: 71805712

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012323\
Data File : BP013558.D
Acq On : 23 Jan 2023 21:30
Operator : CG/JU
Sample : PB150338BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB150338BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

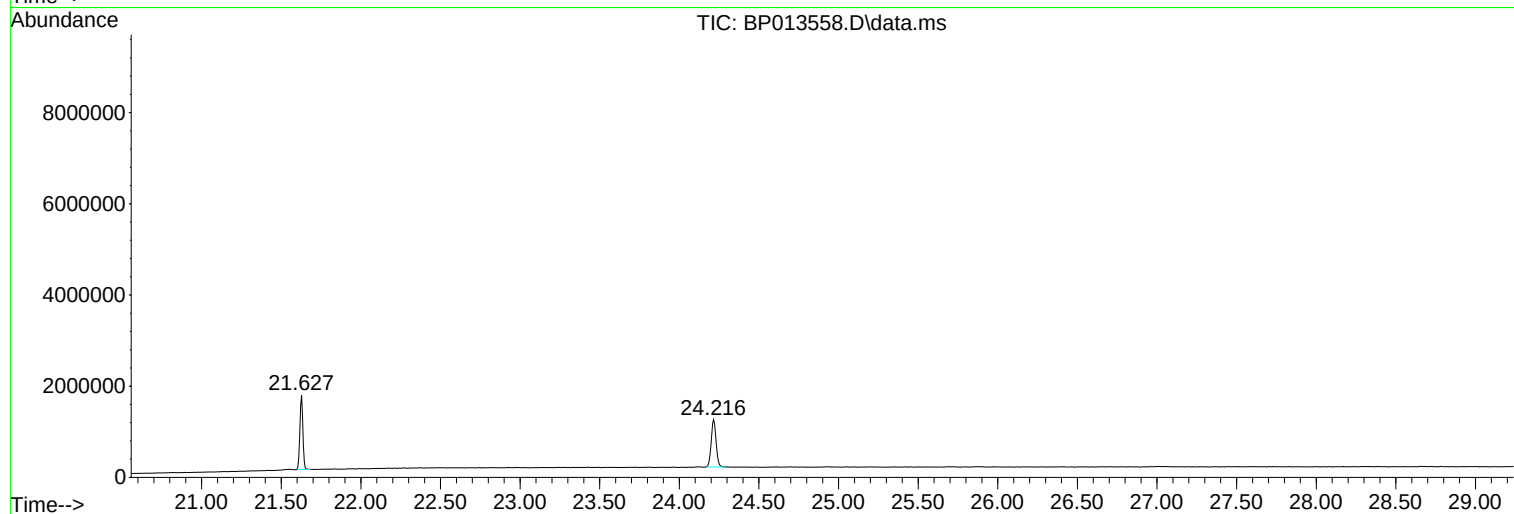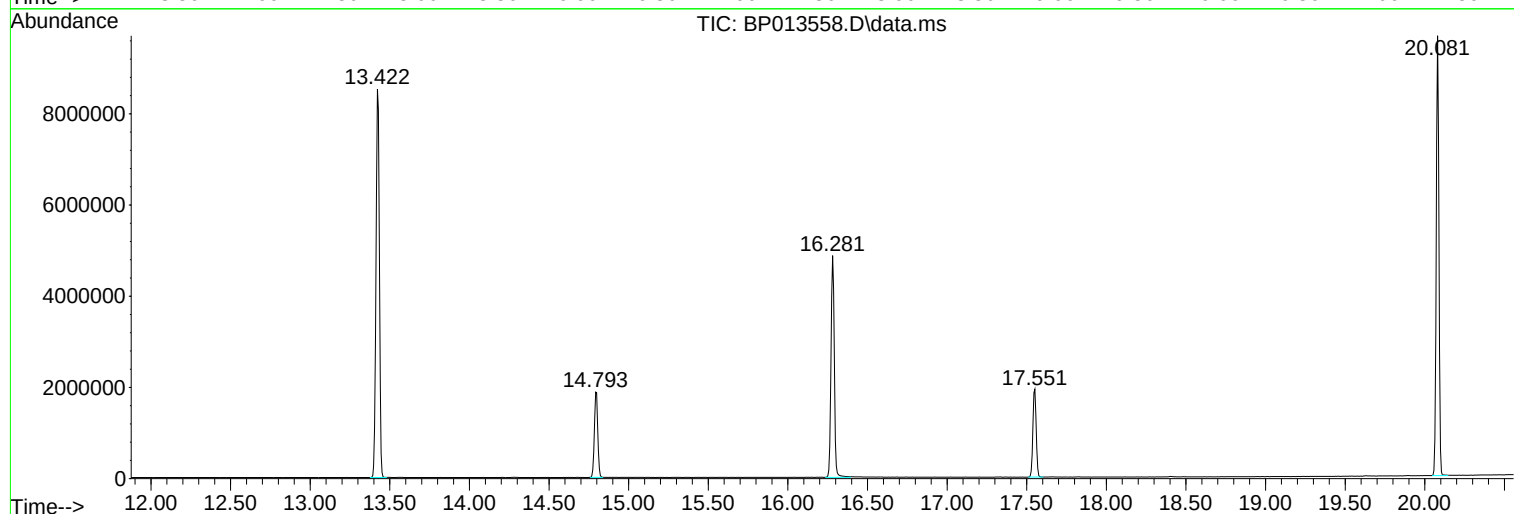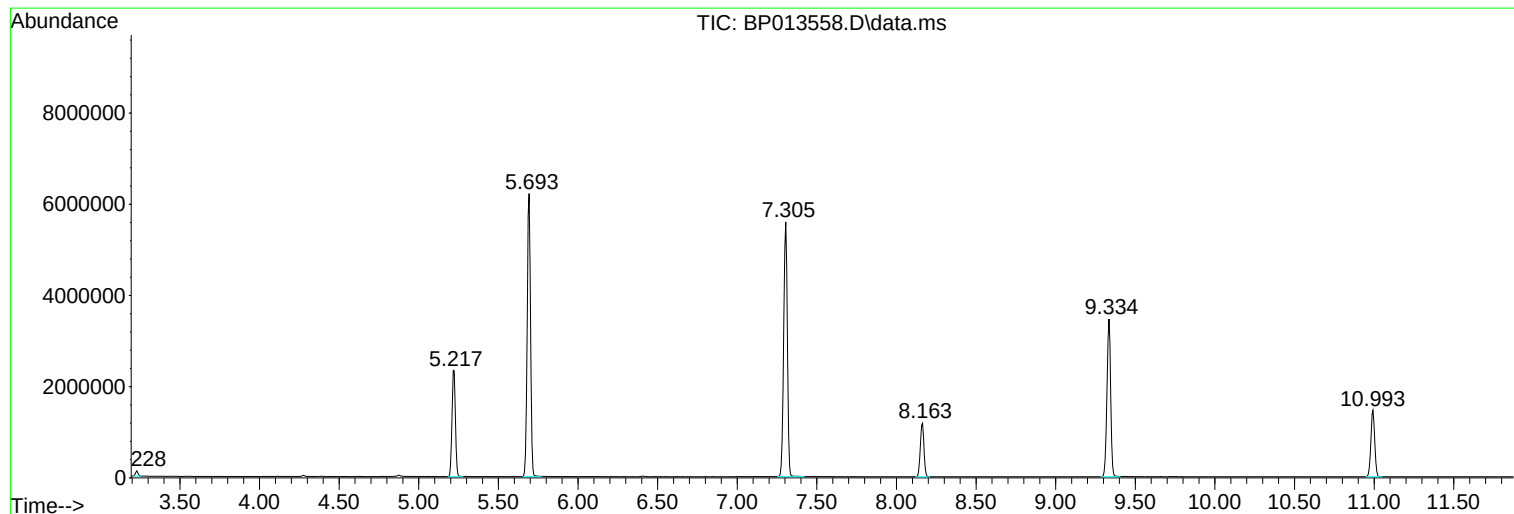

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012323\
Data File : BP013558.D
Acq On : 23 Jan 2023 21:30
Operator : CG/JU
Sample : PB150338BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB150338BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.217	36.39 ng	3388150	1,4-Dichlorobenzene-d4	8.163

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	83
2			Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	36
3			Acetone	58	C3H6O	000067-64-1	27
4			1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	16
5			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	12

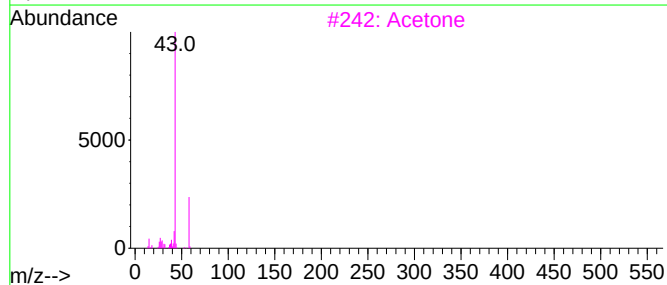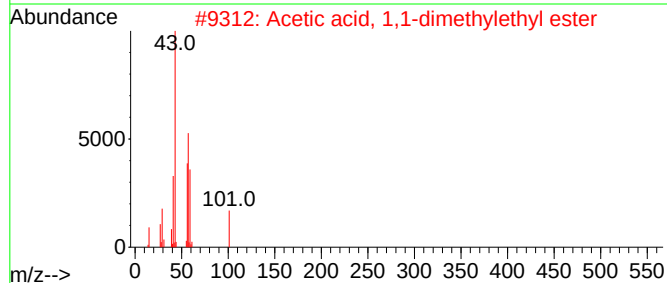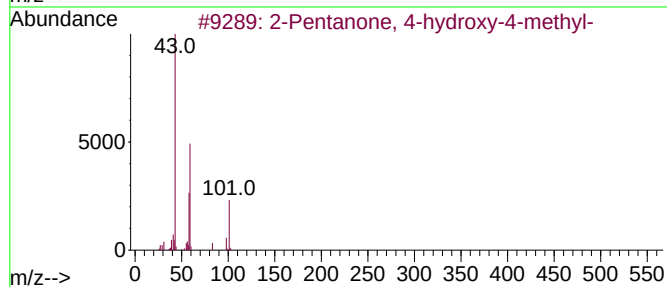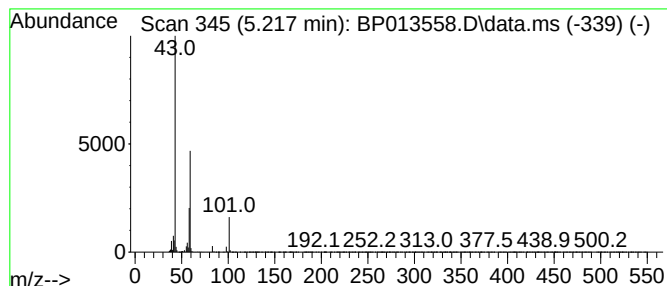

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012323\
Data File : BP013558.D
Acq On : 23 Jan 2023 21:30
Operator : CG/JU
Sample : PB150338BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB150338BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.217	36.4	ng	3388150	1	8.163	1862290	20.0