

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012725\
 Data File : BP023744.D
 Acq On : 27 Jan 2025 17:12
 Operator : RC/JU
 Sample : Q1174-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E2935

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023744.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	33	36	45	rVB	125673	157795	0.85%	0.099%
2	3.717	102	107	120	rBV	442493	723413	3.89%	0.454%
3	4.034	157	161	166	rBV	32228	41880	0.23%	0.026%
4	4.128	174	177	182	rVB2	34301	43967	0.24%	0.028%
5	4.481	233	237	242	rBV2	16626	24727	0.13%	0.016%
6	4.940	311	315	321	rBV2	23547	35094	0.19%	0.022%
7	6.193	524	528	540	rVB	31835	54657	0.29%	0.034%
8	6.975	652	661	672	rBV	667470	1057505	5.68%	0.663%
9	7.122	678	686	697	rBV	2074082	3085921	16.59%	1.935%
10	7.334	715	722	733	rBV	2249883	3463488	18.61%	2.172%
11	7.422	735	737	747	rVB9	11312	18901	0.10%	0.012%
12	7.793	792	800	807	rBV	2022694	3115842	16.75%	1.954%
13	8.216	866	872	877	rBV	19230	31821	0.17%	0.020%
14	8.499	912	920	931	rBV	2088005	3209512	17.25%	2.013%
15	8.934	987	994	1004	rBV	2316447	3709306	19.94%	2.326%
16	9.387	1066	1071	1078	rVB2	34028	53375	0.29%	0.033%
17	9.504	1086	1091	1097	rVB9	10666	19748	0.11%	0.012%
18	9.657	1107	1117	1125	rBV	1794795	3104913	16.69%	1.947%
19	10.204	1202	1210	1224	rBV	3195661	5123074	27.53%	3.213%
20	10.575	1256	1273	1281	rBV	2650387	4713384	25.33%	2.956%
21	10.704	1285	1295	1315	rBV	2584832	4394942	23.62%	2.756%
22	11.881	1490	1495	1498	rBV2	26799	41108	0.22%	0.026%
23	11.922	1498	1502	1509	rVB	47345	77312	0.42%	0.048%
24	12.157	1537	1542	1551	rVB2	54553	89464	0.48%	0.056%
25	12.610	1613	1619	1627	rBV3	33814	56100	0.30%	0.035%
26	13.387	1745	1751	1756	rVB5	10466	20733	0.11%	0.013%
27	13.822	1818	1825	1831	rBV	6317931	8150756	43.81%	5.112%
28	13.875	1831	1834	1840	rVB4	33276	56717	0.30%	0.036%
29	14.110	1866	1874	1887	rBV	6645242	9936353	53.40%	6.231%
30	14.422	1918	1927	1936	rBV	4157015	6656218	35.77%	4.174%
31	14.645	1959	1965	1973	rBV	702654	1025912	5.51%	0.643%
32	14.845	1994	1999	2003	rBV8	14216	23987	0.13%	0.015%
33	14.969	2013	2020	2029	rBV	78681	143851	0.77%	0.090%
34	15.428	2091	2098	2110	rBV	8717314	12731975	68.43%	7.985%
35	15.539	2111	2117	2132	rVV	3056774	3834350	20.61%	2.405%
36	15.669	2135	2139	2145	rVB2	45378	74376	0.40%	0.047%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012725\
Data File : BP023744.D
Acq On : 27 Jan 2025 17:12
Operator : RC/JU
Sample : Q1174-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2935

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
Title : SVOA CALIBRATION

37	15.798	2156	2161	2168	rBV	134226	191824	1.03%	0.120%
38	15.875	2171	2174	2177	rVB4	15090	19444	0.10%	0.012%
39	16.739	2319	2321	2326	rVB4	20168	25817	0.14%	0.016%
40	17.222	2396	2403	2413	rBV2	5493607	8063479	43.34%	5.057%
41	17.322	2413	2420	2432	rVV2	10060913	14711617	79.07%	9.226%
42	18.169	2560	2564	2573	rBV2	207054	405750	2.18%	0.254%
43	19.245	2744	2747	2754	rVB2	132967	188763	1.01%	0.118%
44	19.316	2756	2759	2766	rVV	140153	185965	1.00%	0.117%
45	19.498	2787	2790	2797	rBV3	129800	203893	1.10%	0.128%
46	19.698	2818	2824	2832	rVB	12518817	17804979	95.69%	11.166%
47	21.310	3094	3098	3103	rVB	519974	662194	3.56%	0.415%
48	21.680	3155	3161	3170	rVB	6031716	9172735	49.30%	5.753%
49	24.857	3691	3701	3715	rVB	6415060	18606047	100.00%	11.668%
50	25.092	3732	3741	3754	rVB2	3473097	10111381	54.34%	6.341%




Sum of corrected areas: 159456365

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012725\
Data File : BP023744.D
Acq On : 27 Jan 2025 17:12
Operator : RC/JU
Sample : Q1174-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2935

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

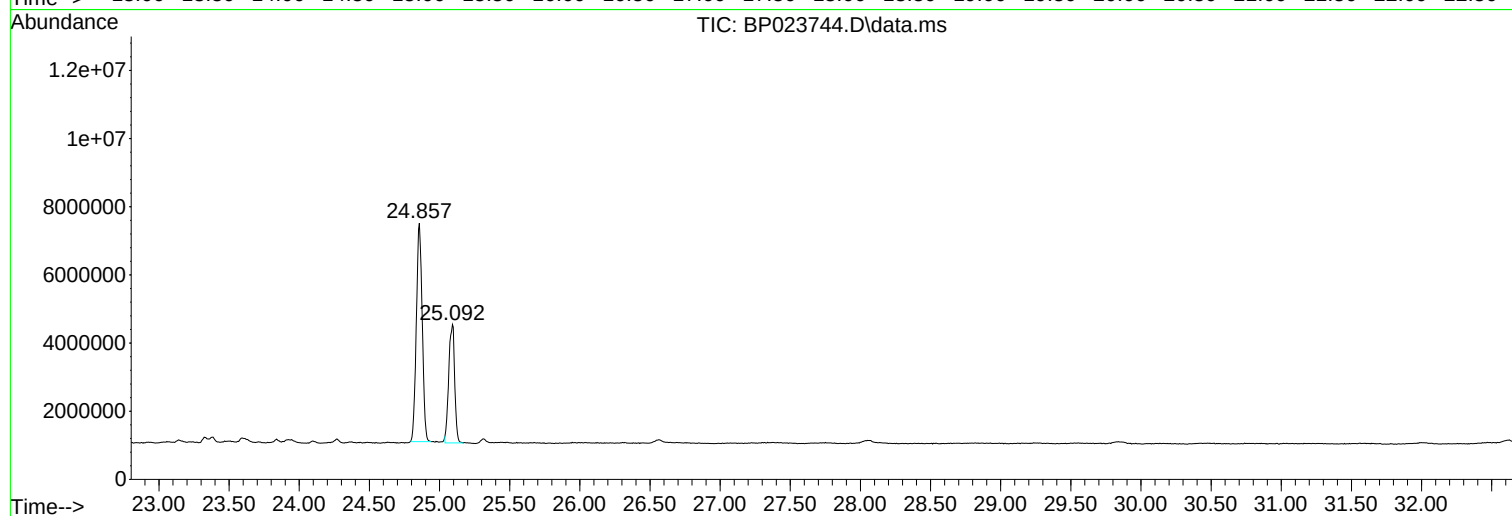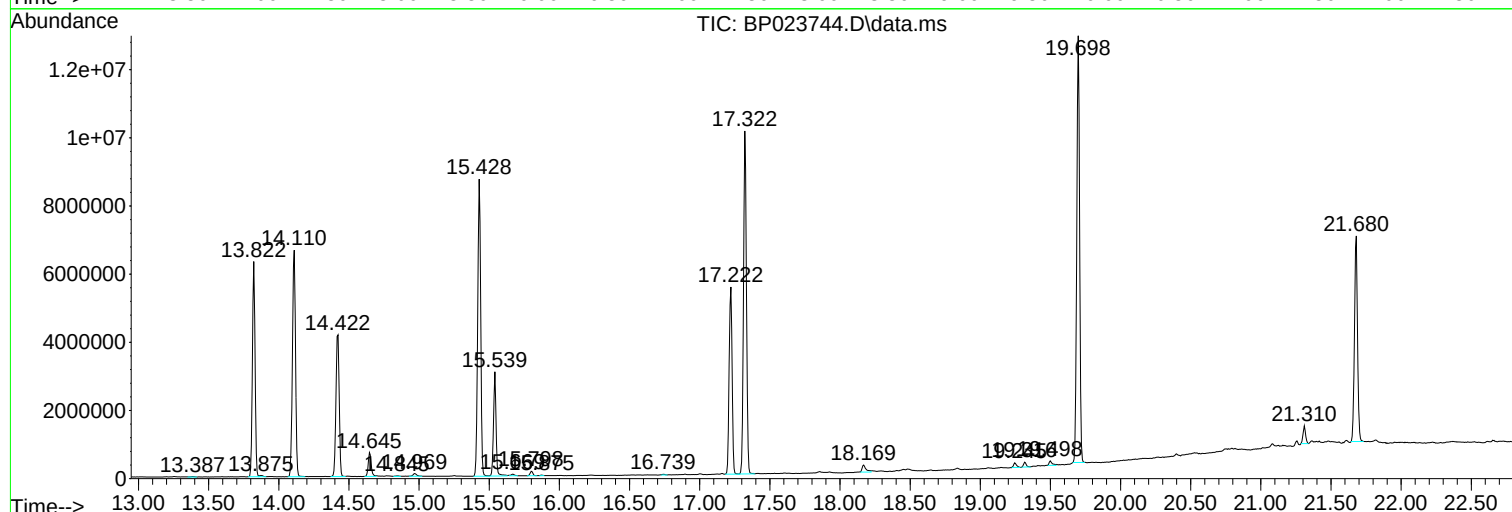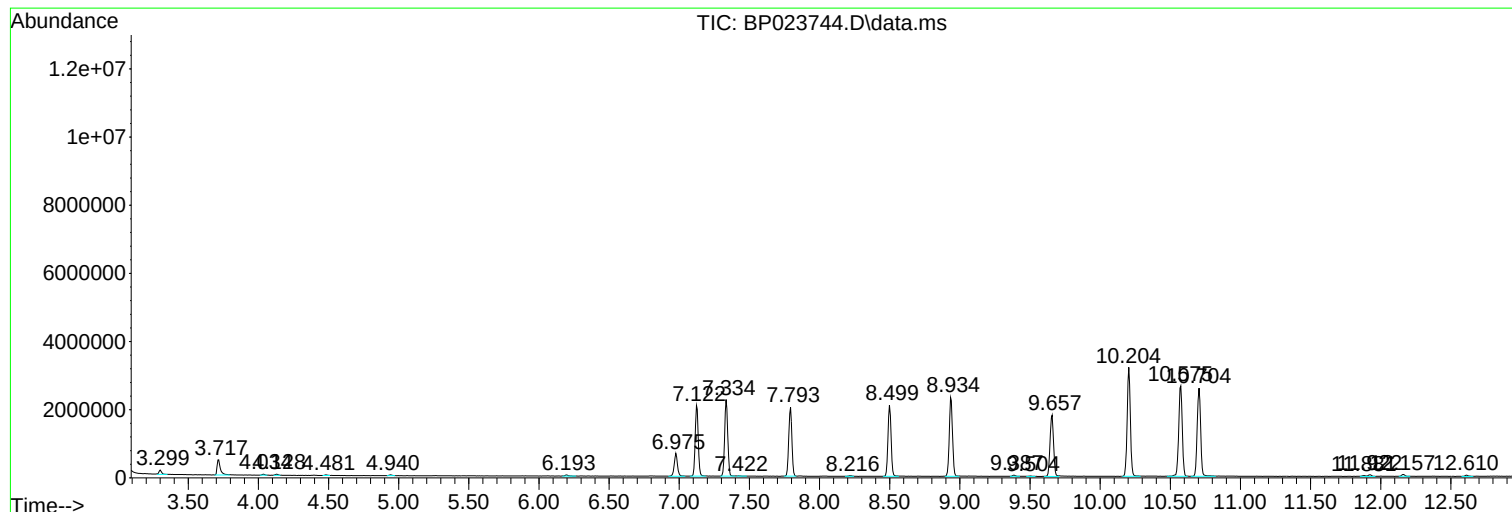

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012725\
Data File : BP023744.D
Acq On : 27 Jan 2025 17:12
Operator : RC/JU
Sample : Q1174-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2935

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012725\
Data File : BP023744.D
Acq On : 27 Jan 2025 17:12
Operator : RC/JU
Sample : Q1174-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2935

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------