

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012725\
 Data File : BP023749.D
 Acq On : 27 Jan 2025 21:16
 Operator : RC/JU
 Sample : PB166248BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK248

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023749.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	32	36	43	rVB	148562	189240	1.27%	0.137%
2	3.711	102	106	133	rBV	1621134	2804347	18.77%	2.037%
3	4.034	157	161	165	rBV	22420	29302	0.20%	0.021%
4	5.005	320	326	327	rBV6	9136	16088	0.11%	0.012%
5	6.975	653	661	674	rBV	2233485	3599303	24.09%	2.615%
6	7.122	679	686	698	rVV	1786386	2678392	17.93%	1.946%
7	7.334	714	722	732	rBV	2305043	3626904	24.28%	2.635%
8	7.787	791	799	807	rBV	1604638	2540388	17.00%	1.845%
9	8.499	906	920	934	rBV	2957689	4679067	31.32%	3.399%
10	8.934	986	994	1005	rBV	1943306	3124603	20.91%	2.270%
11	9.652	1109	1116	1129	rBV	1487759	2469823	16.53%	1.794%
12	10.199	1201	1209	1227	rBV	2874753	4610596	30.86%	3.349%
13	10.569	1264	1272	1283	rBV	2064738	3619897	24.23%	2.629%
14	10.705	1287	1295	1308	rBV	2174511	3759787	25.17%	2.731%
15	12.163	1535	1543	1550	rVB	45128	81396	0.54%	0.059%
16	13.822	1817	1825	1842	rBV	4540720	6723463	45.00%	4.884%
17	14.116	1865	1875	1885	rBV	5197010	8206234	54.93%	5.961%
18	14.422	1918	1927	1936	rBV	3411372	5177145	34.65%	3.761%
19	14.640	1957	1964	1987	rBV	2273249	3376078	22.60%	2.452%
20	15.093	2037	2041	2048	rVB9	12249	21559	0.14%	0.016%
21	15.434	2091	2099	2111	rBV	6865884	10348095	69.27%	7.517%
22	15.545	2111	2118	2133	rVV	1904221	2537790	16.99%	1.843%
23	15.675	2136	2140	2150	rVB2	33639	65995	0.44%	0.048%
24	17.010	2363	2367	2372	rVB	17608	24827	0.17%	0.018%
25	17.228	2398	2404	2414	rBV	4602433	6518564	43.63%	4.735%
26	17.328	2414	2421	2436	rVV	8350038	11692682	78.27%	8.494%
27	19.245	2743	2747	2753	rVB2	98897	122962	0.82%	0.089%
28	19.316	2755	2759	2764	rBV	85223	126442	0.85%	0.092%
29	19.698	2817	2824	2835	rBV	9970939	14204275	95.08%	10.318%
30	21.669	3153	3159	3169	rBV	4712060	7676072	51.38%	5.576%
31	24.833	3688	3697	3715	rVB	6191579	14939648	100.00%	10.852%
32	25.074	3729	3738	3754	rVB	2935366	8074183	54.05%	5.865%




Sum of corrected areas: 137665147

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012725\
Data File : BP023749.D
Acq On : 27 Jan 2025 21:16
Operator : RC/JU
Sample : PB166248BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK248

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

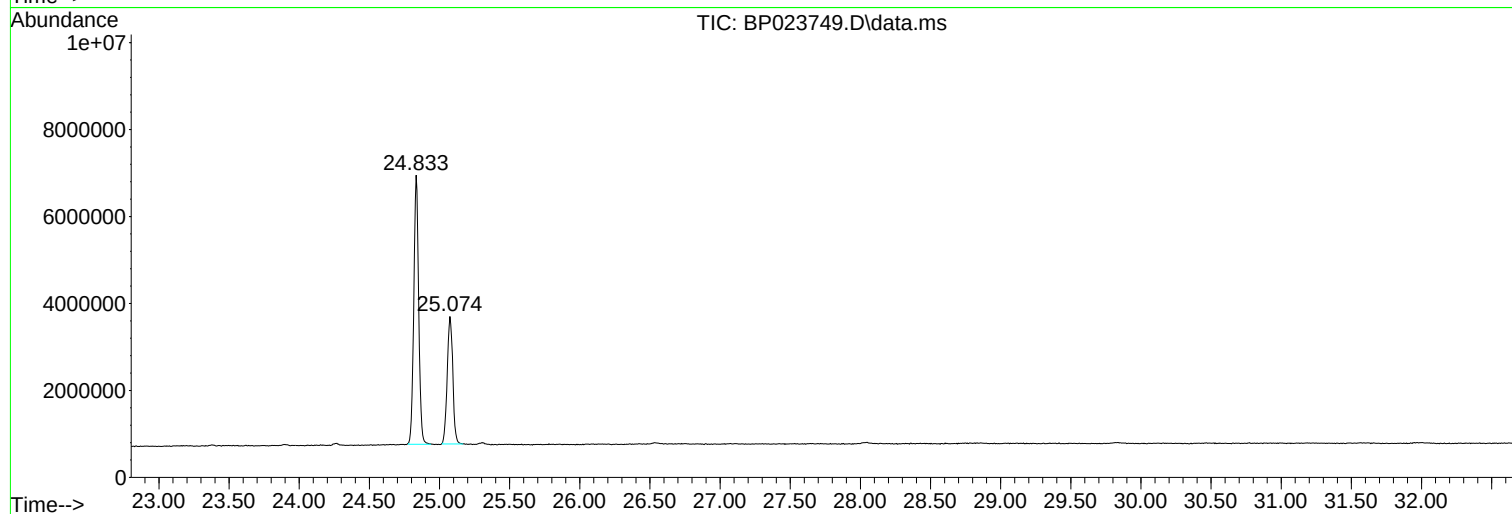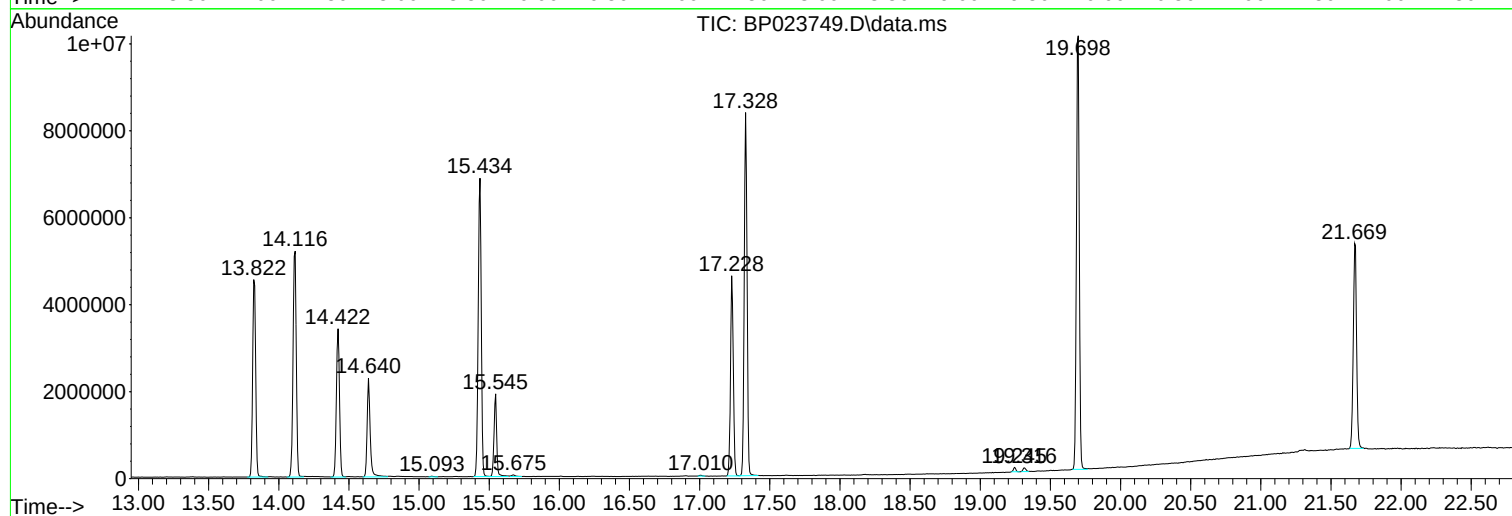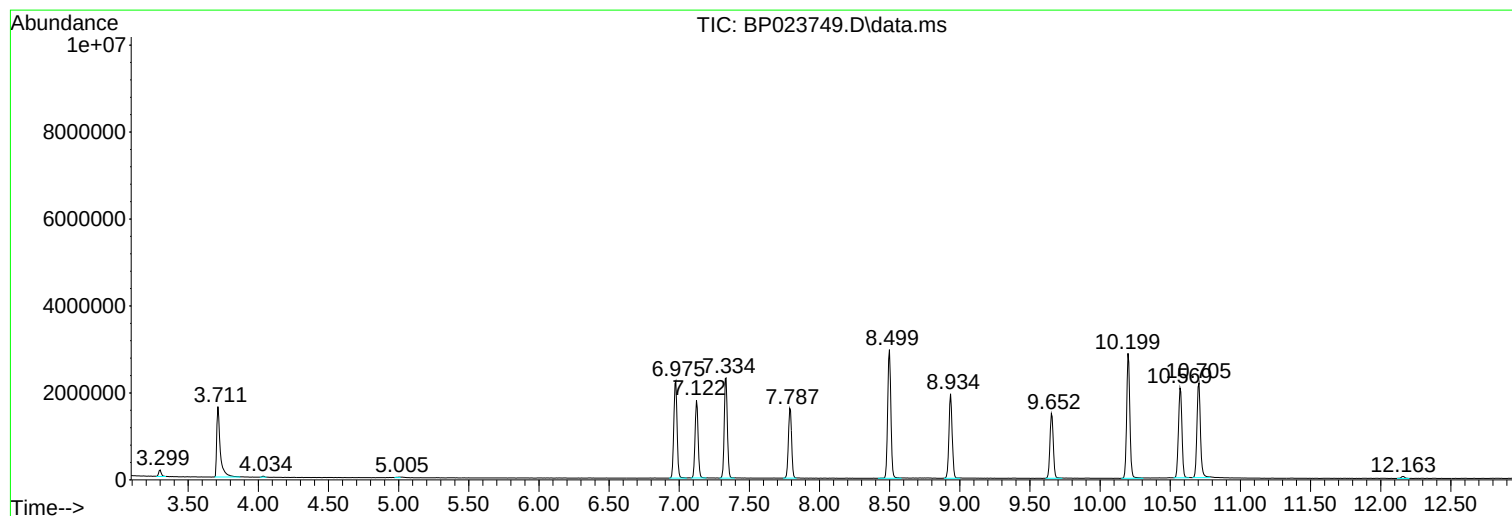

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012725\
Data File : BP023749.D
Acq On : 27 Jan 2025 21:16
Operator : RC/JU
Sample : PB166248BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK248

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012725\
Data File : BP023749.D
Acq On : 27 Jan 2025 21:16
Operator : RC/JU
Sample : PB166248BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK248

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc