

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012725\
 Data File : BP023754.D
 Acq On : 28 Jan 2025 00:38
 Operator : RC/JU
 Sample : Q1174-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E2944

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023754.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	32	36	48	rVB	124416	169950	0.90%	0.100%
2	3.711	102	106	120	rBV	468851	762595	4.02%	0.447%
3	4.034	158	161	168	rVB	31862	42639	0.22%	0.025%
4	4.128	173	177	187	rVB	41114	61990	0.33%	0.036%
5	4.934	310	314	320	rVB	20392	30621	0.16%	0.018%
6	5.540	413	417	425	rVB8	9706	19563	0.10%	0.011%
7	6.193	523	528	534	rBV	35435	52576	0.28%	0.031%
8	6.975	652	661	674	rBV	694277	1096835	5.78%	0.642%
9	7.122	679	686	699	rVB	2150914	3364630	17.74%	1.971%
10	7.334	715	722	732	rBV	2391494	3729478	19.67%	2.184%
11	7.787	792	799	807	rBV	2038731	3263102	17.21%	1.911%
12	8.216	868	872	878	rVB3	13336	21905	0.12%	0.013%
13	8.499	911	920	929	rBV	2328254	3427722	18.08%	2.008%
14	8.934	982	994	1005	rBV	2606406	4137310	21.82%	2.423%
15	9.075	1012	1018	1031	rBV	108017	203435	1.07%	0.119%
16	9.381	1066	1070	1077	rVB	33600	54983	0.29%	0.032%
17	9.499	1084	1090	1094	rBV4	20494	29337	0.15%	0.017%
18	9.652	1108	1116	1124	rBV	2140513	3430238	18.09%	2.009%
19	10.199	1199	1209	1226	rBV	3227363	5678655	29.95%	3.326%
20	10.569	1257	1272	1284	rVB	2971534	5106040	26.93%	2.991%
21	10.699	1286	1294	1314	rBV	2836453	4760274	25.10%	2.788%
22	11.369	1402	1408	1416	rBV	32442	55630	0.29%	0.033%
23	11.875	1489	1494	1498	rBV5	13159	22090	0.12%	0.013%
24	11.922	1498	1502	1507	rVB	47241	68659	0.36%	0.040%
25	12.152	1534	1541	1549	rBV2	57082	98912	0.52%	0.058%
26	12.604	1613	1618	1624	rBV3	17727	30589	0.16%	0.018%
27	13.257	1723	1729	1735	rVB3	44461	75070	0.40%	0.044%
28	13.822	1816	1825	1832	rBV	7013407	9276763	48.92%	5.433%
29	14.110	1862	1874	1883	rBV	8016663	11143180	58.76%	6.527%
30	14.416	1919	1926	1936	rBV	5076072	7326682	38.64%	4.291%
31	14.493	1936	1939	1946	rVB8	15667	26265	0.14%	0.015%
32	14.646	1959	1965	1974	rBV	661048	1085682	5.73%	0.636%
33	14.763	1982	1985	1992	rVB8	15385	29235	0.15%	0.017%
34	14.845	1995	1999	2004	rVB8	14448	24579	0.13%	0.014%
35	14.975	2016	2021	2031	rBV	77940	136833	0.72%	0.080%
36	15.257	2064	2069	2073	rBV4	17503	27298	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012725\
 Data File : BP023754.D
 Acq On : 28 Jan 2025 00:38
 Operator : RC/JU
 Sample : Q1174-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E2944

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
 Title : SVOA CALIBRATION

37	15.428	2091	2098	2110	rBV	9681869	14580797	76.89%	8.540%
38	15.540	2110	2117	2128	rBV	2728423	3861413	20.36%	2.262%
39	15.669	2136	2139	2149	rVB2	48286	85864	0.45%	0.050%
40	15.798	2156	2161	2168	rVB	194027	276294	1.46%	0.162%
41	15.998	2193	2195	2202	rVB8	15229	25860	0.14%	0.015%
42	16.622	2297	2301	2305	rBV4	24200	38459	0.20%	0.023%
43	16.998	2361	2365	2370	rVB2	48946	67614	0.36%	0.040%
44	17.222	2396	2403	2410	rBV	6014028	8689021	45.82%	5.089%
45	17.322	2413	2420	2434	rVV	12172953	16476879	86.89%	9.651%
46	17.769	2492	2496	2499	rBV3	33884	44148	0.23%	0.026%
47	17.928	2521	2523	2528	rVB4	36123	44094	0.23%	0.026%
48	18.169	2560	2564	2571	rBV	227461	364350	1.92%	0.213%
49	18.486	2614	2618	2623	rBV3	90118	121254	0.64%	0.071%
50	18.616	2638	2640	2643	rBV4	27146	31622	0.17%	0.019%
51	19.245	2743	2747	2751	rBV	148353	190262	1.00%	0.111%
52	19.316	2755	2759	2763	rVB	131211	176786	0.93%	0.104%
53	19.698	2817	2824	2830	rBV	13563905	18840929	99.35%	11.035%
54	21.675	3154	3160	3170	rVB2	5828607	9207075	48.55%	5.393%
55	24.851	3689	3700	3716	rVB	6564061	18963559	100.00%	11.107%
56	25.080	3731	3739	3754	rVB	3637967	9775607	51.55%	5.726%




Sum of corrected areas: 170733232

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012725\
Data File : BP023754.D
Acq On : 28 Jan 2025 00:38
Operator : RC/JU
Sample : Q1174-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2944

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

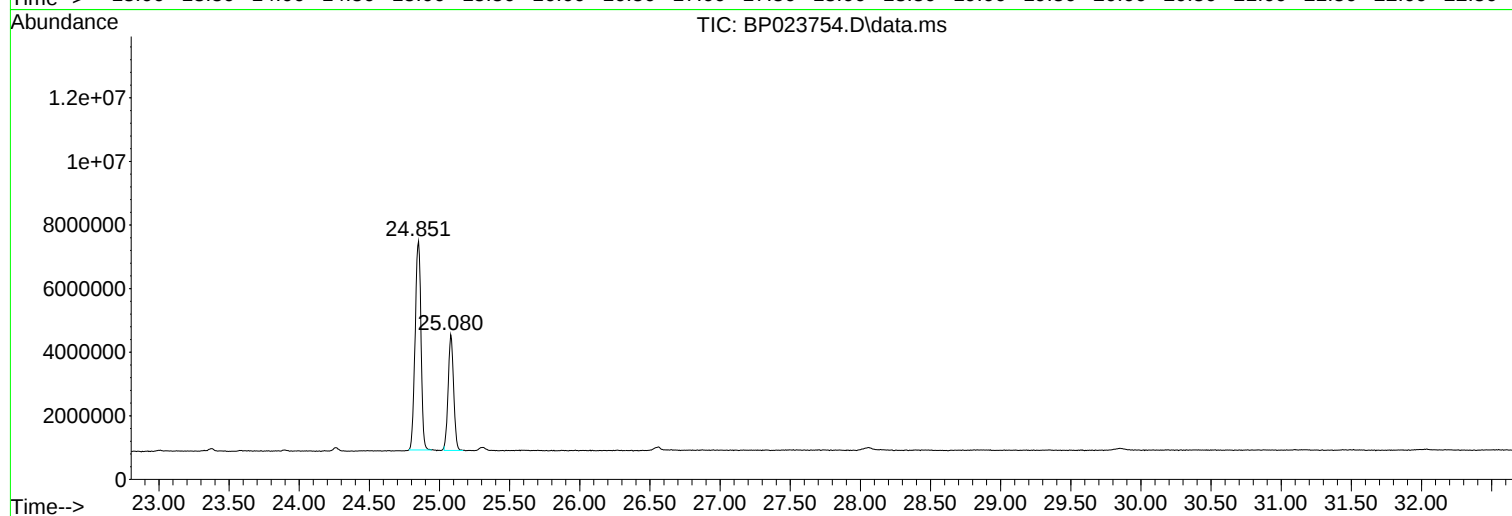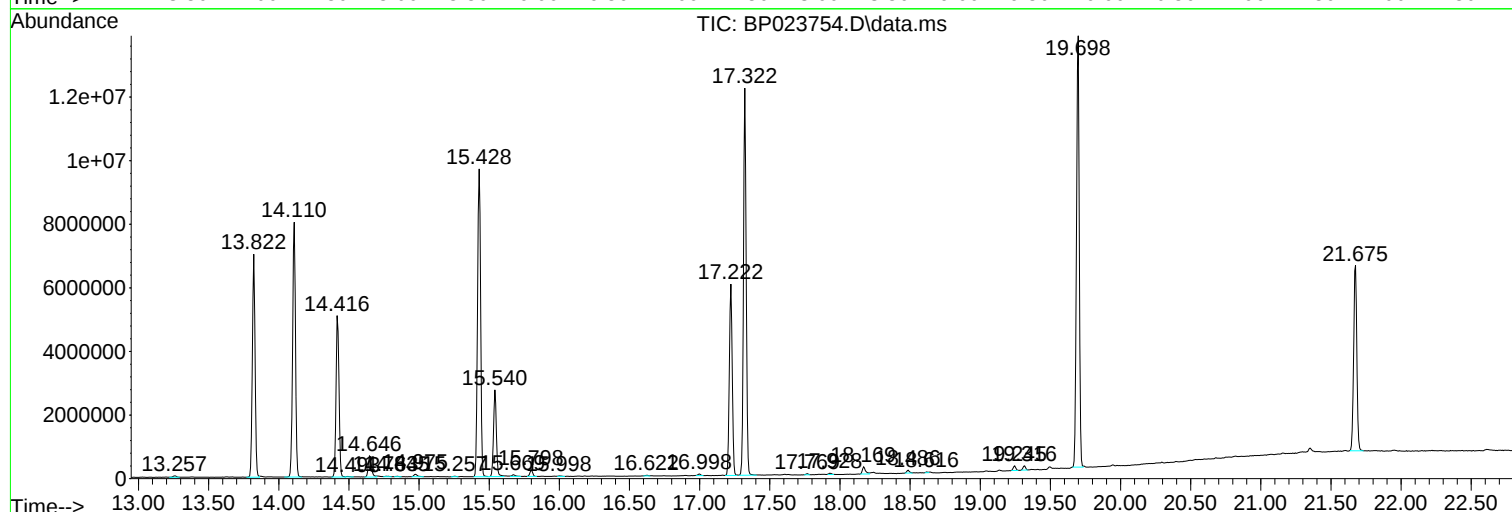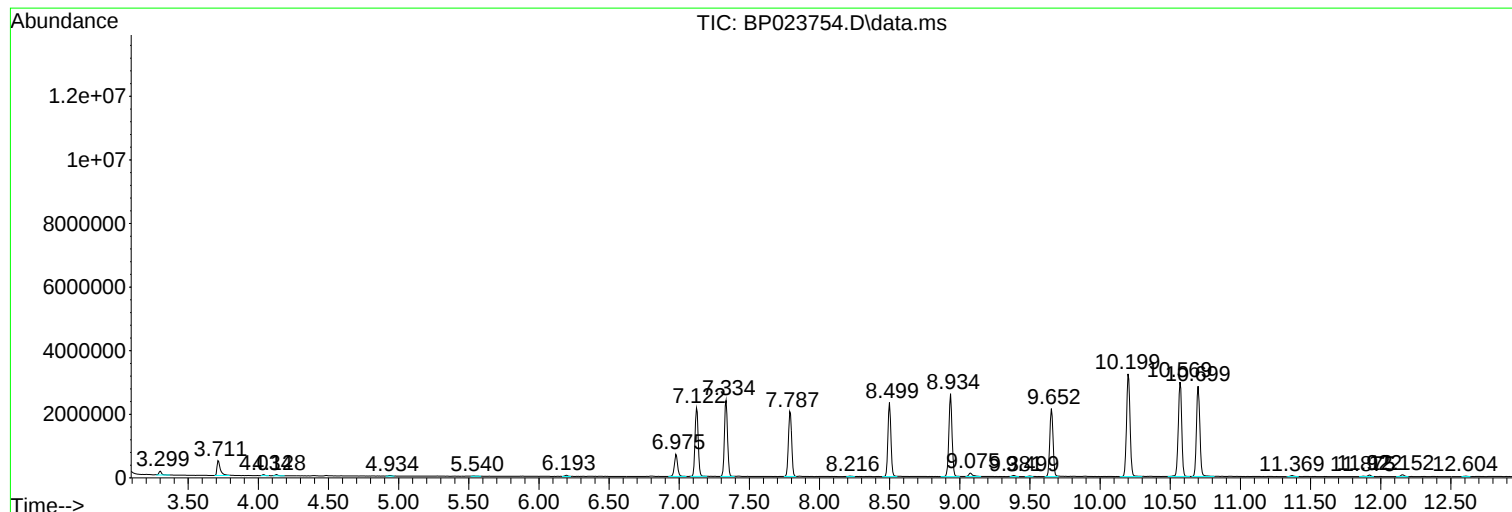

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012725\
Data File : BP023754.D
Acq On : 28 Jan 2025 00:38
Operator : RC/JU
Sample : Q1174-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2944

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012725\
Data File : BP023754.D
Acq On : 28 Jan 2025 00:38
Operator : RC/JU
Sample : Q1174-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2944

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------