

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012725\
 Data File : BP023765.D
 Acq On : 28 Jan 2025 09:05
 Operator : RC/JU
 Sample : PB166254BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK254

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023765.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	29	33	40	rVB	164925	209248	1.38%	0.136%
2	3.693	99	103	129	rBV	1849001	3066808	20.16%	2.000%
3	4.010	153	157	164	rVB2	35901	50738	0.33%	0.033%
4	6.951	650	657	674	rBV	2291815	3658253	24.05%	2.386%
5	7.092	674	681	697	rVB	1945837	2808342	18.46%	1.832%
6	7.304	710	717	727	rBV	2354996	3748672	24.64%	2.445%
7	7.763	787	795	803	rBV	2287200	3633677	23.89%	2.370%
8	8.475	907	916	928	rBV	3011474	4707928	30.95%	3.071%
9	8.904	982	989	1002	rBV	1879349	3206440	21.08%	2.091%
10	9.628	1105	1112	1126	rBV	1524672	2553045	16.78%	1.665%
11	10.181	1197	1206	1220	rBV	2617511	4638966	30.50%	3.026%
12	10.551	1261	1269	1284	rVB	3076324	5003670	32.89%	3.264%
13	10.681	1284	1291	1302	rBV	2260795	3847750	25.30%	2.510%
14	11.198	1371	1379	1385	rBV6	9712	17847	0.12%	0.012%
15	11.363	1400	1407	1414	rVB6	7928	16793	0.11%	0.011%
16	12.139	1533	1539	1548	rVB	45864	80852	0.53%	0.053%
17	13.374	1742	1749	1755	rVB4	9886	17318	0.11%	0.011%
18	13.816	1816	1824	1839	rBV	4753677	6979885	45.89%	4.553%
19	13.922	1839	1842	1850	rVB10	9861	20043	0.13%	0.013%
20	14.104	1865	1873	1887	rBV	5610456	8228336	54.09%	5.367%
21	14.416	1918	1926	1933	rBV	4796964	7022890	46.17%	4.581%
22	14.639	1957	1964	1985	rBV	1775124	3302148	21.71%	2.154%
23	14.827	1994	1996	2004	rVB8	10029	17685	0.12%	0.012%
24	15.086	2036	2040	2044	rVB6	12180	18125	0.12%	0.012%
25	15.421	2090	2097	2109	rBV	7013713	10462324	68.78%	6.824%
26	15.533	2110	2116	2128	rVV	1919795	2594385	17.06%	1.692%
27	15.663	2134	2138	2144	rVB3	25956	48172	0.32%	0.031%
28	16.227	2229	2234	2241	rVB3	9748	19101	0.13%	0.012%
29	17.004	2361	2366	2369	rBV2	26725	36545	0.24%	0.024%
30	17.221	2396	2403	2412	rBV2	6053612	8969691	58.97%	5.851%
31	17.321	2414	2420	2431	rBV2	8352073	11725630	77.09%	7.648%
32	19.245	2743	2747	2753	rBV2	91805	150737	0.99%	0.098%
33	19.321	2756	2760	2766	rVV2	95290	144079	0.95%	0.094%
34	19.409	2771	2775	2780	rVV	108510	131564	0.86%	0.086%
35	19.657	2813	2817	2819	rBV	250878	303843	2.00%	0.198%
36	19.698	2819	2824	2835	rVB	10849978	14352909	94.36%	9.362%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012725\
Data File : BP023765.D
Acq On : 28 Jan 2025 09:05
Operator : RC/JU
Sample : PB166254BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK254

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
Title : SVOA CALIBRATION

37	20.751	3001	3003	3007	rVB2	164765	166809	1.10%	0.109%
38	21.686	3156	3162	3175	rVB	7039847	10614371	69.78%	6.923%
39	24.874	3695	3704	3723	rVB	5802677	15211242	100.00%	9.922%
40	25.103	3734	3743	3759	rVB	4125976	11527918	75.79%	7.519%




Sum of corrected areas: 153314779

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012725\
Data File : BP023765.D
Acq On : 28 Jan 2025 09:05
Operator : RC/JU
Sample : PB166254BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK254

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

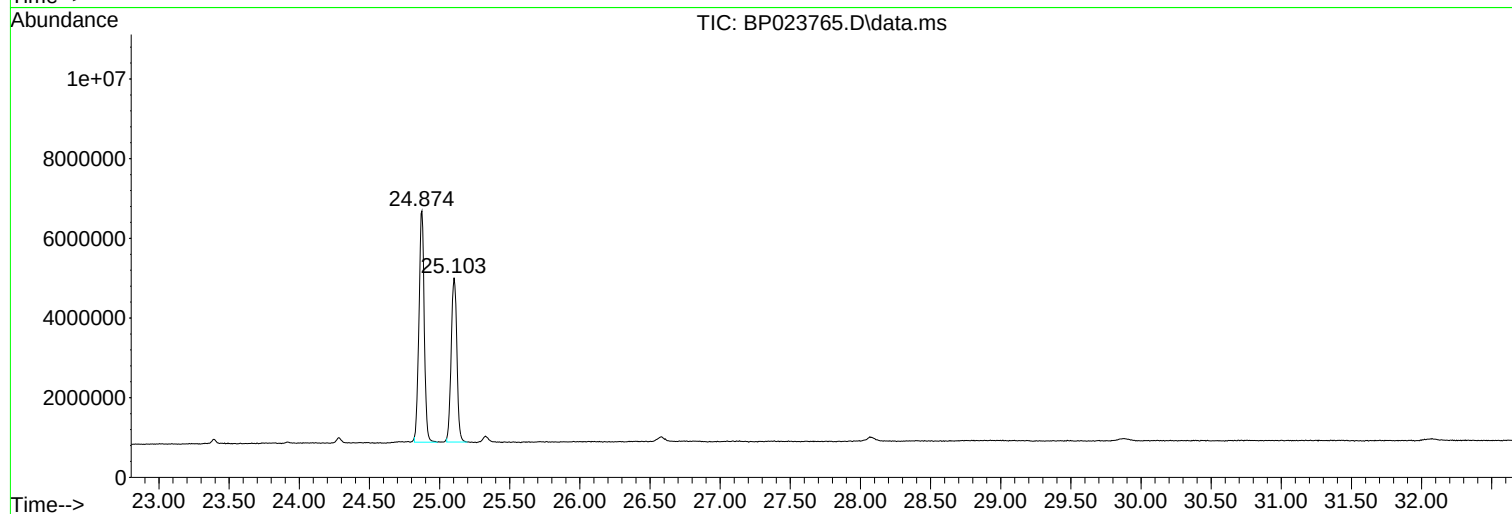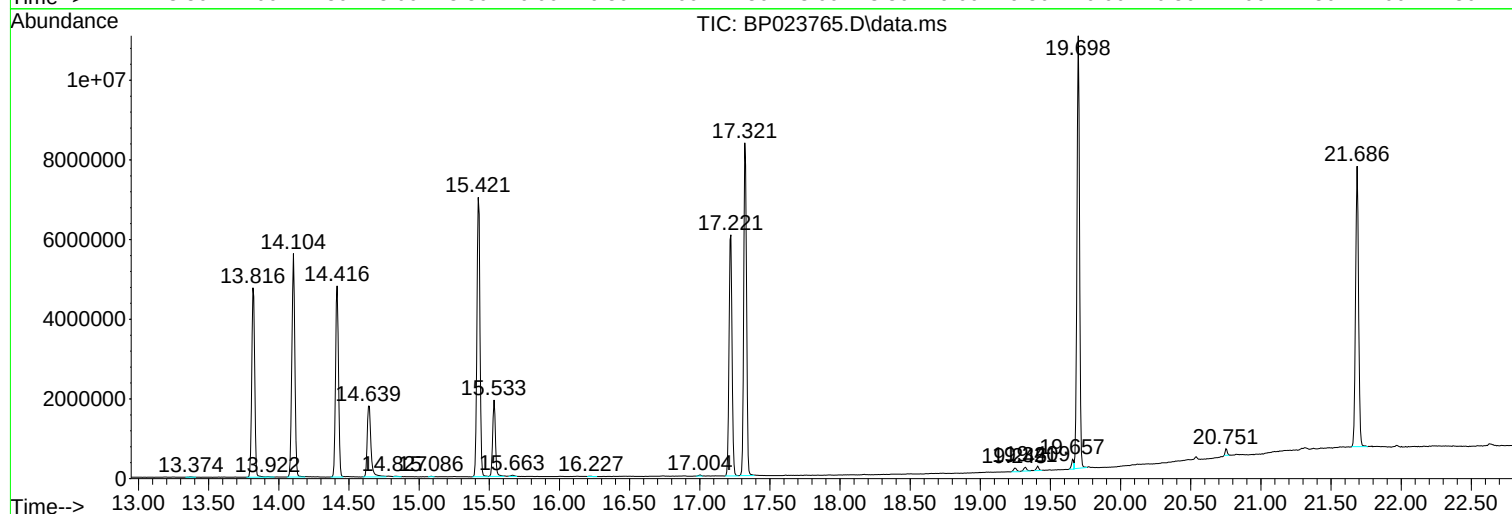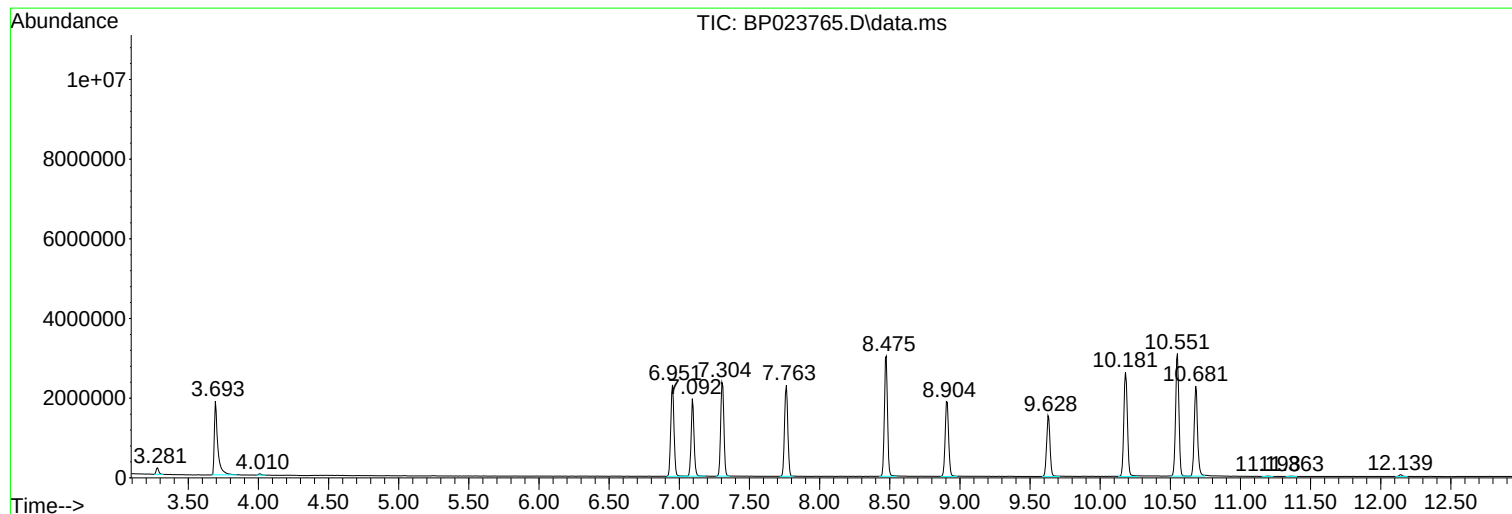

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012725\
Data File : BP023765.D
Acq On : 28 Jan 2025 09:05
Operator : RC/JU
Sample : PB166254BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK254

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012725\
Data File : BP023765.D
Acq On : 28 Jan 2025 09:05
Operator : RC/JU
Sample : PB166254BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK254

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------