

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013125\
 Data File : BN036178.D
 Acq On : 31 Jan 2025 21:15
 Operator : RC/JU
 Sample : 01197-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E2986

Quant Time: Feb 03 08:52:22 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 21 23:52:22 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.795	152	2778	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.583	136	7036	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.436	164	4466	0.400	ng/ul	-0.01
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.19
17) Chrysene-d12	21.369	240	10790	0.400	ng/ul	0.00
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.67
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.259	96	12838	4.221	ng/ul	-0.02
6) 2-Methylnaphthalene-d10	12.183	152	2959	0.333	ng/ul	-0.02
18) Fluoranthene-d10	19.210	212	10692	0.361	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.431	166	1262	0.074	ng/ul#	17
20) Pyrene	19.578	202	1535	0.036	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013125\
Data File : BN036178.D
Acq On : 31 Jan 2025 21:15
Operator : RC/JU
Sample : 01197-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2986

Quant Time: Feb 03 08:52:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN012125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 21 23:52:22 2025
Response via : Initial Calibration




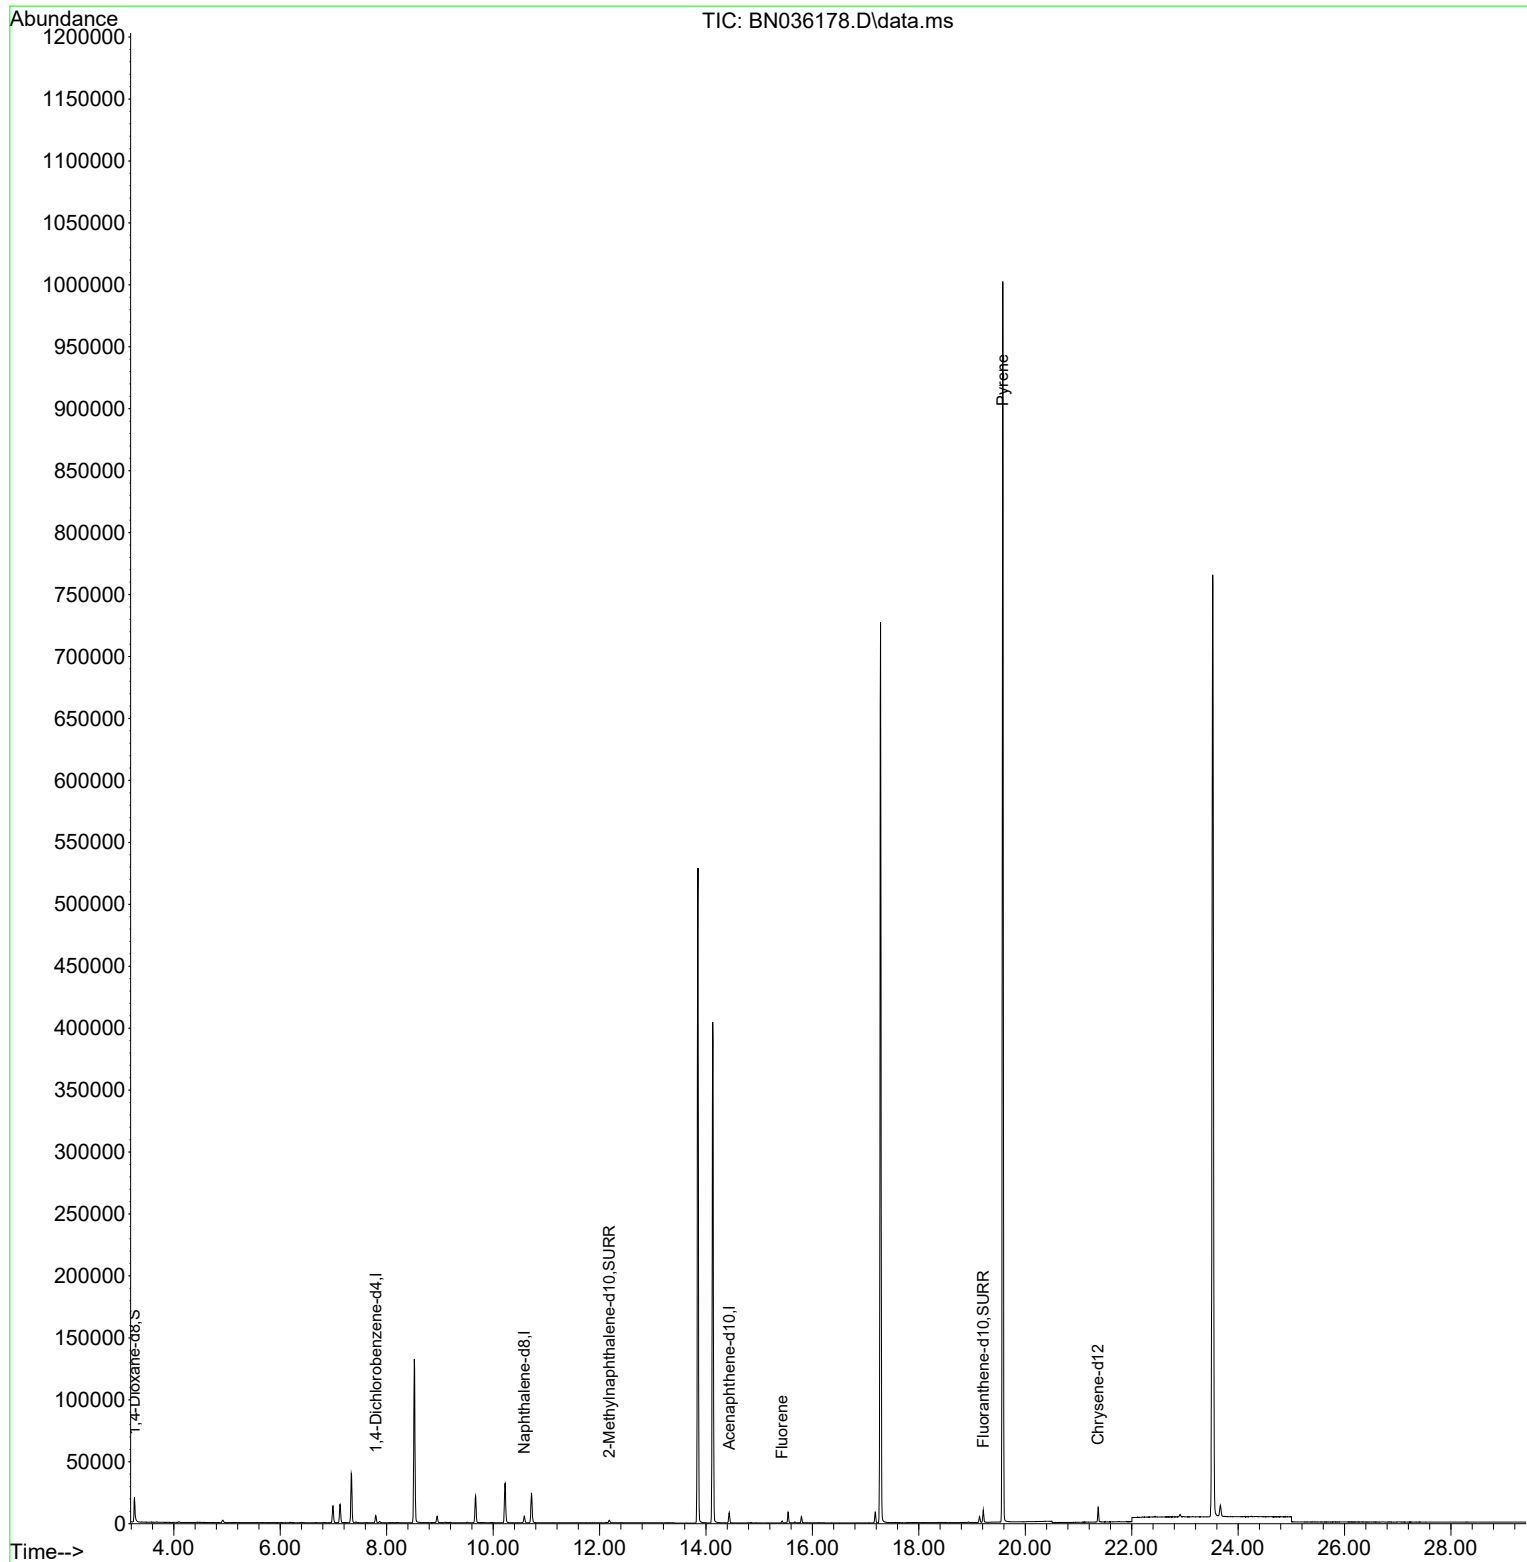


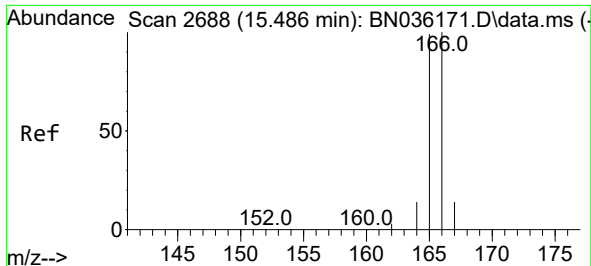

#12
Fluorene
Concen: 0.074 ng/ul
RT: 15.431 min Scan# 2676
Delta R.T. -0.070 min
Lab File: BN036178.D
Acq: 31 Jan 2025 21:15

Instrument :
BNA_P
ClientSampleId :
E2986

Tgt Ion:166 Resp: 1262
Ion Ratio Lower Upper
166 100
165 13.3 80.3 120.5#
167 38.9 12.3 18.5#

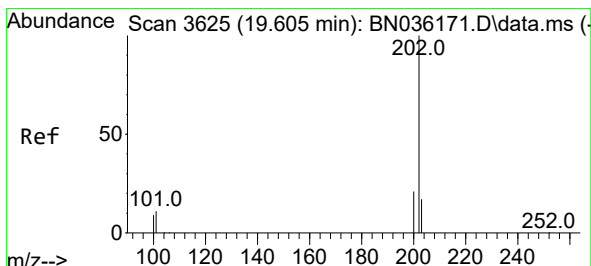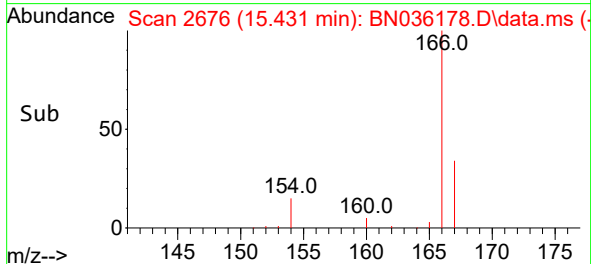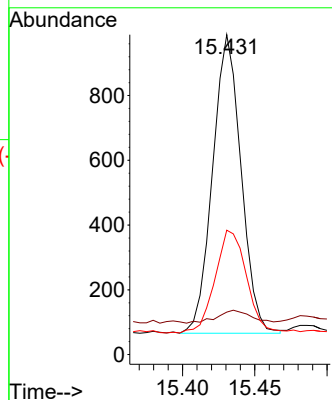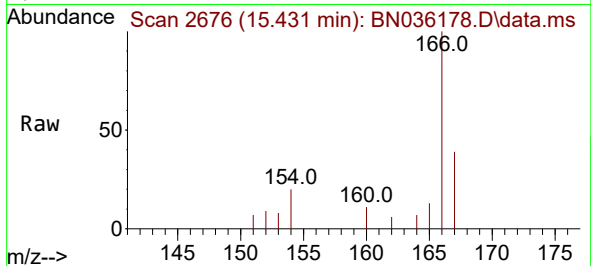

#20
Pyrene
Concen: 0.036 ng/ul
RT: 19.578 min Scan# 3619
Delta R.T. -0.032 min
Lab File: BN036178.D
Acq: 31 Jan 2025 21:15

Tgt Ion:202 Resp: 1535
Ion Ratio Lower Upper
202 100
101 167.7 9.3 13.9#
100 1170.0 7.5 11.3#

