

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
 Data File : BP023831.D
 Acq On : 31 Jan 2025 18:43
 Operator : RC/JU
 Sample : Q1224-14
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A6321

Quant Time: Feb 03 07:36:31 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 31 11:40:55 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	449283	20.000	ng/ul	0.02
20) Naphthalene-d8	10.557	136	1889941	20.000	ng/ul	0.01
38) Acenaphthene-d10	14.404	164	1275740	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.210	188	2605623	20.000	ng/ul	0.00
79) Chrysene-d12	21.651	240	2586130	20.000	ng/ul	0.00
88) Perylene-d12	25.033	264	2809018	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	38449	3.556	ng/uL	0.01
4) Pyridine-d5	3.711	84	487370	15.620	ng/ul	0.02
7) Phenol-d5	6.969	99	719912	18.106	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	7.116	67	395675	18.801	ng/ul	0.02
11) 2-Chlorophenol-d4	7.328	132	586858	18.796	ng/ul	0.02
15) 4-Methylphenol-d8	8.493	113	584283	17.989	ng/ul	0.02
21) Nitrobenzene-d5	8.928	128	277749	18.369	ng/ul	0.02
24) 2-Nitrophenol-d4	9.646	143	296601	18.179	ng/ul	0.02
28) 2,4-Dichlorophenol-d3	10.187	165	526160	17.579	ng/ul	0.01
31) 4-Chloroaniline-d4	10.693	131	746150	16.669	ng/ul	0.01
46) Dimethylphthalate-d6	13.804	166	1708008	17.949	ng/ul	0.00
49) Acenaphthylene-d8	14.093	160	1817763	16.937	ng/ul	0.00
54) 4-Nitrophenol-d4	14.628	143	250579	13.260	ng/ul	0.00
60) Fluorene-d10	15.410	176	1303191	16.263	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.528	200	146835	9.135	ng/ul	0.00
73) Anthracene-d10	17.304	188	1913748	14.959	ng/ul	-0.01
81) Pyrene-d10	19.675	212	2038137	14.708	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.792	264	1801444	12.291	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	6.993	94	43439	1.064	ng/ul	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023831.D
Acq On : 31 Jan 2025 18:43
Operator : RC/JU
Sample : Q1224-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A6321

Quant Time: Feb 03 07:36:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 31 11:40:55 2025
Response via : Initial Calibration

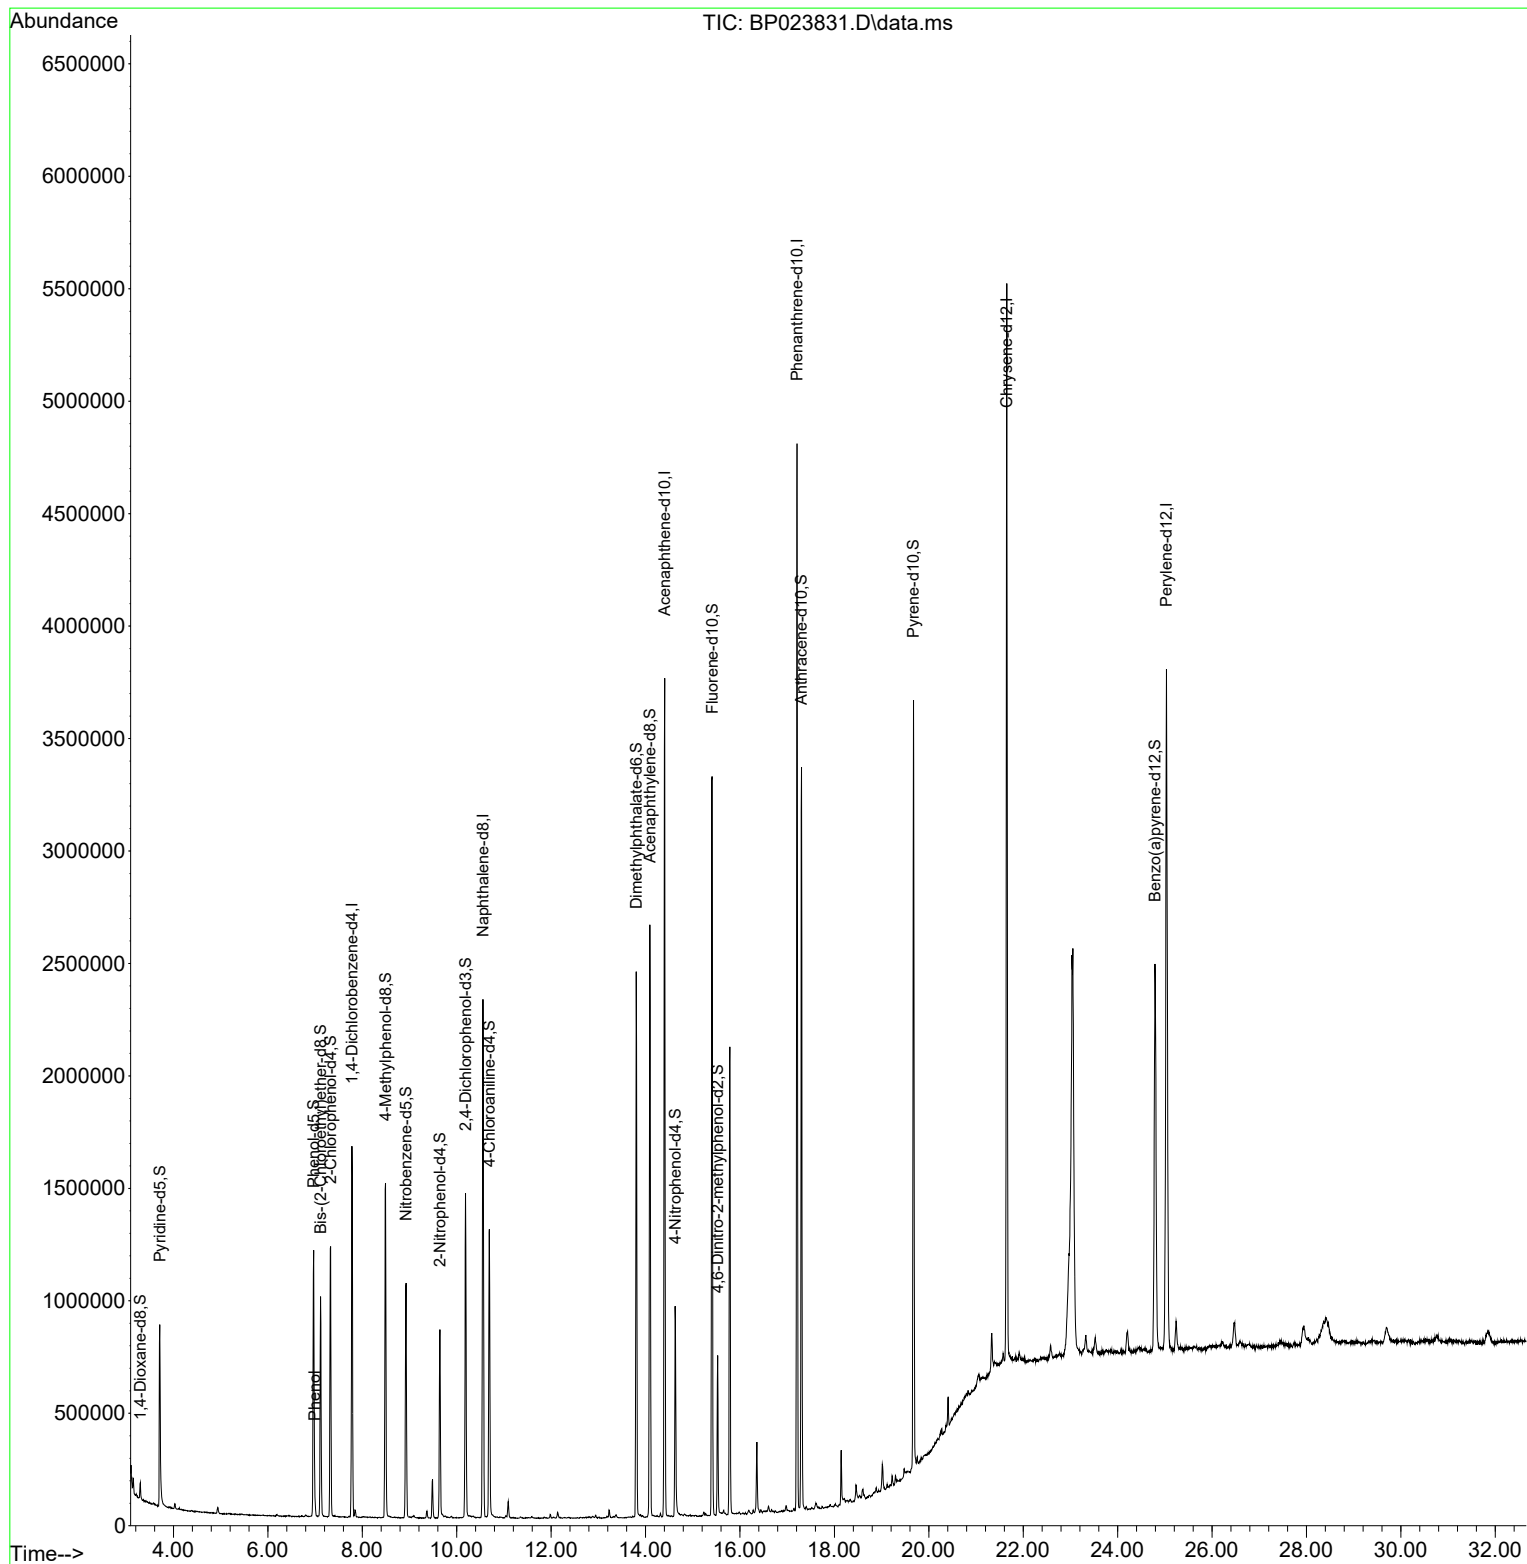

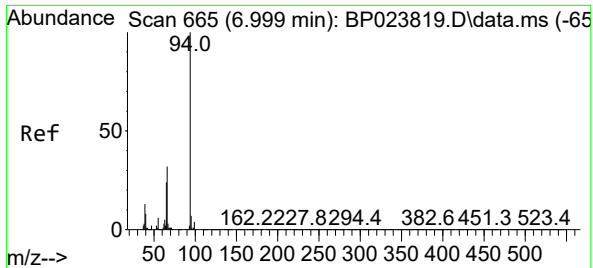

#8
Phenol
Concen: 1.064 ng/ul
RT: 6.993 min Scan# 60
Delta R.T. 0.018 min
Lab File: BP023831.D
Acq: 31 Jan 2025 18:43

Instrument :
BNA_P
ClientSampleId :
A6321

Tgt Ion: 94 Resp: 43439
Ion Ratio Lower Upper
94 100
65 24.2 20.1 30.1
66 36.7 26.0 39.0

