

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
 Data File : BP023832.D
 Acq On : 31 Jan 2025 19:24
 Operator : RC/JU
 Sample : Q1224-15
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A6322

Quant Time: Feb 03 07:36:45 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 31 11:40:55 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	421165	20.000	ng/ul	0.02
20) Naphthalene-d8	10.557	136	1760662	20.000	ng/ul	0.01
38) Acenaphthene-d10	14.404	164	1130983	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.192	188	2277201	20.000	ng/ul	-0.02
79) Chrysene-d12	21.639	240	2335943	20.000	ng/ul	0.00
88) Perylene-d12	25.027	264	2487269	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	41340	4.078	ng/uL	0.01
4) Pyridine-d5	3.711	84	555199	18.981	ng/ul	0.02
7) Phenol-d5	6.963	99	734203	19.699	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	7.116	67	432009	21.898	ng/ul	0.02
11) 2-Chlorophenol-d4	7.328	132	635021	21.696	ng/ul	0.02
15) 4-Methylphenol-d8	8.487	113	615815	20.226	ng/ul	0.02
21) Nitrobenzene-d5	8.928	128	295409	20.971	ng/ul	0.02
24) 2-Nitrophenol-d4	9.646	143	275571	18.130	ng/ul	0.02
28) 2,4-Dichlorophenol-d3	10.193	165	548326	19.665	ng/ul	0.02
31) 4-Chloroaniline-d4	10.687	131	779209	18.686	ng/ul	0.00
46) Dimethylphthalate-d6	13.804	166	1843599	21.854	ng/ul	0.00
49) Acenaphthylene-d8	14.092	160	1484527	15.603	ng/ul	0.00
54) 4-Nitrophenol-d4	14.628	143	136232	8.132	ng/ul	0.00
60) Fluorene-d10	15.404	176	999822	14.074	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.522	200	76789	5.466	ng/ul	-0.01
73) Anthracene-d10	17.292	188	1417391	12.677	ng/ul	-0.02
81) Pyrene-d10	19.657	212	1430374	11.428	ng/ul	-0.02
92) Benzo(a)pyrene-d12	24.786	264	1135958	8.753	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	6.993	94	60593	1.583	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023832.D
Acq On : 31 Jan 2025 19:24
Operator : RC/JU
Sample : Q1224-15
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A6322

Quant Time: Feb 03 07:36:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 31 11:40:55 2025
Response via : Initial Calibration

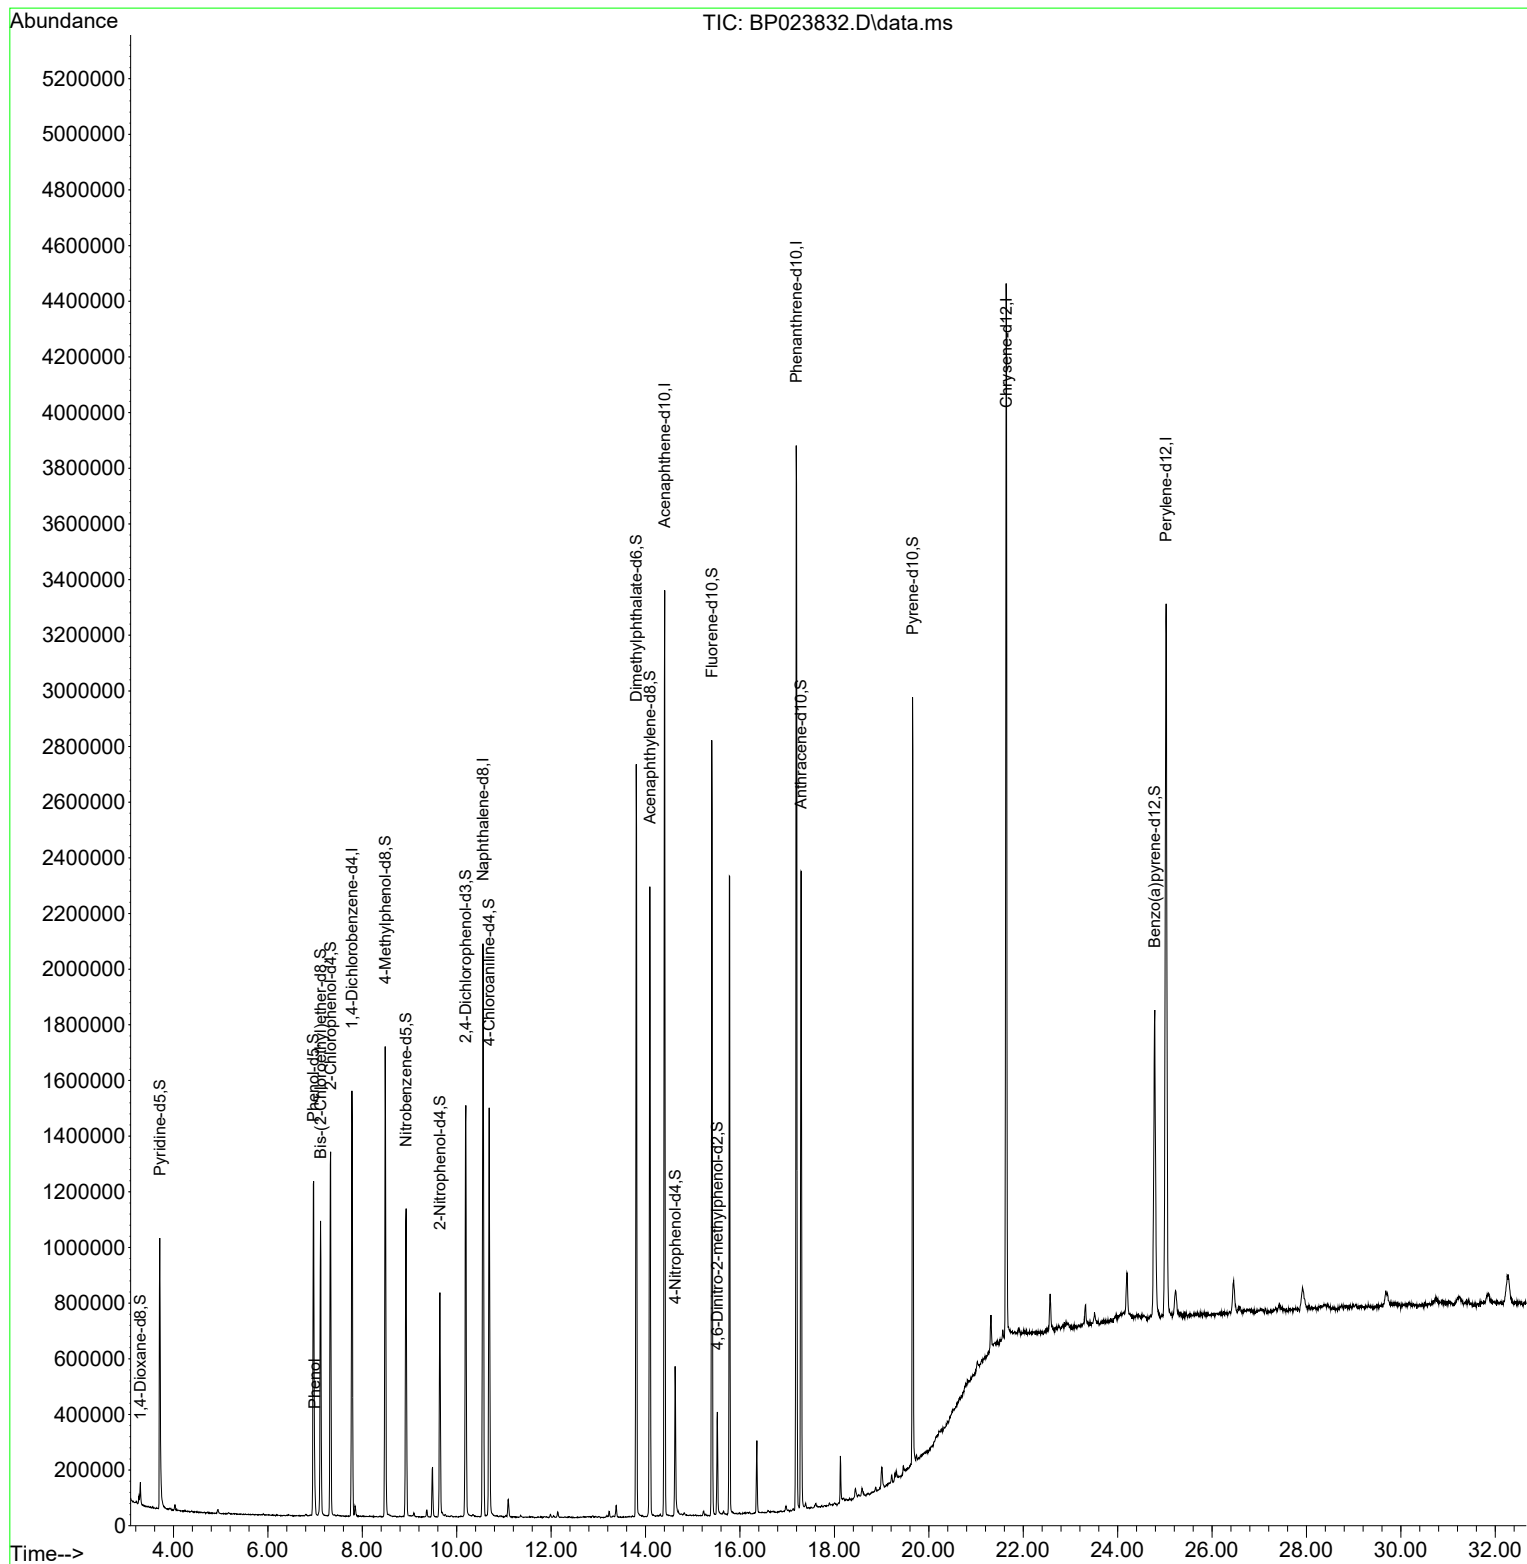

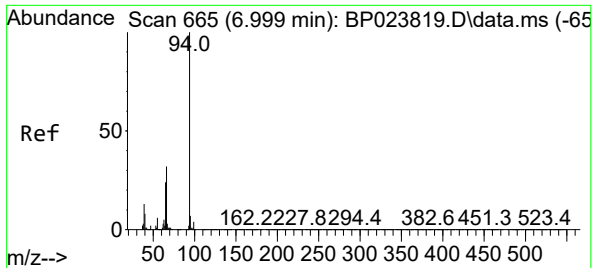

#8
Phenol
Concen: 1.583 ng/ul
RT: 6.993 min Scan# 60
Delta R.T. 0.018 min
Lab File: BP023832.D
Acq: 31 Jan 2025 19:24

Instrument :
BNA_P
ClientSampleId :
A6322

Tgt Ion: 94	Resp: 60593
Ion Ratio	Lower Upper
94 100	
65 25.0	20.1 30.1
66 32.8	26.0 39.0

