

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
 Data File : BP023837.D
 Acq On : 31 Jan 2025 23:29
 Operator : RC/JU
 Sample : Q1224-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A6301

Quant Time: Feb 03 07:37:29 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 31 11:40:55 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	415943	20.000	ng/ul	0.02
20) Naphthalene-d8	10.557	136	1734709	20.000	ng/ul	0.01
38) Acenaphthene-d10	14.404	164	1119689	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.198	188	2299495	20.000	ng/ul	-0.01
79) Chrysene-d12	21.645	240	2282101	20.000	ng/ul	0.00
88) Perylene-d12	25.021	264	2441420	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	31647	3.161	ng/uL	0.01
4) Pyridine-d5	3.710	84	407250	14.098	ng/ul	0.02
7) Phenol-d5	6.969	99	588515	15.988	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	7.116	67	339411	17.420	ng/ul	0.02
11) 2-Chlorophenol-d4	7.322	132	483538	16.728	ng/ul	0.01
15) 4-Methylphenol-d8	8.487	113	486054	16.164	ng/ul	0.02
21) Nitrobenzene-d5	8.922	128	228927	16.495	ng/ul	0.01
24) 2-Nitrophenol-d4	9.640	143	225994	15.091	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	10.187	165	433127	15.766	ng/ul	0.01
31) 4-Chloroaniline-d4	10.692	131	601101	14.630	ng/ul	0.01
46) Dimethylphthalate-d6	13.804	166	1514558	18.135	ng/ul	0.00
49) Acenaphthylene-d8	14.092	160	1246439	13.232	ng/ul	0.00
54) 4-Nitrophenol-d4	14.628	143	205753	12.405	ng/ul	0.00
60) Fluorene-d10	15.410	176	825405	11.736	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.522	200	121348	8.554	ng/ul	-0.01
73) Anthracene-d10	17.298	188	1134873	10.052	ng/ul	-0.02
81) Pyrene-d10	19.668	212	1130885	9.248	ng/ul	-0.01
92) Benzo(a)pyrene-d12	24.780	264	874117	6.862	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	6.993	94	41741	1.104	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023837.D
Acq On : 31 Jan 2025 23:29
Operator : RC/JU
Sample : Q1224-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A6301

Quant Time: Feb 03 07:37:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 31 11:40:55 2025
Response via : Initial Calibration

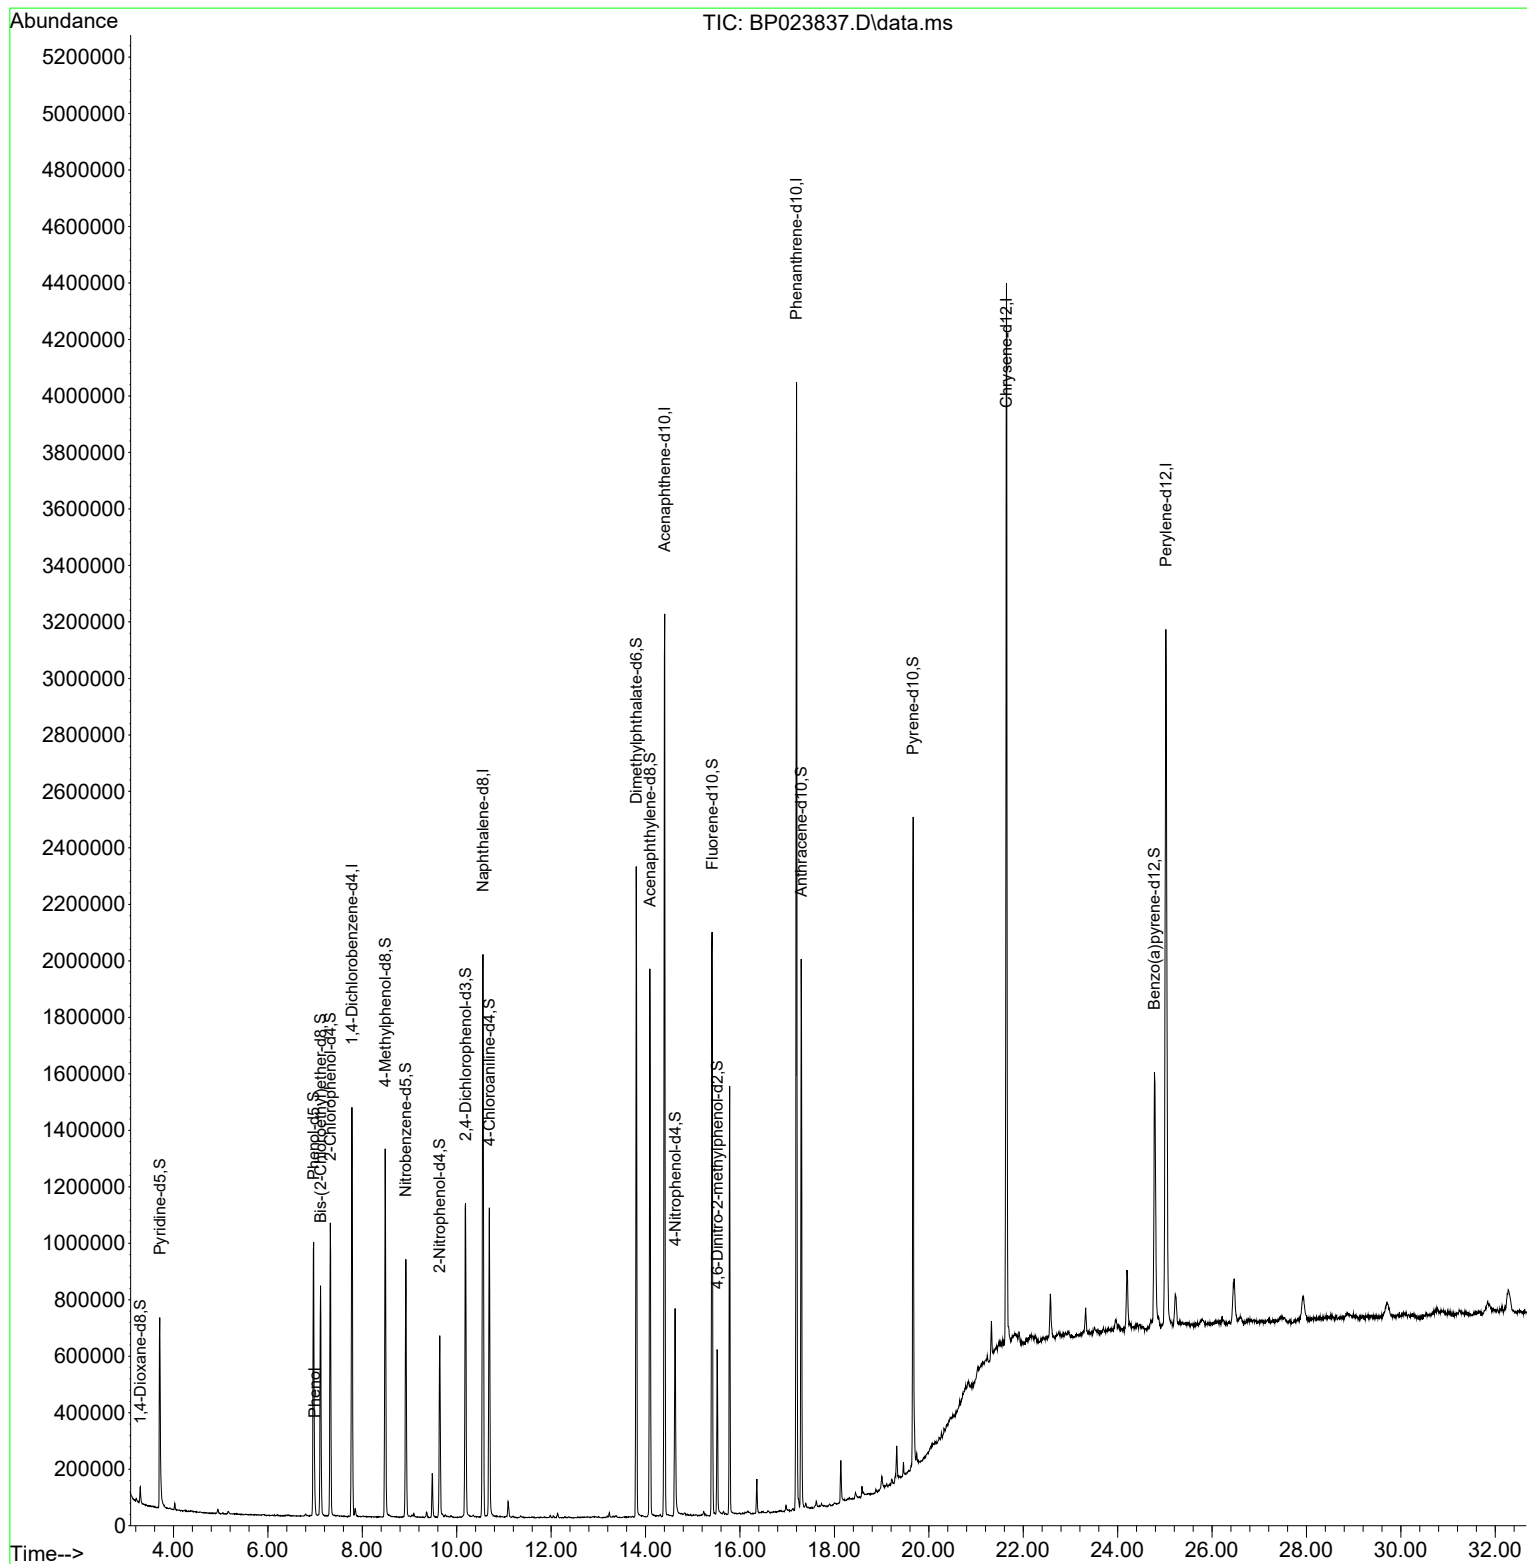

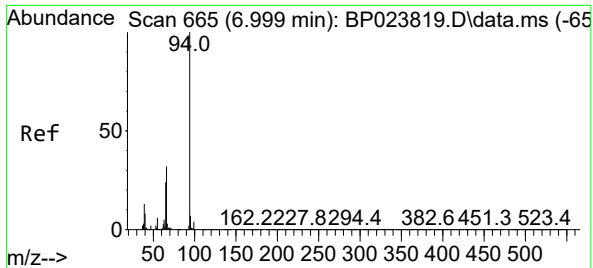

#8
Phenol
Concen: 1.104 ng/ul
RT: 6.993 min Scan# 6
Delta R.T. 0.018 min
Lab File: BP023837.D
Acq: 31 Jan 2025 23:29

Instrument :
BNA_P
ClientSampleId :
A6301

Tgt Ion: 94	Resp:	41741
Ion	Ratio	Lower Upper
94	100	
65	25.2	20.1 30.1
66	36.1	26.0 39.0

