

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
 Data File : BP023854.D
 Acq On : 01 Feb 2025 12:06
 Operator : RC/JU
 Sample : Q1248-04
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A6326

Quant Time: Feb 03 08:22:46 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 31 11:40:55 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	343990	20.000	ng/ul	0.02
20) Naphthalene-d8	10.557	136	1469278	20.000	ng/ul	0.01
38) Acenaphthene-d10	14.398	164	976930	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.187	188	2045125	20.000	ng/ul	-0.02
79) Chrysene-d12	21.639	240	2004840	20.000	ng/ul	0.00
88) Perylene-d12	24.998	264	2185428	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	23916	2.889	ng/uL	0.00
4) Pyridine-d5	3.711	84	293271	12.276	ng/ul	0.02
7) Phenol-d5	6.964	99	442809	14.546	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	7.117	67	265092	16.452	ng/ul	0.02
11) 2-Chlorophenol-d4	7.322	132	359313	15.031	ng/ul	0.01
15) 4-Methylphenol-d8	8.487	113	318171	12.794	ng/ul	0.02
21) Nitrobenzene-d5	8.922	128	176964	15.054	ng/ul	0.01
24) 2-Nitrophenol-d4	9.640	143	185651	14.637	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	10.181	165	325098	13.971	ng/ul	0.00
31) 4-Chloroaniline-d4	10.687	131	416318	11.964	ng/ul	0.00
46) Dimethylphthalate-d6	13.799	166	1199808	16.465	ng/ul	0.00
49) Acenaphthylene-d8	14.087	160	994561	12.101	ng/ul	0.00
54) 4-Nitrophenol-d4	14.616	143	171488	11.850	ng/ul	0.00
60) Fluorene-d10	15.398	176	693448	11.300	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.516	200	95095	7.537	ng/ul	-0.02
73) Anthracene-d10	17.287	188	1020421	10.162	ng/ul	-0.03
81) Pyrene-d10	19.663	212	912795	8.497	ng/ul	-0.02
92) Benzo(a)pyrene-d12	24.769	264	720454	6.318	ng/ul	-0.02


Target Compounds					Qvalue
8) Phenol	6.993	94	32298	1.033 ng/ul	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023854.D
Acq On : 01 Feb 2025 12:06
Operator : RC/JU
Sample : Q1248-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A6326

Quant Time: Feb 03 08:22:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 31 11:40:55 2025
Response via : Initial Calibration

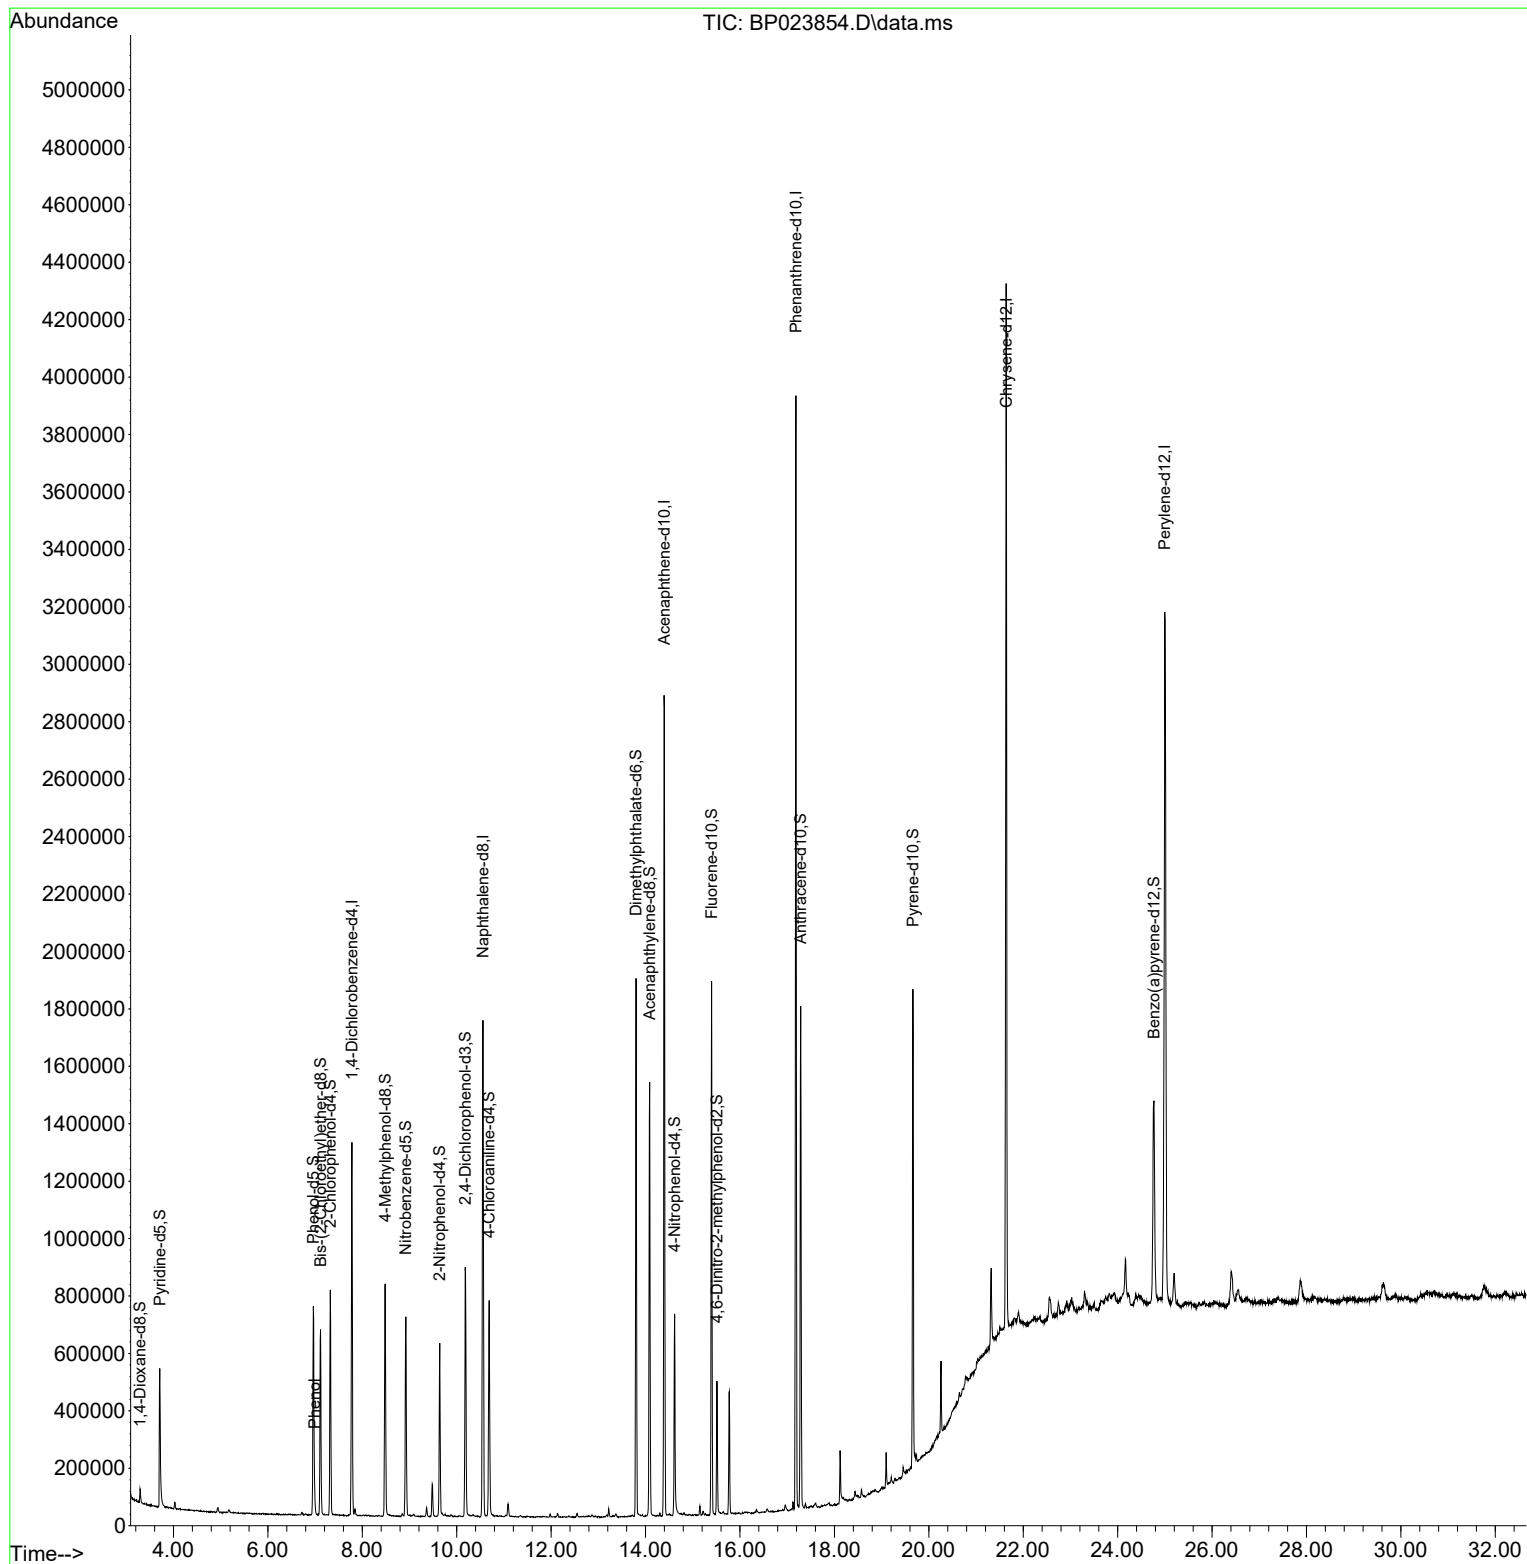

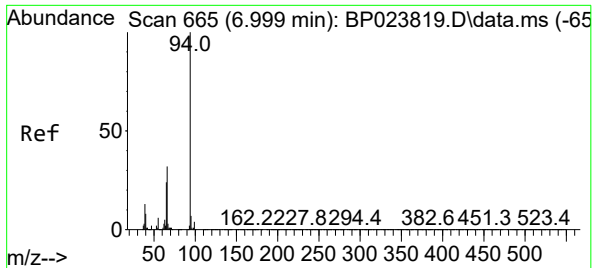

#8
Phenol
Concen: 1.033 ng/ul
RT: 6.993 min Scan# 6
Delta R.T. 0.018 min
Lab File: BP023854.D
Acq: 01 Feb 2025 12:06

Instrument :
BNA_P
ClientSampleId :
A6326

Tgt Ion: 94	Resp:	32298
Ion	Ratio	Lower Upper
94	100	
65	27.9	20.1 30.1
66	37.1	26.0 39.0

