

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
 Data File : BP023856.D
 Acq On : 01 Feb 2025 13:27
 Operator : RC/JU
 Sample : Q1248-06
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A6332

Quant Time: Feb 03 08:23:13 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 31 11:40:55 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	352972	20.000	ng/ul	0.02
20) Naphthalene-d8	10.557	136	1500111	20.000	ng/ul	0.01
38) Acenaphthene-d10	14.404	164	954036	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.192	188	1894854	20.000	ng/ul	-0.02
79) Chrysene-d12	21.639	240	1811312	20.000	ng/ul	0.00
88) Perylene-d12	25.010	264	1933085	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	36482	4.294	ng/uL	0.01
4) Pyridine-d5	3.711	84	476371	19.433	ng/ul	0.02
7) Phenol-d5	6.964	99	647776	20.737	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	7.116	67	381966	23.102	ng/ul	0.02
11) 2-Chlorophenol-d4	7.322	132	541437	22.073	ng/ul	0.01
15) 4-Methylphenol-d8	8.481	113	531121	20.814	ng/ul	0.01
21) Nitrobenzene-d5	8.922	128	251873	20.986	ng/ul	0.01
24) 2-Nitrophenol-d4	9.640	143	251597	19.428	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	10.187	165	462504	19.468	ng/ul	0.01
31) 4-Chloroaniline-d4	10.681	131	628497	17.690	ng/ul	0.00
46) Dimethylphthalate-d6	13.810	166	1521572	21.382	ng/ul	0.00
49) Acenaphthylene-d8	14.087	160	1210127	15.078	ng/ul	0.00
54) 4-Nitrophenol-d4	14.622	143	205655	14.552	ng/ul	0.00
60) Fluorene-d10	15.404	176	756230	12.619	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.516	200	90718	7.760	ng/ul	-0.02
73) Anthracene-d10	17.292	188	1056937	11.360	ng/ul	-0.02
81) Pyrene-d10	19.663	212	833838	8.592	ng/ul	-0.02
92) Benzo(a)pyrene-d12	24.774	264	566950	5.621	ng/ul	-0.01
Target Compounds						
8) Phenol	6.993	94	47685	1.487	ng/ul	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023856.D
Acq On : 01 Feb 2025 13:27
Operator : RC/JU
Sample : Q1248-06
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A6332

Quant Time: Feb 03 08:23:13 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 31 11:40:55 2025
Response via : Initial Calibration

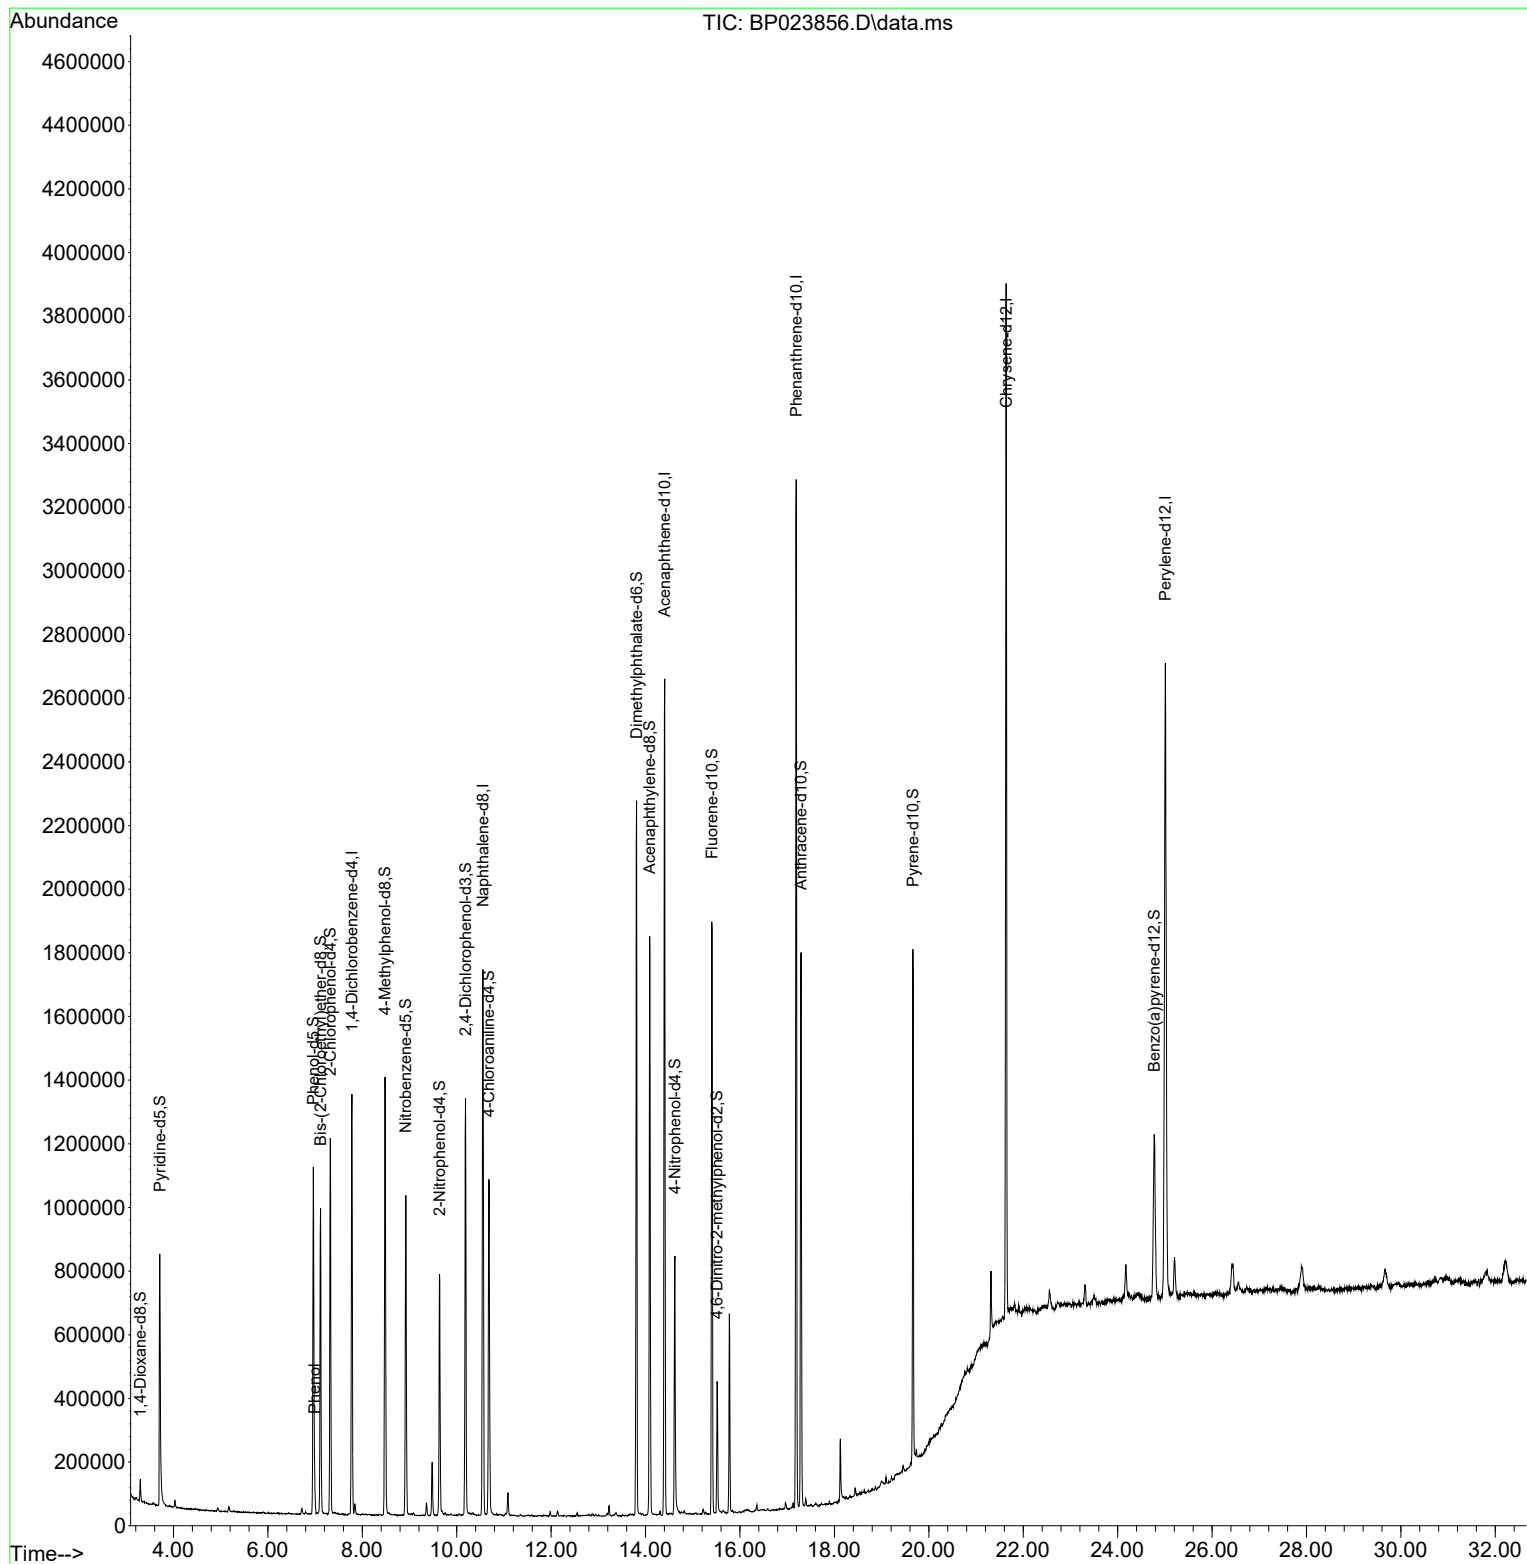

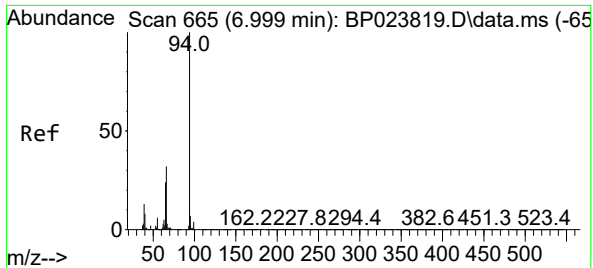

#8
Phenol
Concen: 1.487 ng/ul
RT: 6.993 min Scan# 60
Delta R.T. 0.018 min
Lab File: BP023856.D
Acq: 01 Feb 2025 13:27

Instrument :
BNA_P
ClientSampleId :
A6332

Tgt Ion:	94	Resp:	47685
Ion	Ratio	Lower	Upper
94	100		
65	26.1	20.1	30.1
66	34.7	26.0	39.0

