

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
 Data File : BP023858.D
 Acq On : 01 Feb 2025 14:48
 Operator : RC/JU
 Sample : Q1248-08
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A6334

Quant Time: Feb 03 08:23:42 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 31 11:40:55 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	323163	20.000	ng/ul	0.02
20) Naphthalene-d8	10.551	136	1380488	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.398	164	927010	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.186	188	1954325	20.000	ng/ul	-0.02
79) Chrysene-d12	21.633	240	1925016	20.000	ng/ul	-0.01
88) Perylene-d12	24.986	264	1935817	20.000	ng/ul	-0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	24479	3.147	ng/uL	0.00
4) Pyridine-d5	3.711	84	325951	14.523	ng/ul	0.02
7) Phenol-d5	6.963	99	433750	15.167	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	7.116	67	259040	17.112	ng/ul	0.02
11) 2-Chlorophenol-d4	7.322	132	357151	15.903	ng/ul	0.01
15) 4-Methylphenol-d8	8.481	113	359227	15.376	ng/ul	0.01
21) Nitrobenzene-d5	8.922	128	165501	14.985	ng/ul	0.01
24) 2-Nitrophenol-d4	9.640	143	153667	12.894	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	10.187	165	314077	14.366	ng/ul	0.01
31) 4-Chloroaniline-d4	10.681	131	452623	13.843	ng/ul	0.00
46) Dimethylphthalate-d6	13.804	166	1157319	16.737	ng/ul	0.00
49) Acenaphthylene-d8	14.092	160	853476	10.944	ng/ul	0.00
54) 4-Nitrophenol-d4	14.616	143	138681	10.099	ng/ul	0.00
60) Fluorene-d10	15.404	176	554082	9.516	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.516	200	59341	4.922	ng/ul	-0.02
73) Anthracene-d10	17.286	188	734813	7.658	ng/ul	-0.03
81) Pyrene-d10	19.657	212	661751	6.416	ng/ul	-0.02
92) Benzo(a)pyrene-d12	24.762	264	386513	3.827	ng/ul	-0.02
Target Compounds						
8) Phenol	6.987	94	32102	1.093	ng/ul	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023858.D
Acq On : 01 Feb 2025 14:48
Operator : RC/JU
Sample : Q1248-08
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A6334

Quant Time: Feb 03 08:23:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 31 11:40:55 2025
Response via : Initial Calibration

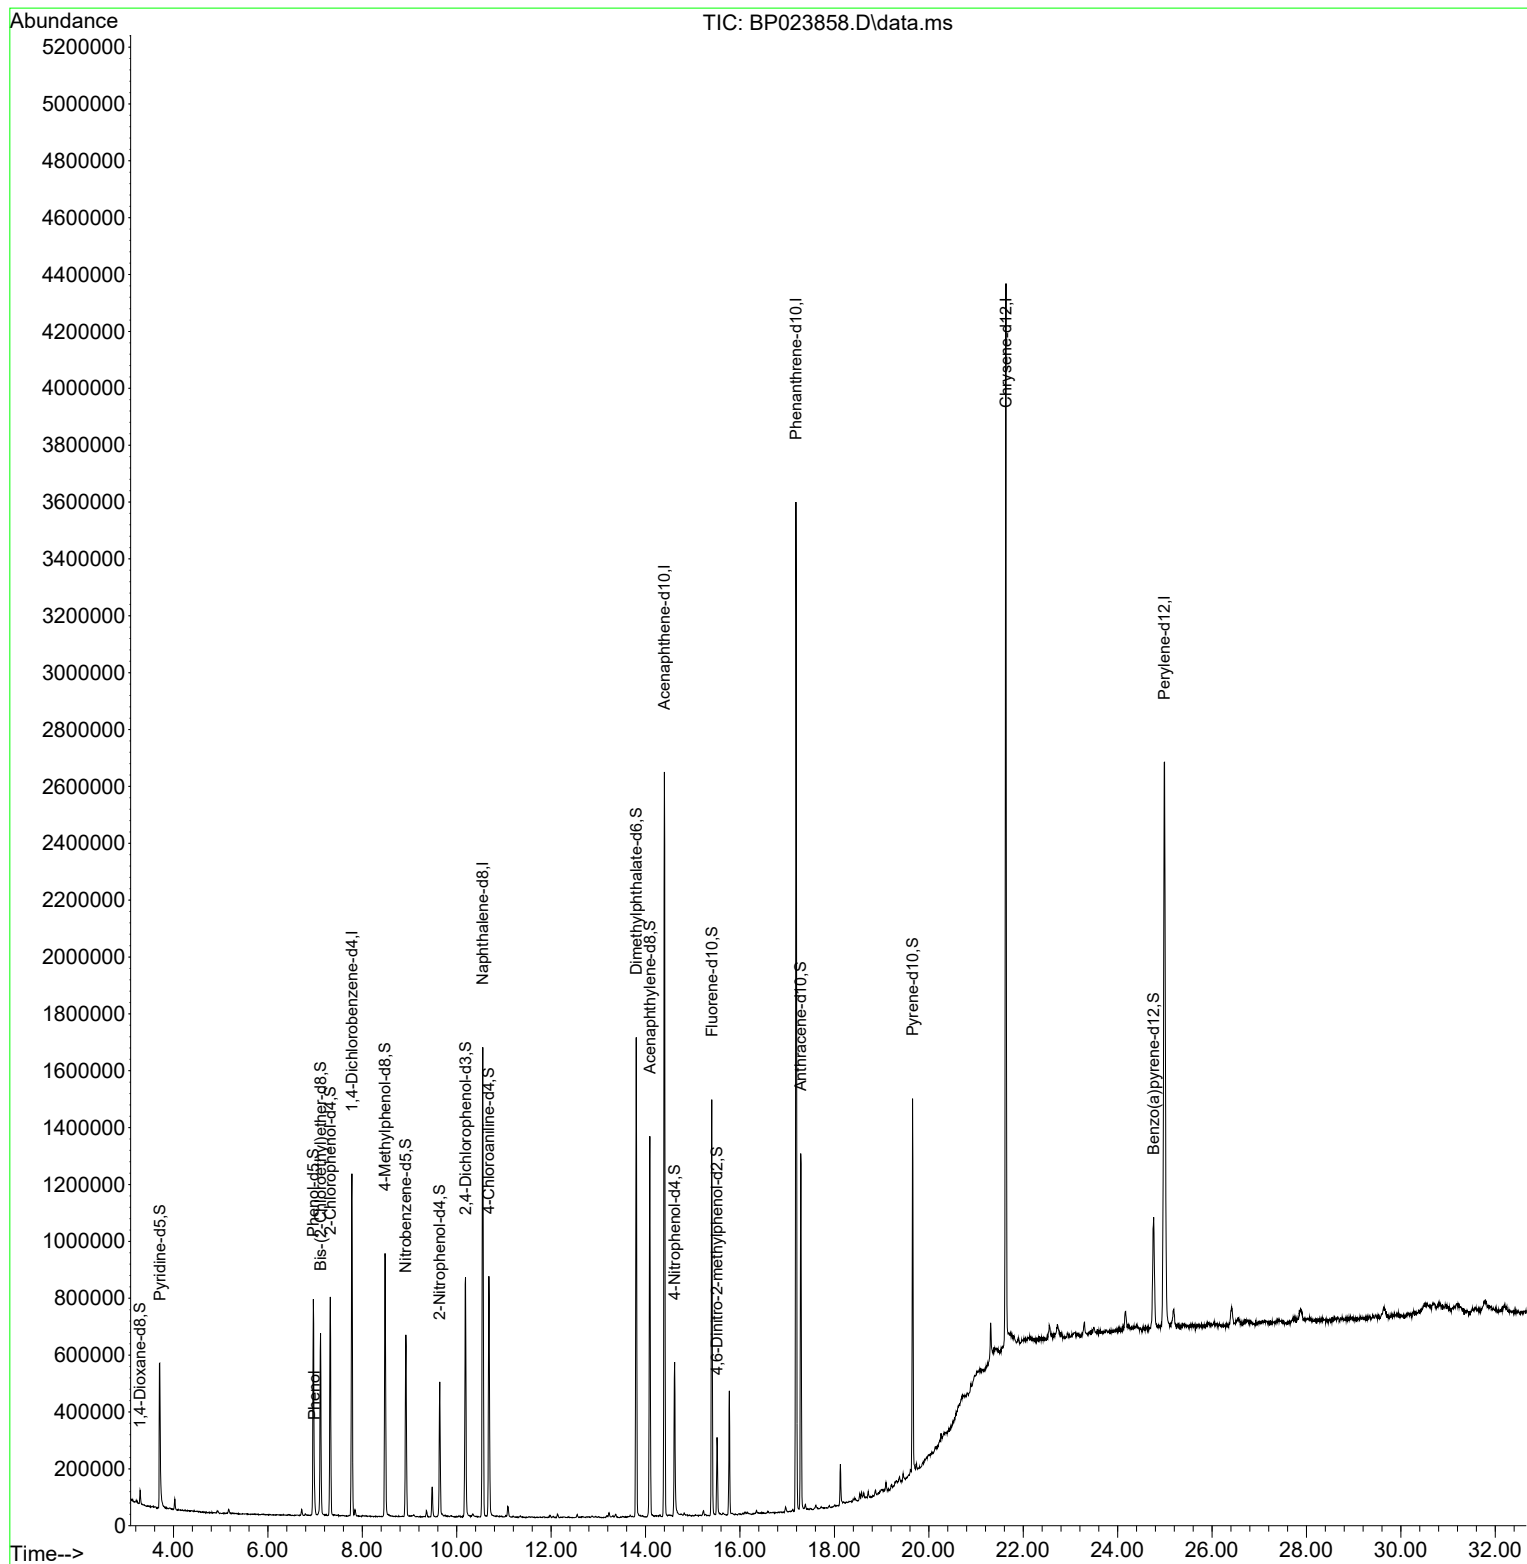

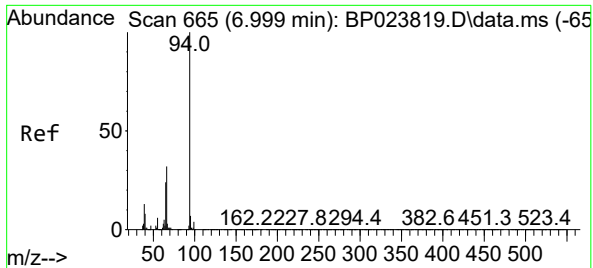

#8
Phenol
Concen: 1.093 ng/ul
RT: 6.987 min Scan# 60
Delta R.T. 0.012 min
Lab File: BP023858.D
Acq: 01 Feb 2025 14:48

Instrument :
BNA_P
ClientSampleId :
A6334

Tgt Ion:	94	Resp:	32102
Ion	Ratio	Lower	Upper
94	100		
65	27.8	20.1	30.1
66	36.5	26.0	39.0

