

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
 Data File : BP023865.D
 Acq On : 01 Feb 2025 20:13
 Operator : RC/JU
 Sample : Q1248-12
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A6343

Quant Time: Feb 03 08:24:23 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 31 11:40:55 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.781	152	362206	20.000	ng/ul	0.02
20) Naphthalene-d8	10.552	136	1558748	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.392	164	1023398	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.192	188	2057996	20.000	ng/ul	-0.02
79) Chrysene-d12	21.627	240	1960033	20.000	ng/ul	-0.02
88) Perylene-d12	24.998	264	1998140	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	29828	3.422	ng/uL	0.01
4) Pyridine-d5	3.705	84	371734	14.778	ng/ul	0.01
7) Phenol-d5	6.963	99	548326	17.106	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	7.111	67	333344	19.647	ng/ul	0.01
11) 2-Chlorophenol-d4	7.322	132	461153	18.321	ng/ul	0.01
15) 4-Methylphenol-d8	8.481	113	459094	17.533	ng/ul	0.01
21) Nitrobenzene-d5	8.922	128	221498	17.761	ng/ul	0.01
24) 2-Nitrophenol-d4	9.634	143	221155	16.435	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.181	165	409503	16.589	ng/ul	0.00
31) 4-Chloroaniline-d4	10.687	131	573707	15.540	ng/ul	0.00
46) Dimethylphthalate-d6	13.798	166	1445812	18.940	ng/ul	0.00
49) Acenaphthylene-d8	14.081	160	1341618	15.583	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.616	143	173126	11.420	ng/ul	0.00
60) Fluorene-d10	15.398	176	956550	14.880	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.522	200	96666	7.614	ng/ul	-0.01
73) Anthracene-d10	17.292	188	1384015	13.697	ng/ul	-0.02
81) Pyrene-d10	19.651	212	1358949	12.940	ng/ul	-0.03
92) Benzo(a)pyrene-d12	24.751	264	997471	9.568	ng/ul	-0.03
Target Compounds						
8) Phenol	6.987	94	38935	1.183	ng/ul	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023865.D
Acq On : 01 Feb 2025 20:13
Operator : RC/JU
Sample : Q1248-12
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A6343

Quant Time: Feb 03 08:24:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 31 11:40:55 2025
Response via : Initial Calibration

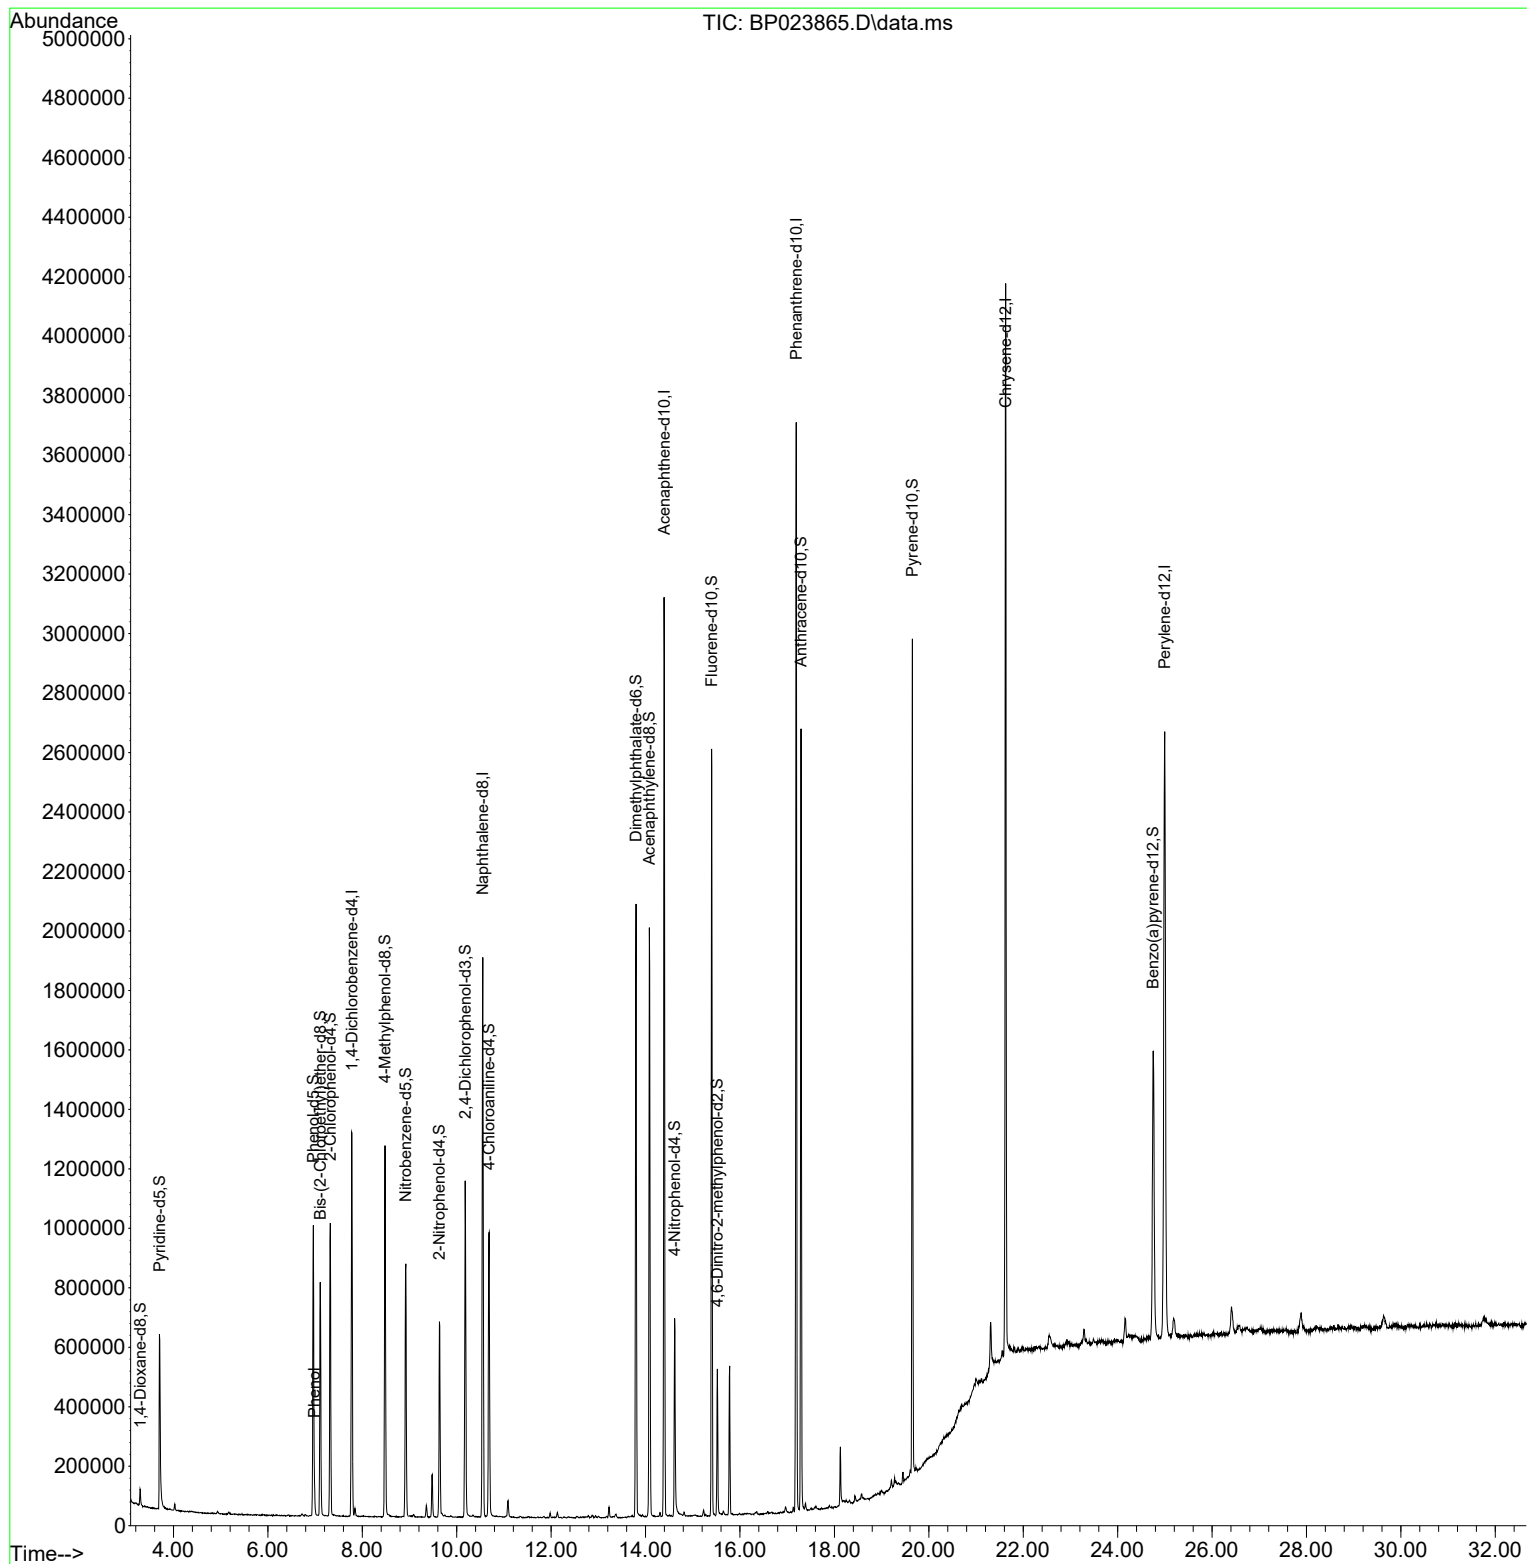

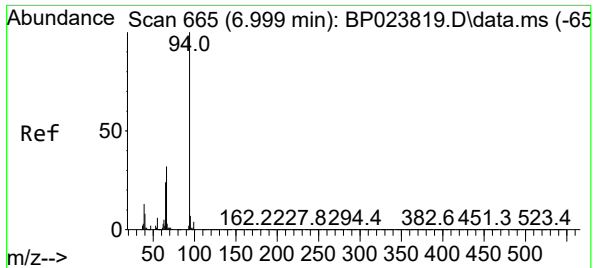

#8
Phenol
Concen: 1.183 ng/ul
RT: 6.987 min Scan# 60
Delta R.T. 0.012 min
Lab File: BP023865.D
Acq: 01 Feb 2025 20:13

Instrument :
BNA_P
ClientSampleId :
A6343

Tgt Ion:	94	Resp:	38935
Ion	Ratio	Lower	Upper
94	100		
65	27.3	20.1	30.1
66	38.7	26.0	39.0

