

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP013125\  
 Data File : BP023868.D  
 Acq On : 01 Feb 2025 22:14  
 Operator : RC/JU  
 Sample : Q1248-15  
 Misc :  
 ALS Vial : 54 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 A6346

Quant Time: Feb 03 08:25:05 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP012925.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Fri Jan 31 11:40:55 2025  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc   | Units | Dev(Min)     |
|-------------------------------|--------|------|----------|--------|-------|--------------|
| Internal Standards            |        |      |          |        |       |              |
| 1) 1,4-Dichlorobenzene-d4     | 7.775  | 152  | 337755   | 20.000 | ng/ul | 0.01         |
| 20) Naphthalene-d8            | 10.551 | 136  | 1448881  | 20.000 | ng/ul | 0.00         |
| 38) Acenaphthene-d10          | 14.392 | 164  | 948713   | 20.000 | ng/ul | 0.00         |
| 64) Phenanthrene-d10          | 17.180 | 188  | 1943383  | 20.000 | ng/ul | -0.03        |
| 79) Chrysene-d12              | 21.621 | 240  | 1926564  | 20.000 | ng/ul | -0.02        |
| 88) Perylene-d12              | 24.986 | 264  | 2060710  | 20.000 | ng/ul | -0.04        |
| System Monitoring Compounds   |        |      |          |        |       |              |
| 3) 1,4-Dioxane-d8             | 3.293  | 96   | 30379    | 3.737  | ng/uL | 0.00         |
| 4) Pyridine-d5                | 3.705  | 84   | 442363   | 18.858 | ng/ul | 0.01         |
| 7) Phenol-d5                  | 6.963  | 99   | 580715   | 19.428 | ng/ul | 0.02         |
| 9) Bis-(2-Chloroethyl)eth...  | 7.110  | 67   | 330224   | 20.872 | ng/ul | 0.01         |
| 11) 2-Chlorophenol-d4         | 7.322  | 132  | 464419   | 19.786 | ng/ul | 0.01         |
| 15) 4-Methylphenol-d8         | 8.481  | 113  | 477923   | 19.573 | ng/ul | 0.01         |
| 21) Nitrobenzene-d5           | 8.922  | 128  | 218091   | 18.814 | ng/ul | 0.01         |
| 24) 2-Nitrophenol-d4          | 9.634  | 143  | 221060   | 17.673 | ng/ul | 0.00         |
| 28) 2,4-Dichlorophenol-d3     | 10.181 | 165  | 429832   | 18.732 | ng/ul | 0.00         |
| 31) 4-Chloroaniline-d4        | 10.681 | 131  | 637154   | 18.567 | ng/ul | 0.00         |
| 46) Dimethylphthalate-d6      | 13.798 | 166  | 1455366  | 20.566 | ng/ul | 0.00         |
| 49) Acenaphthylene-d8         | 14.086 | 160  | 1392016  | 17.441 | ng/ul | 0.00         |
| 54) 4-Nitrophenol-d4          | 14.604 | 143  | 206267   | 14.677 | ng/ul | -0.02        |
| 60) Fluorene-d10              | 15.392 | 176  | 982775   | 16.492 | ng/ul | -0.02        |
| 65) 4,6-Dinitro-2-methylph... | 15.510 | 200  | 88919    | 7.417  | ng/ul | -0.02        |
| 73) Anthracene-d10            | 17.286 | 188  | 1459669  | 15.297 | ng/ul | -0.03        |
| 81) Pyrene-d10                | 19.645 | 212  | 1425777  | 13.812 | ng/ul | -0.04        |
| 92) Benzo(a)pyrene-d12        | 24.745 | 264  | 1100699  | 10.237 | ng/ul | -0.04        |
| Target Compounds              |        |      |          |        |       |              |
| 8) Phenol                     | 6.987  | 94   | 38279    | 1.247  | ng/ul | Qvalue<br>95 |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP013125\  
Data File : BP023868.D  
Acq On : 01 Feb 2025 22:14  
Operator : RC/JU  
Sample : Q1248-15  
Misc :  
ALS Vial : 54 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
A6346

Quant Time: Feb 03 08:25:05 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP012925.MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Fri Jan 31 11:40:55 2025  
Response via : Initial Calibration

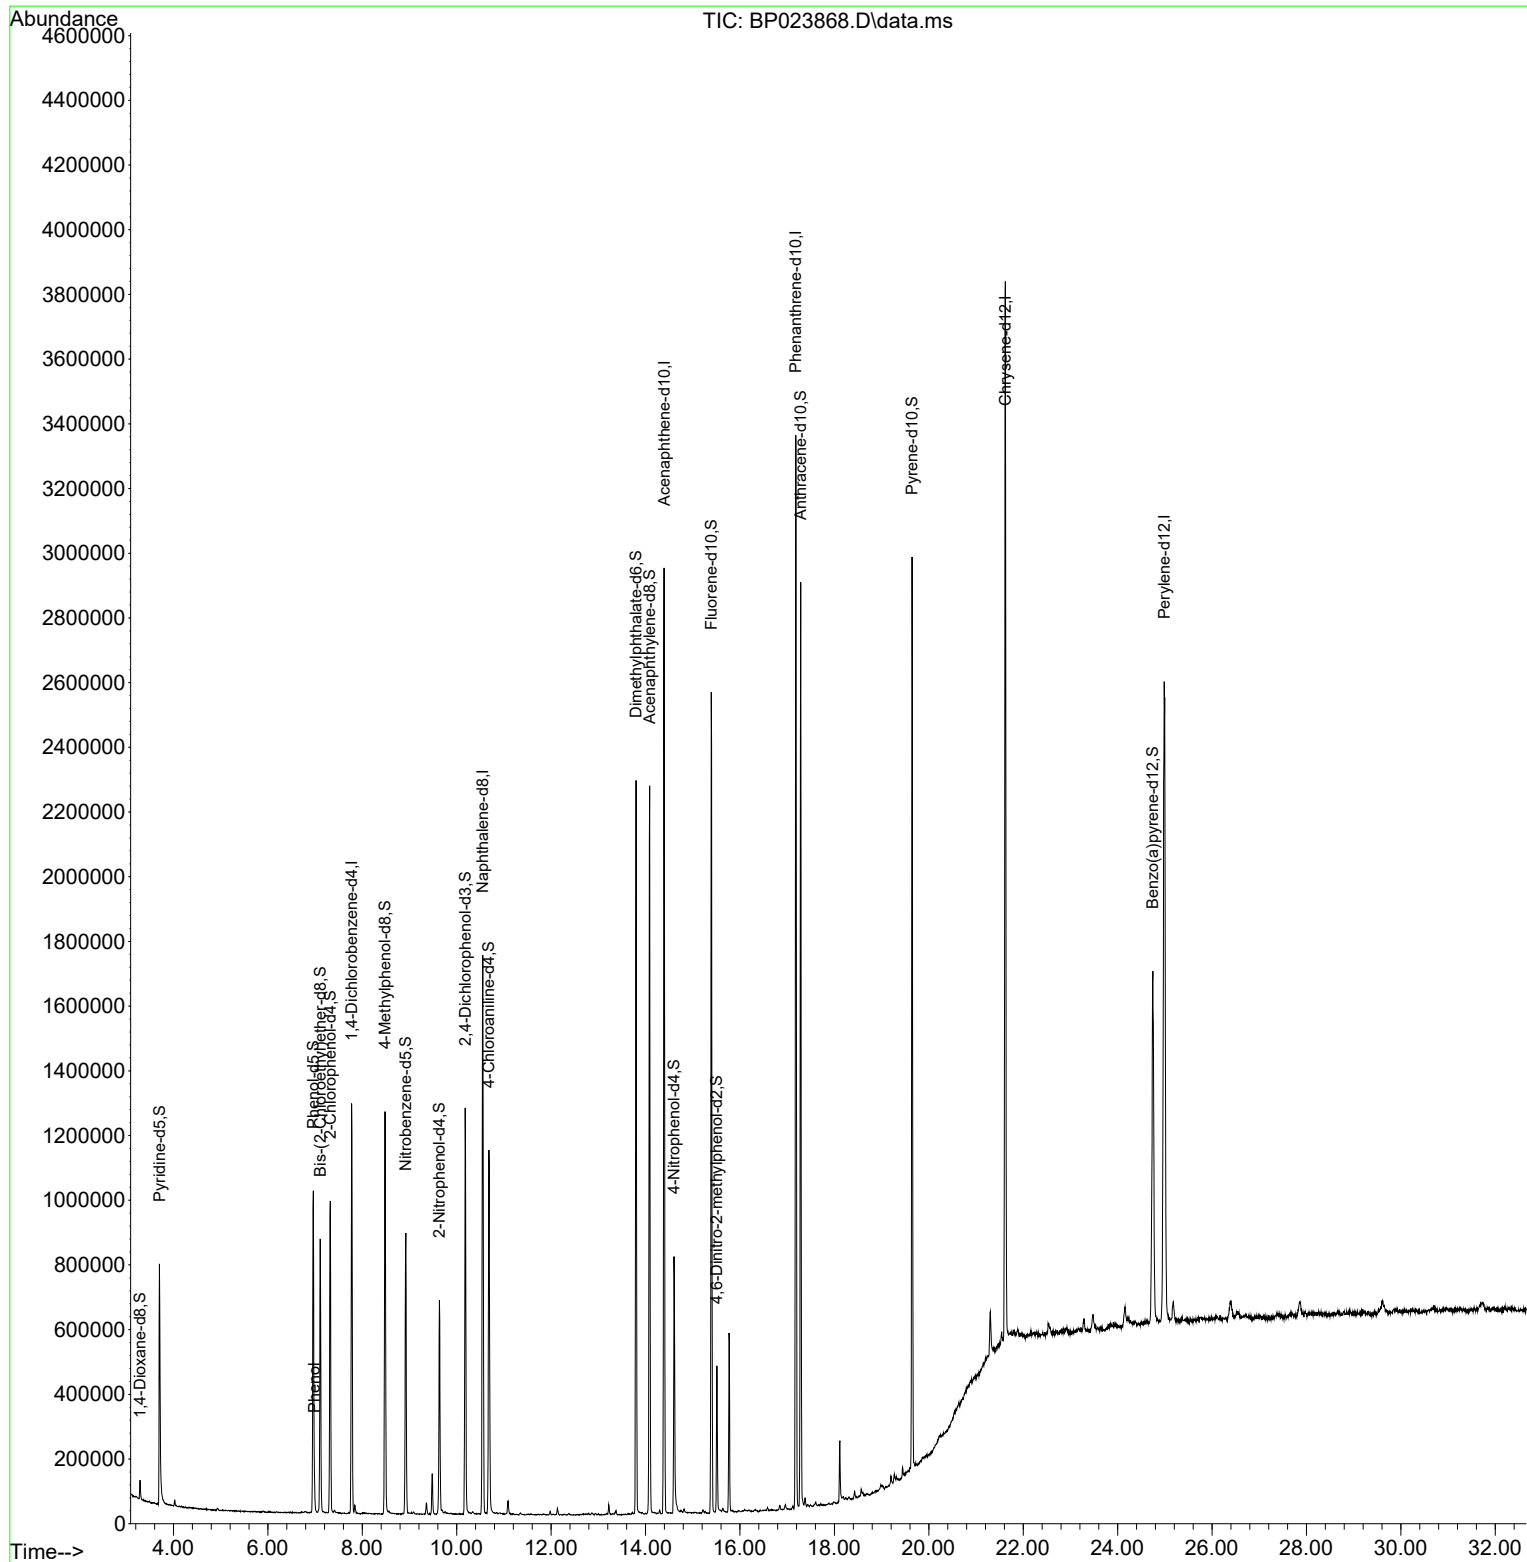

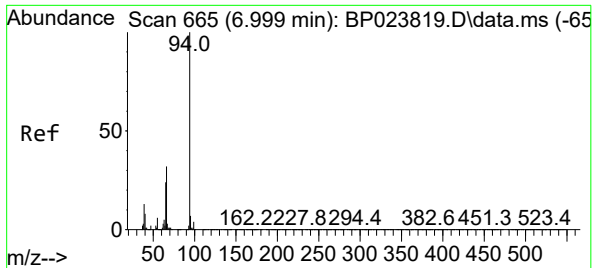

#8  
Phenol  
Concen: 1.247 ng/ul  
RT: 6.987 min Scan# 60  
Delta R.T. 0.012 min  
Lab File: BP023868.D  
Acq: 01 Feb 2025 22:14

Instrument :  
BNA\_P  
ClientSampleId :  
A6346

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 94    | Resp: | 38279 |
| Ion      | Ratio | Lower | Upper |
| 94       | 100   |       |       |
| 65       | 27.8  | 20.1  | 30.1  |
| 66       | 34.6  | 26.0  | 39.0  |

