

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
 Data File : BP023869.D
 Acq On : 01 Feb 2025 22:55
 Operator : RC/JU
 Sample : Q1248-16
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A6347

Quant Time: Feb 03 08:25:19 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 31 11:40:55 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.775	152	364786	20.000	ng/ul	0.01
20) Naphthalene-d8	10.546	136	1562309	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.398	164	1023881	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.186	188	2085192	20.000	ng/ul	-0.02
79) Chrysene-d12	21.627	240	1982673	20.000	ng/ul	-0.02
88) Perylene-d12	24.980	264	2021960	20.000	ng/ul	-0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	29240	3.330	ng/uL	0.00
4) Pyridine-d5	3.705	84	361112	14.254	ng/ul	0.01
7) Phenol-d5	6.958	99	532635	16.499	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.111	67	306188	17.919	ng/ul	0.01
11) 2-Chlorophenol-d4	7.316	132	438597	17.301	ng/ul	0.00
15) 4-Methylphenol-d8	8.481	113	432252	16.391	ng/ul	0.01
21) Nitrobenzene-d5	8.916	128	199290	15.944	ng/ul	0.00
24) 2-Nitrophenol-d4	9.634	143	198245	14.699	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.175	165	374829	15.149	ng/ul	0.00
31) 4-Chloroaniline-d4	10.681	131	514945	13.917	ng/ul	0.00
46) Dimethylphthalate-d6	13.798	166	1207498	15.811	ng/ul	0.00
49) Acenaphthylene-d8	14.081	160	997398	11.579	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.610	143	141204	9.310	ng/ul	-0.01
60) Fluorene-d10	15.392	176	662143	10.295	ng/ul	-0.02
65) 4,6-Dinitro-2-methylph...	15.504	200	72466	5.633	ng/ul	-0.03
73) Anthracene-d10	17.292	188	1001243	9.779	ng/ul	-0.02
81) Pyrene-d10	19.669	212	843673	7.942	ng/ul	-0.01
92) Benzo(a)pyrene-d12	24.763	264	682360	6.468	ng/ul	-0.02
Target Compounds						
					Qvalue	
8) Phenol	6.987	94	40436	1.220	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023869.D
Acq On : 01 Feb 2025 22:55
Operator : RC/JU
Sample : Q1248-16
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A6347

Quant Time: Feb 03 08:25:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 31 11:40:55 2025
Response via : Initial Calibration

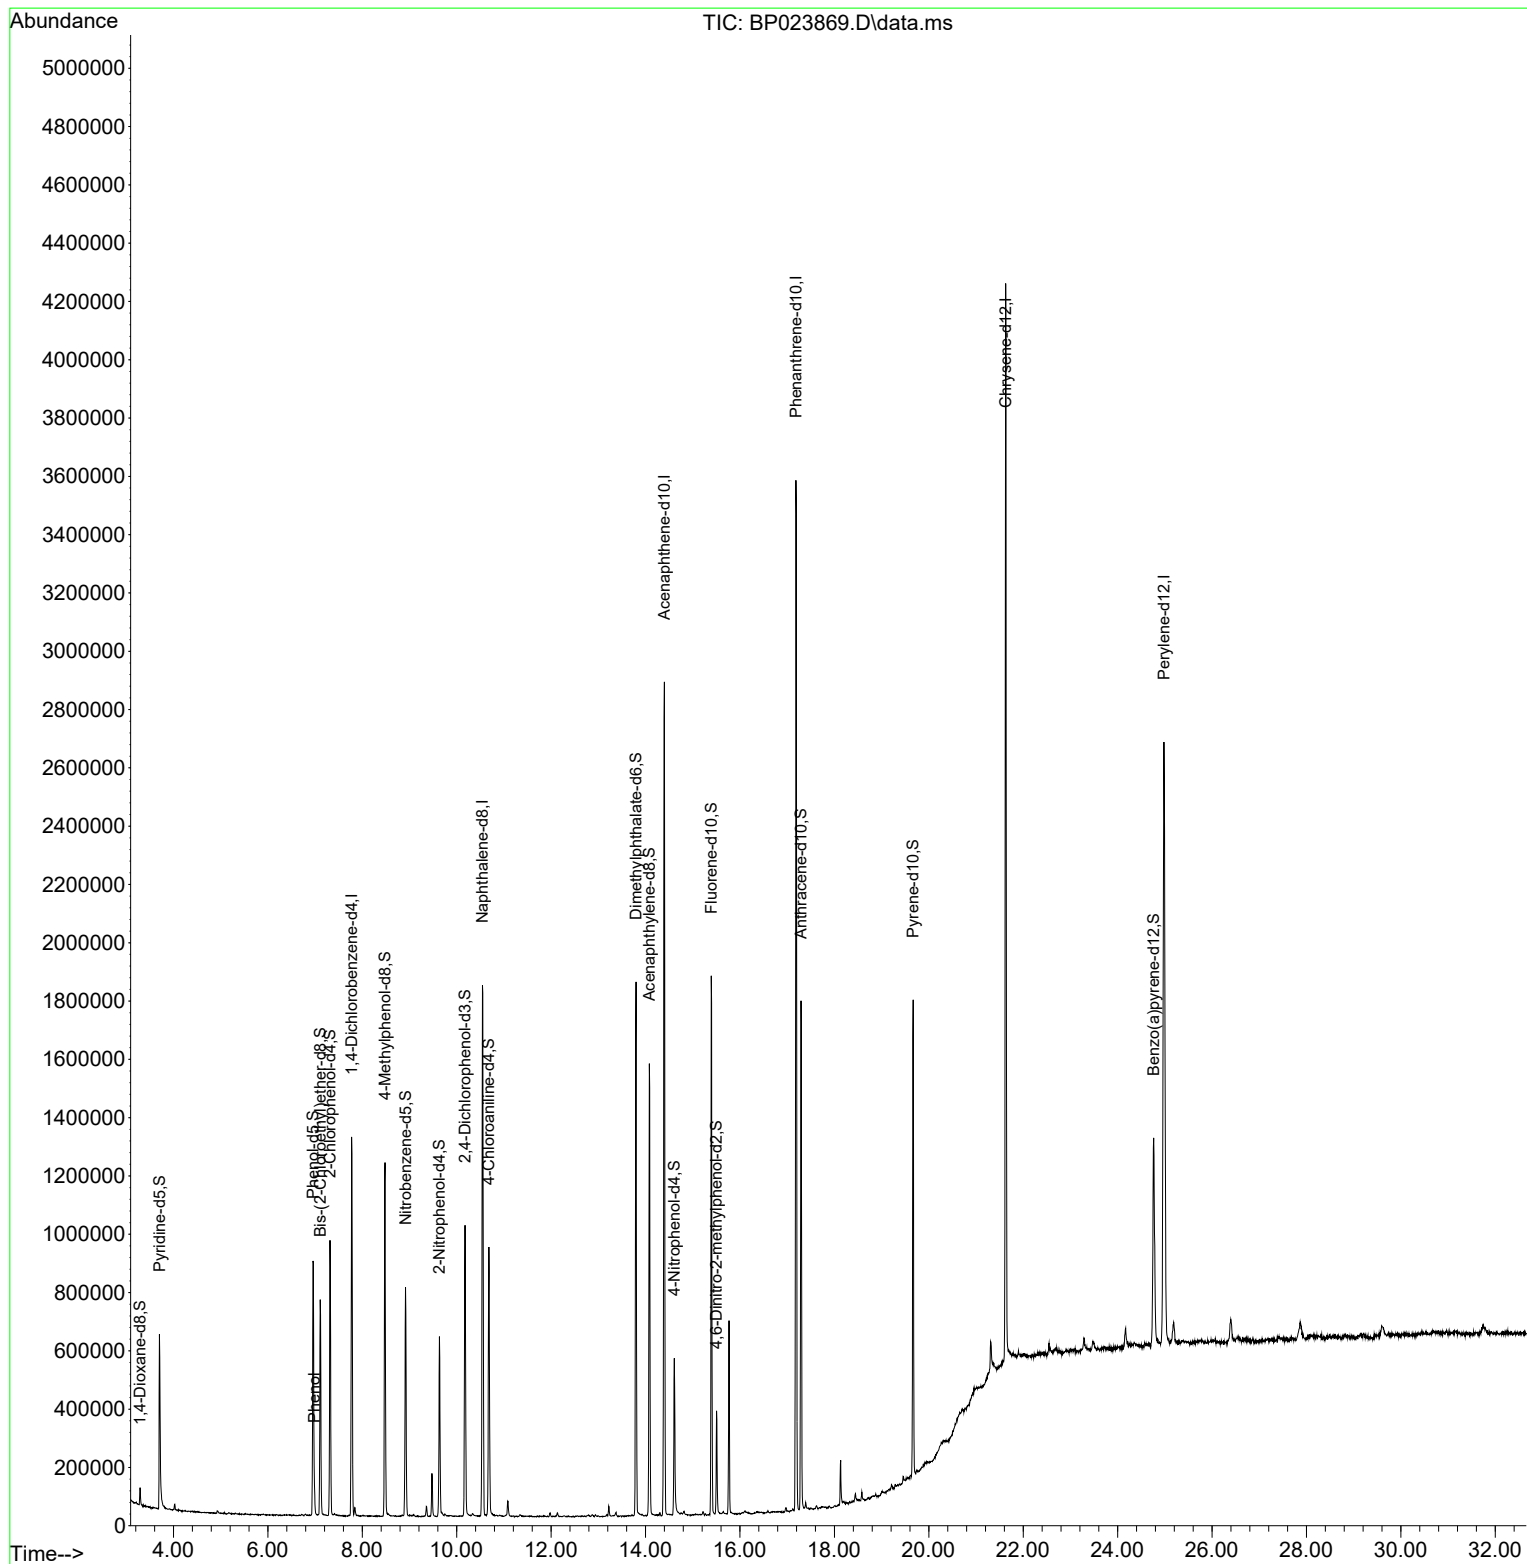

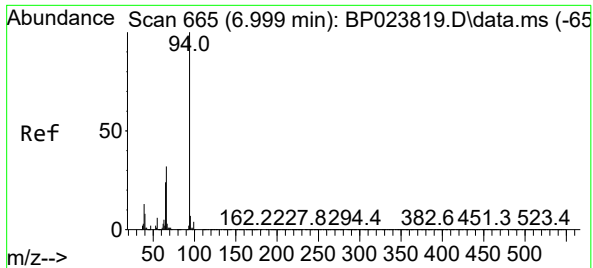

#8
Phenol
Concen: 1.220 ng/ul
RT: 6.987 min Scan# 60
Delta R.T. 0.012 min
Lab File: BP023869.D
Acq: 01 Feb 2025 22:55

Instrument :
BNA_P
ClientSampleId :
A6347

Tgt Ion:	94	Resp:	40436
Ion	Ratio	Lower	Upper
94	100		
65	25.8	20.1	30.1
66	33.3	26.0	39.0

