

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
 Data File : BP023820.D
 Acq On : 31 Jan 2025 11:16
 Operator : RC/JU
 Sample : PB166295BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK295

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023820.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	44	rVB	122313	169390	1.42%	0.151%
2	3.711	102	106	128	rBV	1556552	2304725	19.36%	2.058%
3	4.028	156	160	167	rVB	25808	36260	0.30%	0.032%
4	6.969	653	660	672	rBV	1861395	2932964	24.64%	2.619%
5	7.116	679	685	696	rVB	1424641	2146576	18.03%	1.917%
6	7.328	713	721	732	rBV	1946229	2975179	24.99%	2.656%
7	7.781	789	798	805	rBV	1291402	1970206	16.55%	1.759%
8	8.493	907	919	934	rBV	2488504	3830239	32.18%	3.420%
9	8.928	985	993	1006	rBV	1507670	2519298	21.16%	2.249%
10	9.063	1012	1016	1020	rBV3	11489	16041	0.13%	0.014%
11	9.646	1107	1115	1127	rBV	1288054	2082542	17.49%	1.859%
12	10.193	1199	1208	1220	rBV	2183885	3771789	31.69%	3.368%
13	10.557	1262	1270	1281	rBV	1680809	2805351	23.57%	2.505%
14	10.687	1284	1292	1308	rBV	2252101	3611328	30.34%	3.224%
15	11.357	1399	1406	1411	rBV10	7263	15053	0.13%	0.013%
16	12.140	1533	1539	1546	rBV	35507	59326	0.50%	0.053%
17	13.369	1742	1748	1753	rVB5	7039	13075	0.11%	0.012%
18	13.804	1815	1822	1838	rBV	3685441	5645934	47.43%	5.041%
19	14.093	1864	1871	1885	rBV	4540447	6762454	56.81%	6.038%
20	14.404	1918	1924	1933	rBV	3077714	4098879	34.43%	3.660%
21	14.634	1954	1963	1982	rBV	1588794	2609878	21.92%	2.330%
22	14.757	1982	1984	1992	rVB9	9550	23236	0.20%	0.021%
23	15.075	2034	2038	2045	rVB9	9299	13306	0.11%	0.012%
24	15.240	2061	2066	2070	rVB4	8154	12875	0.11%	0.011%
25	15.410	2088	2095	2107	rBV	6167147	8581547	72.09%	7.662%
26	15.522	2107	2114	2128	rVV	1481472	2141285	17.99%	1.912%
27	15.657	2133	2137	2142	rVB2	25525	41079	0.35%	0.037%
28	16.969	2356	2360	2367	rBV2	17424	27865	0.23%	0.025%
29	17.198	2392	2399	2408	rBV	3812411	5189395	43.59%	4.633%
30	17.292	2409	2415	2431	rVB	7663705	9876108	82.96%	8.818%
31	18.139	2556	2559	2563	rBV4	16813	23621	0.20%	0.021%
32	19.210	2738	2741	2747	rVB2	83713	108824	0.91%	0.097%
33	19.286	2750	2754	2758	rVB	65473	90576	0.76%	0.081%
34	19.663	2812	2818	2828	rBV	8460216	11675130	98.08%	10.424%
35	21.639	3149	3154	3166	rVB	3522149	5799217	48.72%	5.178%
36	24.792	3681	3690	3703	rVB	4211104	11903957	100.00%	10.629%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023820.D
Acq On : 31 Jan 2025 11:16
Operator : RC/JU
Sample : PB166295BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK295

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Title : SVOA CALIBRATION

37 25.027 3723 3730 3743 rVB 2284959 6114679 51.37% 5.460%




Sum of corrected areas: 111999187

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023820.D
Acq On : 31 Jan 2025 11:16
Operator : RC/JU
Sample : PB166295BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK295

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

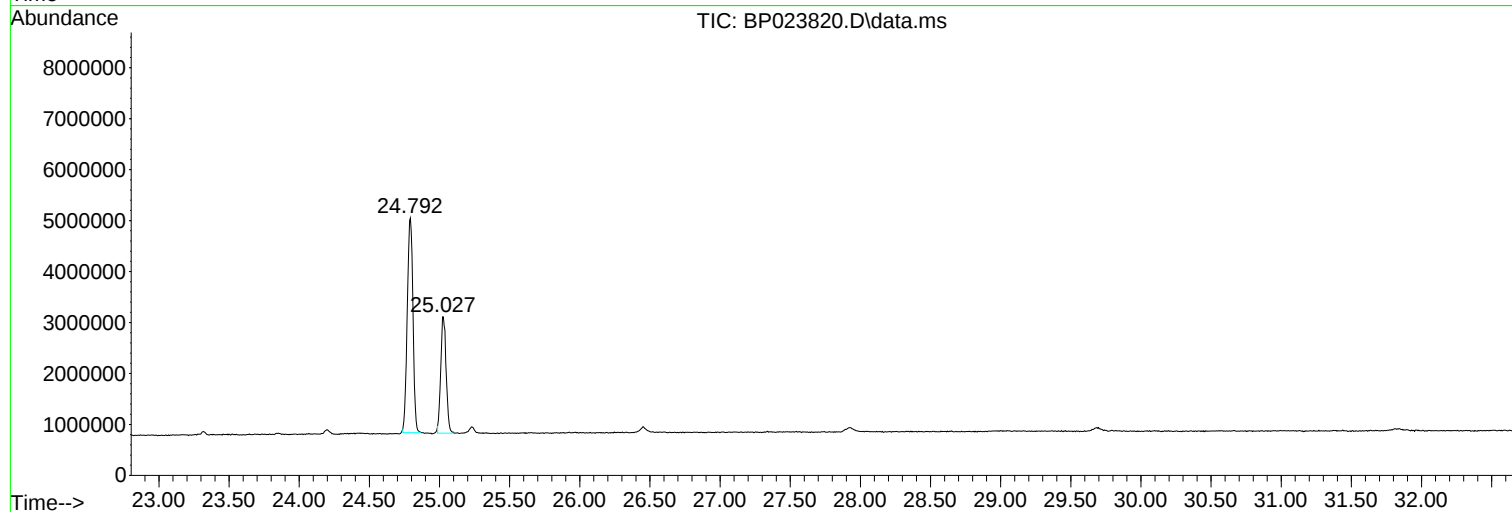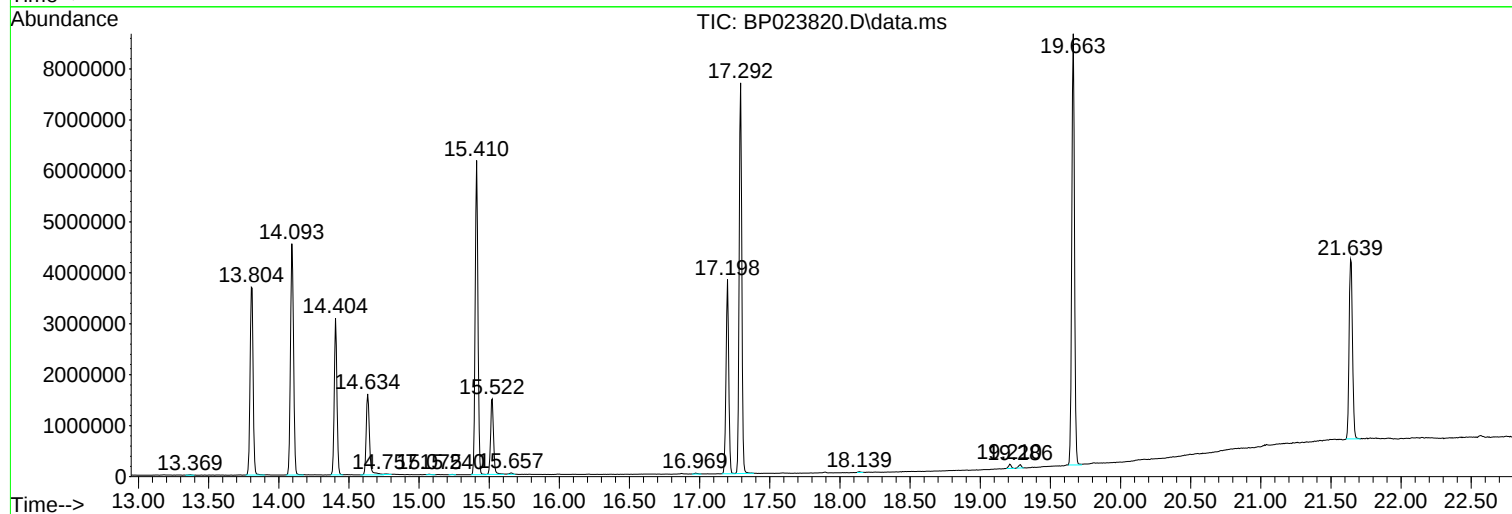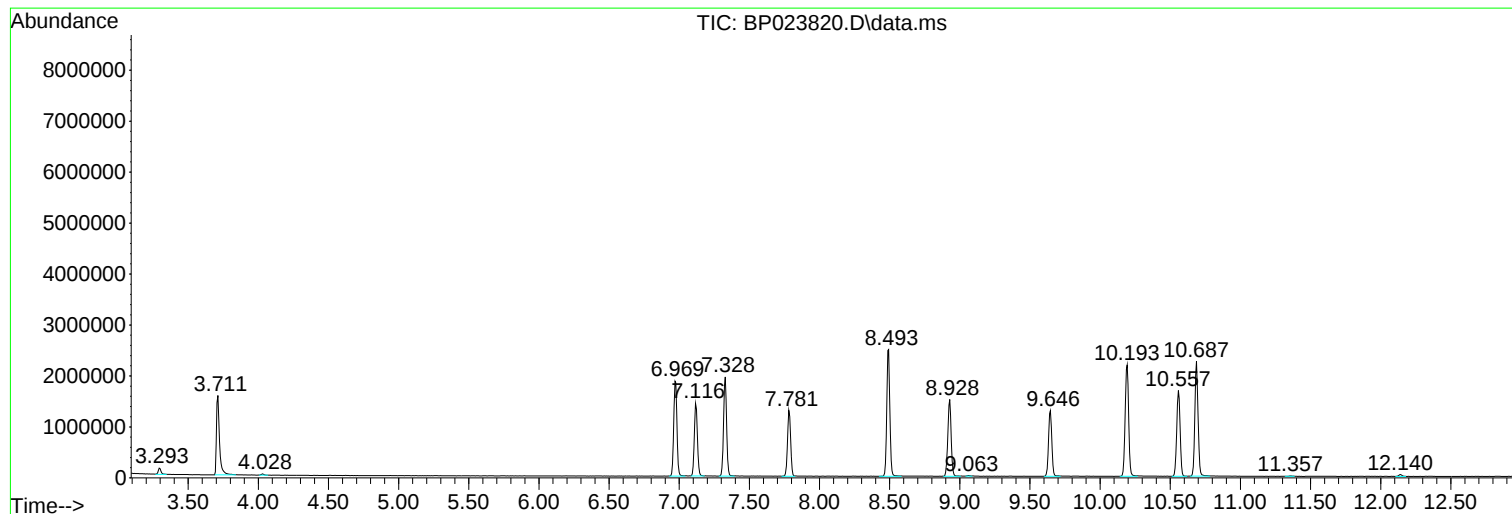

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023820.D
Acq On : 31 Jan 2025 11:16
Operator : RC/JU
Sample : PB166295BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK295

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023820.D
Acq On : 31 Jan 2025 11:16
Operator : RC/JU
Sample : PB166295BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK295

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc