

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
 Data File : BP023822.D
 Acq On : 31 Jan 2025 12:38
 Operator : RC/JU
 Sample : Q1197-14
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E2992

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023822.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	32	36	44	rVB	125116	159291	1.02%	0.120%
2	3.711	103	106	121	rBV	577872	934267	6.00%	0.703%
3	4.034	157	161	165	rVB	21232	28896	0.19%	0.022%
4	4.940	312	315	320	rVB2	18948	29145	0.19%	0.022%
5	6.975	651	661	671	rBV	728289	1194336	7.67%	0.898%
6	7.122	679	686	698	rBV	1607056	2668243	17.14%	2.007%
7	7.328	714	721	733	rBV	2053780	3177682	20.41%	2.390%
8	7.416	733	736	744	rVB7	9793	18592	0.12%	0.014%
9	7.787	791	799	806	rBV	1519610	2435654	15.65%	1.832%
10	7.858	806	811	816	rVB	13925	20922	0.13%	0.016%
11	8.493	912	919	929	rBV	2080891	3220792	20.69%	2.422%
12	8.928	980	993	1004	rBV	2046288	3208108	20.61%	2.413%
13	9.063	1012	1016	1020	rBV3	11712	17000	0.11%	0.013%
14	9.369	1062	1068	1075	rVB	36132	57813	0.37%	0.043%
15	9.640	1105	1114	1128	rBV	1609013	2669952	17.15%	2.008%
16	10.193	1198	1208	1221	rBV	2547467	4341293	27.89%	3.265%
17	10.557	1263	1270	1278	rVB	2267095	3578505	22.99%	2.691%
18	10.693	1285	1293	1313	rBV	2435497	4147973	26.65%	3.120%
19	11.987	1509	1513	1517	rVB7	10242	16539	0.11%	0.012%
20	12.081	1524	1529	1534	rBV3	15893	29490	0.19%	0.022%
21	12.146	1534	1540	1545	rVB	40738	70556	0.45%	0.053%
22	13.010	1682	1687	1692	rVB	18109	29096	0.19%	0.022%
23	13.228	1717	1724	1729	rVB2	24693	34243	0.22%	0.026%
24	13.363	1744	1747	1753	rVB5	16602	26533	0.17%	0.020%
25	13.804	1813	1822	1833	rBV	5511336	7195459	46.22%	5.411%
26	14.093	1861	1871	1883	rBV	5759175	8365435	53.74%	6.291%
27	14.310	1904	1908	1912	rVB3	11936	16412	0.11%	0.012%
28	14.398	1915	1923	1932	rVV	3444514	5068281	32.56%	3.812%
29	14.481	1934	1937	1945	rVB10	9900	17286	0.11%	0.013%
30	14.628	1954	1962	1975	rBV	796006	1209635	7.77%	0.910%
31	14.822	1991	1995	2001	rVB8	15048	24451	0.16%	0.018%
32	15.404	2087	2094	2102	rBV	7243833	11328386	72.77%	8.520%
33	15.522	2107	2114	2127	rVV	2387914	3235776	20.79%	2.433%
34	15.645	2131	2135	2140	rVB2	34535	58235	0.37%	0.044%
35	15.781	2152	2158	2162	rBV	83117	118038	0.76%	0.089%
36	15.904	2176	2179	2184	rVB7	12480	17257	0.11%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023822.D
Acq On : 31 Jan 2025 12:38
Operator : RC/JU
Sample : Q1197-14
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2992

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Title : SVOA CALIBRATION

37	16.975	2356	2361	2367	rBV4	21516	39744	0.26%	0.030%
38	17.192	2391	2398	2408	rBV2	4154934	6029807	38.73%	4.535%
39	17.292	2408	2415	2428	rBV	9571969	13106631	84.19%	9.857%
40	18.128	2554	2557	2562	rBV4	34852	47740	0.31%	0.036%
41	19.210	2737	2741	2747	rBV	118614	160692	1.03%	0.121%
42	19.281	2750	2753	2758	rVV	93617	129669	0.83%	0.098%
43	19.663	2812	2818	2828	rBV	11399701	15567386	100.00%	11.708%
44	21.639	3148	3154	3161	rBV	4418667	6664769	42.81%	5.012%
45	24.792	3680	3690	3707	rVB	5565220	15531605	99.77%	11.681%
46	25.016	3721	3728	3741	rVB	2627965	6921212	44.46%	5.205%




Sum of corrected areas: 132968827

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023822.D
Acq On : 31 Jan 2025 12:38
Operator : RC/JU
Sample : Q1197-14
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2992

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

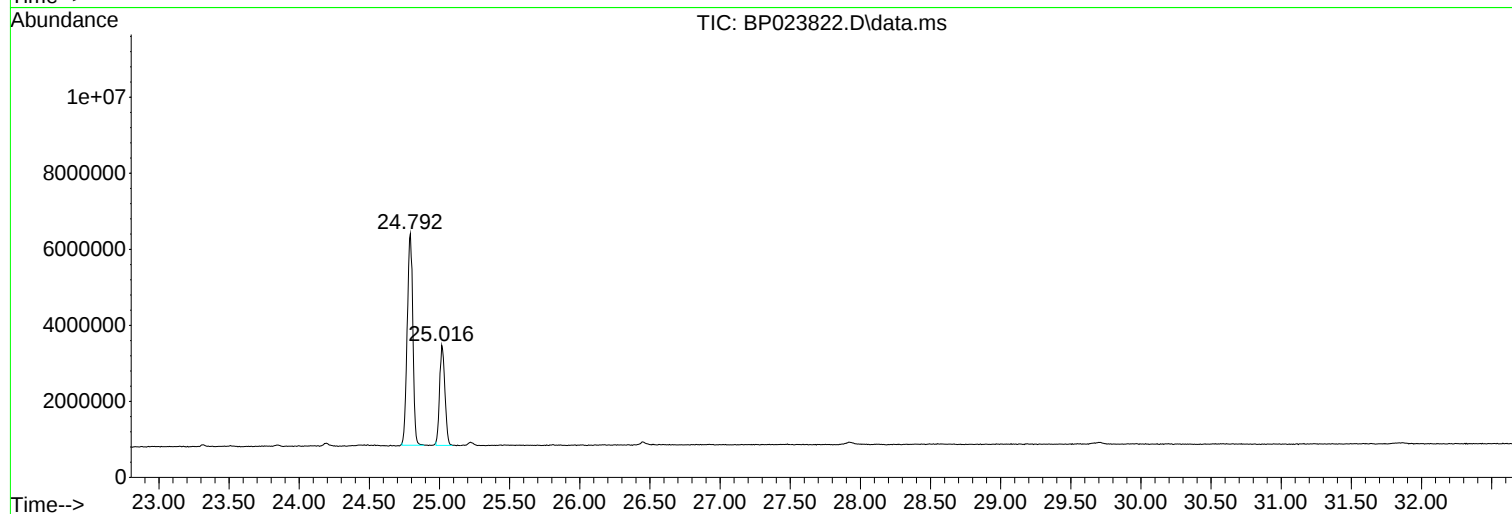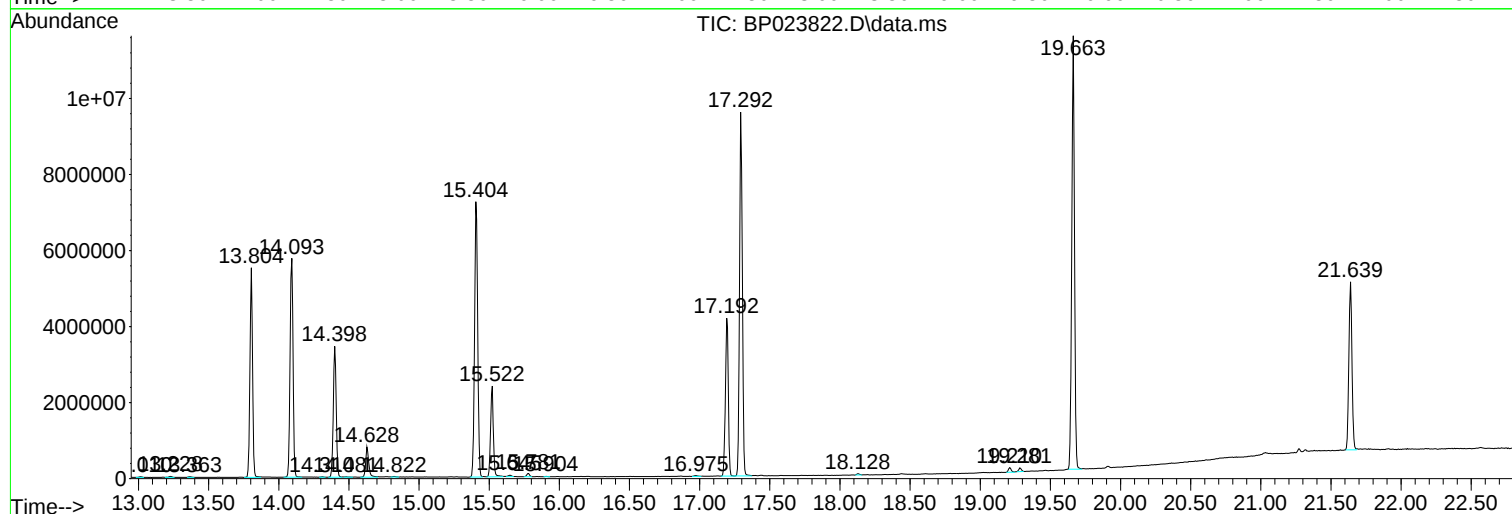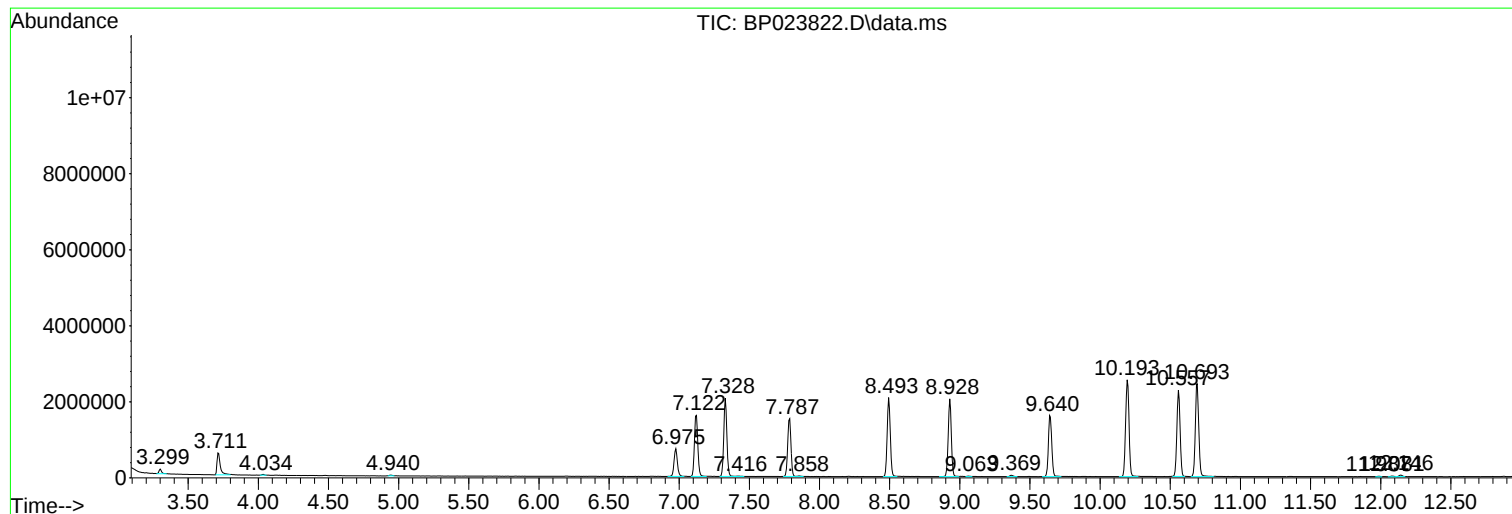

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023822.D
Acq On : 31 Jan 2025 12:38
Operator : RC/JU
Sample : Q1197-14
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2992

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023822.D
Acq On : 31 Jan 2025 12:38
Operator : RC/JU
Sample : Q1197-14
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E2992

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc