

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
 Data File : BP023836.D
 Acq On : 31 Jan 2025 22:48
 Operator : RC/JU
 Sample : PB166393BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK393

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023836.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	42	rVB	117878	149767	1.20%	0.119%
2	3.705	101	105	121	rBV	1619806	2325334	18.57%	1.853%
3	4.028	156	160	166	rVB	30139	40735	0.33%	0.032%
4	6.969	651	660	672	rBV	2050368	3102203	24.77%	2.472%
5	7.111	676	684	694	rVV	1550526	2304550	18.40%	1.837%
6	7.322	713	720	732	rBV	2051884	3098919	24.75%	2.470%
7	7.781	790	798	808	rBV	1495567	2480464	19.81%	1.977%
8	8.487	910	918	938	rBV	2584575	4008492	32.01%	3.195%
9	8.922	984	992	1002	rBV	1645035	2713587	21.67%	2.163%
10	9.058	1010	1015	1019	rBV2	20505	32583	0.26%	0.026%
11	9.640	1105	1114	1124	rBV	1392136	2180401	17.41%	1.738%
12	10.187	1199	1207	1224	rBV	2568090	3959614	31.62%	3.156%
13	10.558	1262	1270	1283	rBV	2266908	3723888	29.74%	2.968%
14	10.693	1285	1293	1307	rBV	2317825	3895685	31.11%	3.105%
15	12.146	1534	1540	1547	rVB2	35951	66176	0.53%	0.053%
16	13.375	1743	1749	1755	rVB7	9011	19751	0.16%	0.016%
17	13.810	1816	1823	1832	rBV	4366967	5986844	47.81%	4.772%
18	14.099	1862	1872	1884	rBV	5060917	7213242	57.60%	5.749%
19	14.404	1918	1924	1933	rBV	4055289	5500377	43.92%	4.384%
20	14.628	1954	1962	1979	rBV	1654342	2877201	22.98%	2.293%
21	14.822	1993	1995	2001	rVB7	11008	15301	0.12%	0.012%
22	15.075	2034	2038	2045	rVB8	6531	12919	0.10%	0.010%
23	15.416	2088	2096	2105	rBV	6051493	9171448	73.24%	7.310%
24	15.522	2107	2114	2129	rVV	1379234	2106503	16.82%	1.679%
25	15.651	2132	2136	2144	rVB4	27682	53869	0.43%	0.043%
26	16.210	2228	2231	2236	rVB5	8785	12757	0.10%	0.010%
27	16.987	2358	2363	2369	rVB	20448	29578	0.24%	0.024%
28	17.204	2393	2400	2410	rBV2	4353179	6842362	54.64%	5.453%
29	17.304	2411	2417	2432	rVV	8517292	10511954	83.94%	8.378%
30	18.139	2556	2559	2563	rBV4	14327	20267	0.16%	0.016%
31	19.216	2738	2742	2748	rBV3	75038	122189	0.98%	0.097%
32	19.292	2751	2755	2762	rVV2	73316	115546	0.92%	0.092%
33	19.669	2813	2819	2830	rBV2	9355181	12417851	99.16%	9.897%
34	21.639	3148	3154	3167	rBV	5189151	7742915	61.83%	6.171%
35	24.798	3681	3691	3710	rVB	4793351	12522784	100.00%	9.981%
36	25.027	3721	3730	3747	rVB	2972259	8090657	64.61%	6.448%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023836.D
Acq On : 31 Jan 2025 22:48
Operator : RC/JU
Sample : PB166393BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK393

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 125468713

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023836.D
Acq On : 31 Jan 2025 22:48
Operator : RC/JU
Sample : PB166393BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK393

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

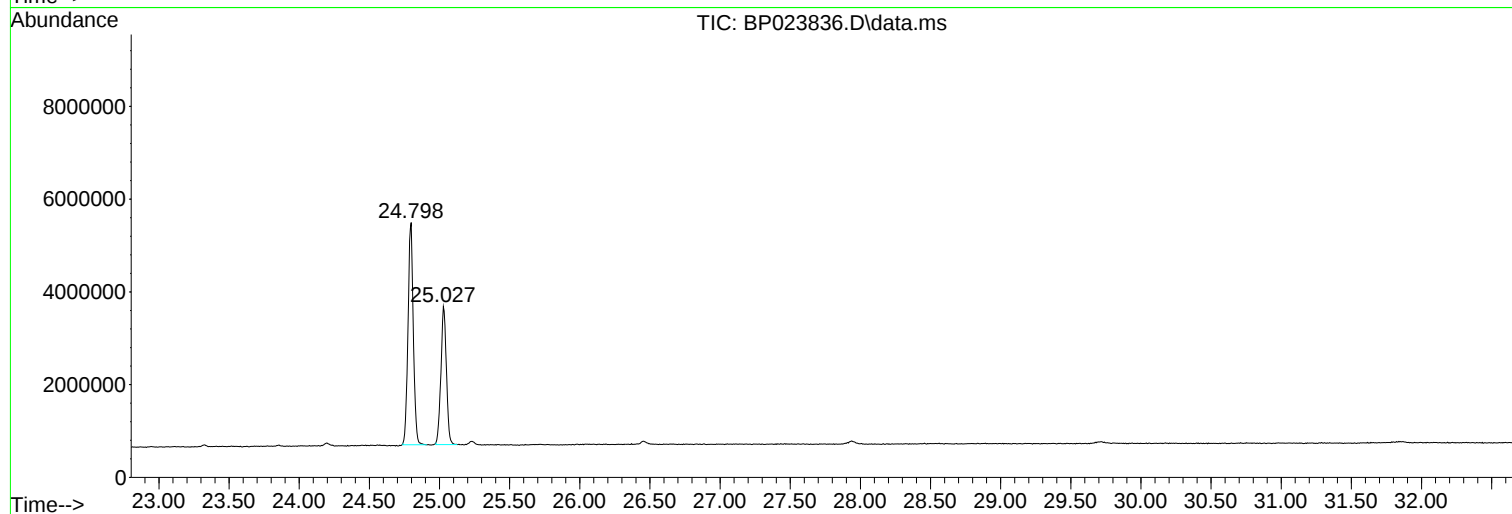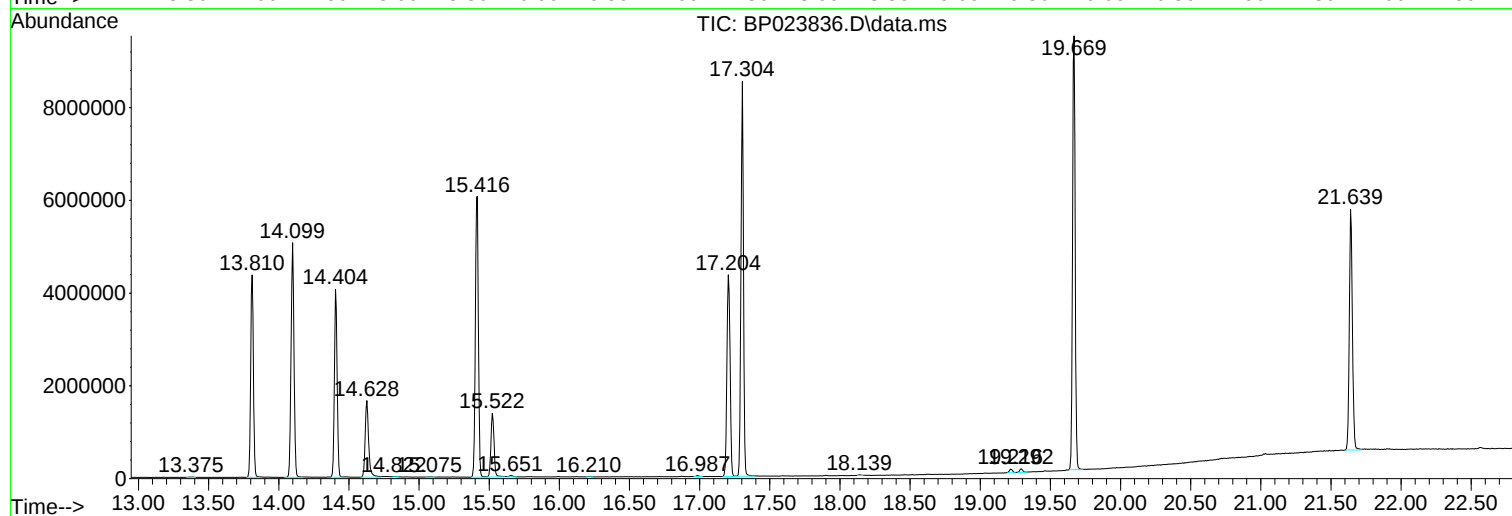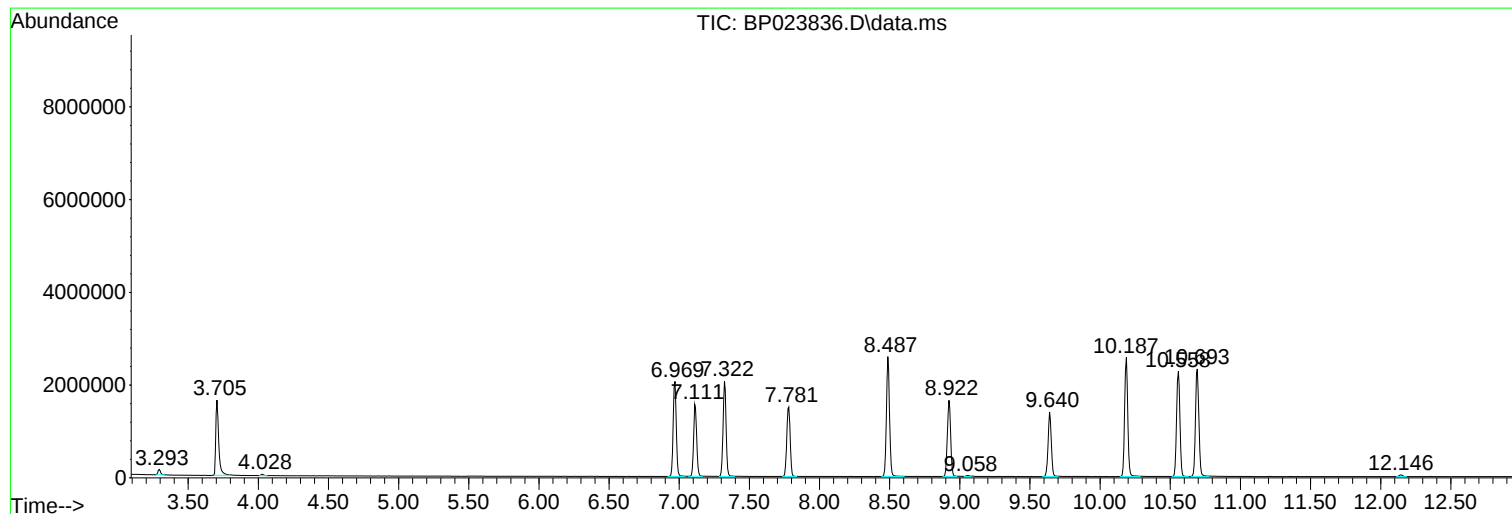

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023836.D
Acq On : 31 Jan 2025 22:48
Operator : RC/JU
Sample : PB166393BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK393

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023836.D
Acq On : 31 Jan 2025 22:48
Operator : RC/JU
Sample : PB166393BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK393

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------