

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
 Data File : BP023852.D
 Acq On : 01 Feb 2025 10:38
 Operator : RC/JU
 Sample : PB166436BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK436

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023852.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	29	33	39	rVB	117176	153422	1.30%	0.124%
2	3.687	98	102	124	rBV	1697098	2486234	21.00%	2.013%
3	4.004	152	156	163	rVB	25017	38545	0.33%	0.031%
4	6.940	648	655	666	rBV	2063515	3213693	27.14%	2.602%
5	7.092	674	681	692	rVB	1494737	2359322	19.92%	1.910%
6	7.298	709	716	729	rBV	2152738	3216983	27.17%	2.605%
7	7.757	786	794	805	rBV	1732568	2680511	22.64%	2.170%
8	8.463	907	914	932	rBV	2594728	4050438	34.20%	3.279%
9	8.898	981	988	997	rBV	1704576	2744700	23.18%	2.222%
10	9.622	1103	1111	1123	rBV	1342655	2225666	18.79%	1.802%
11	10.163	1196	1203	1218	rBV	2369762	4009625	33.86%	3.246%
12	10.533	1258	1266	1277	rBV	2179769	3862383	32.62%	3.127%
13	10.669	1281	1289	1305	rBV	2262023	3912100	33.04%	3.167%
14	11.333	1398	1402	1410	rBV	6527	16083	0.14%	0.013%
15	12.122	1531	1536	1544	rVB2	34607	63275	0.53%	0.051%
16	13.798	1814	1821	1838	rBV	3741067	5634498	47.58%	4.562%
17	14.086	1862	1870	1884	rBV	4415466	7018542	59.27%	5.682%
18	14.398	1915	1923	1932	rBV	3535212	5491070	46.37%	4.446%
19	14.622	1954	1961	1981	rBV	1928632	2851225	24.08%	2.308%
20	15.398	2086	2093	2108	rBV	5957920	8888347	75.06%	7.196%
21	15.521	2108	2114	2126	rBV	1437209	2073392	17.51%	1.679%
22	15.651	2131	2136	2145	rVB	32460	60669	0.51%	0.049%
23	16.986	2359	2363	2369	rVB	21314	27552	0.23%	0.022%
24	17.204	2392	2400	2407	rBV2	4082173	6854640	57.88%	5.550%
25	17.304	2411	2417	2430	rVV	7801498	10053767	84.90%	8.140%
26	17.586	2463	2465	2469	rBV5	7987	12353	0.10%	0.010%
27	19.215	2739	2742	2748	rVB2	84204	113958	0.96%	0.092%
28	19.286	2751	2754	2763	rVB	65157	99585	0.84%	0.081%
29	19.668	2813	2819	2826	rBV	9329866	11842001	100.00%	9.588%
30	21.633	3147	3153	3164	rBV	5457514	7717669	65.17%	6.249%
31	24.780	3679	3688	3701	rVB	5142652	11735537	99.10%	9.502%
32	25.015	3720	3728	3743	rVB	2582558	8003979	67.59%	6.480%




Sum of corrected areas: 123511764

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023852.D
Acq On : 01 Feb 2025 10:38
Operator : RC/JU
Sample : PB166436BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK436

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

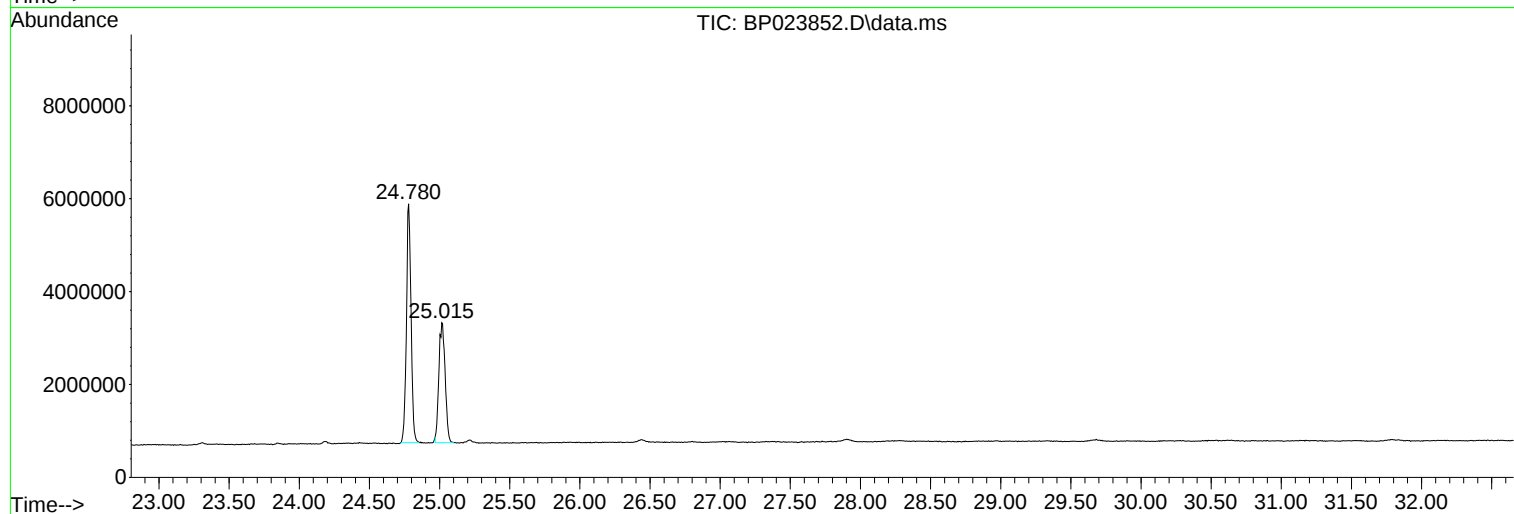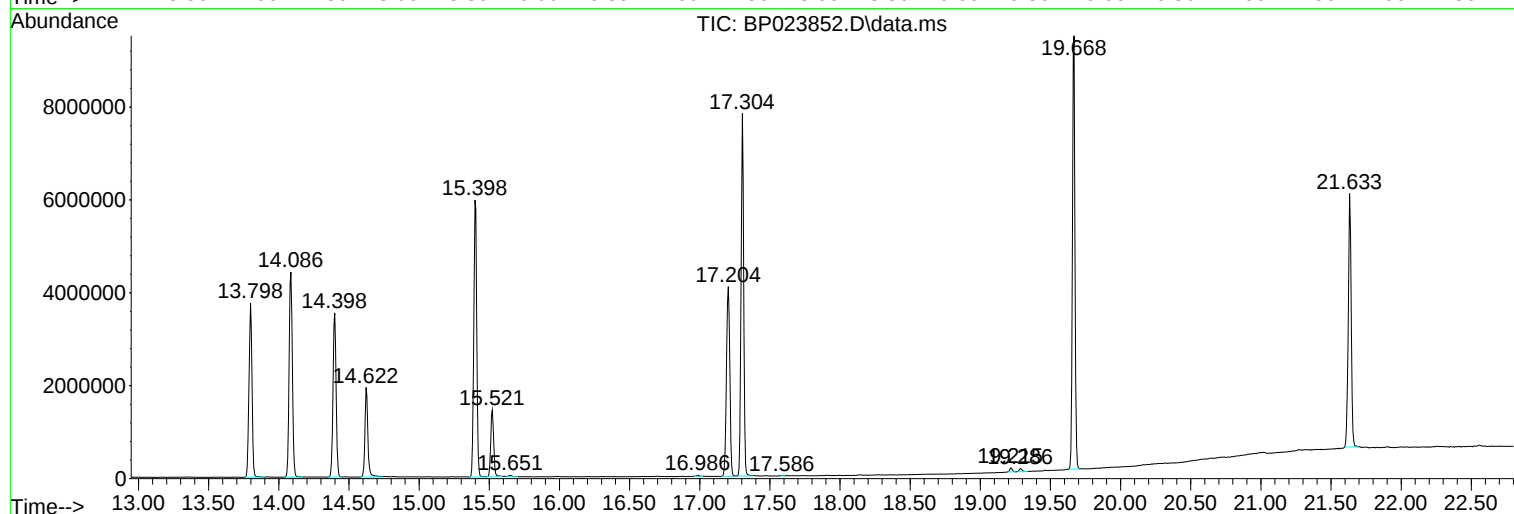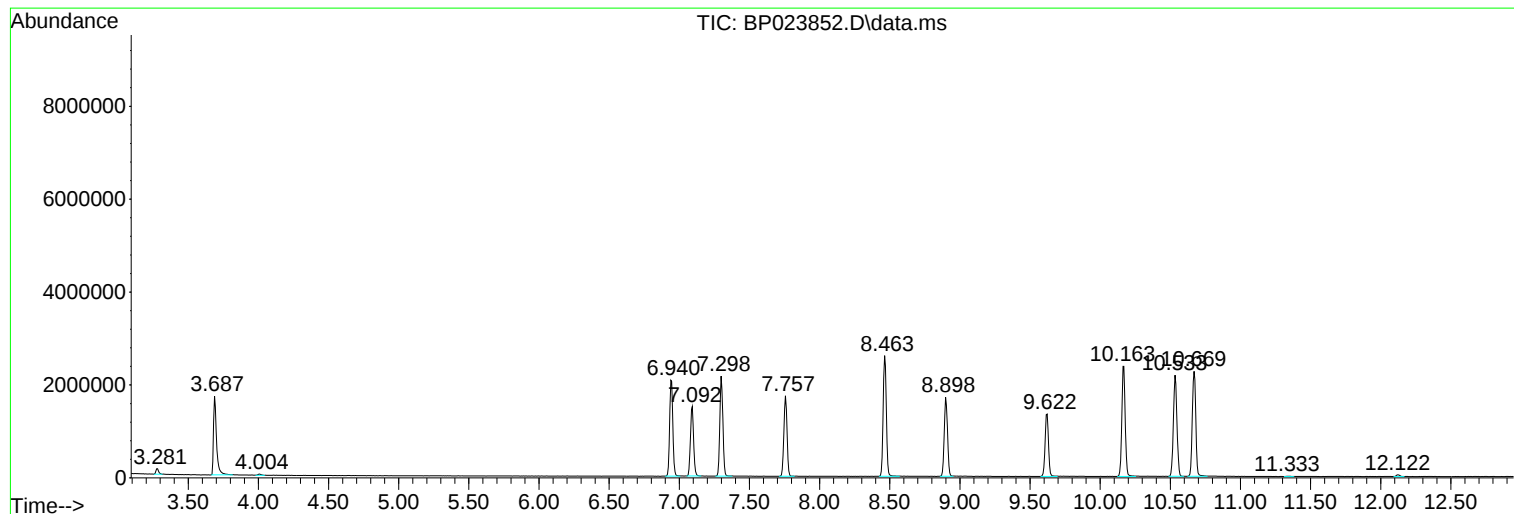

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023852.D
Acq On : 01 Feb 2025 10:38
Operator : RC/JU
Sample : PB166436BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK436

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023852.D
Acq On : 01 Feb 2025 10:38
Operator : RC/JU
Sample : PB166436BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK436

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------