

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
 Data File : BP023864.D
 Acq On : 01 Feb 2025 19:32
 Operator : RC/JU
 Sample : PB166436BL
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK436

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023864.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	48	rVB	130870	185765	1.57%	0.160%
2	3.705	101	105	124	rBV	1694226	2564830	21.68%	2.204%
3	4.028	156	160	165	rVB	23847	31481	0.27%	0.027%
4	6.963	652	659	676	rBV	2123206	3262292	27.58%	2.803%
5	7.116	678	685	695	rVV	1568362	2404734	20.33%	2.066%
6	7.322	712	720	733	rBV	2198258	3307872	27.97%	2.842%
7	7.781	789	798	805	rBV	1425951	2177989	18.41%	1.871%
8	8.487	908	918	936	rBV	2663745	4140883	35.01%	3.558%
9	8.922	985	992	1004	rBV	1783541	2829974	23.93%	2.432%
10	9.640	1106	1114	1128	rBV	1373795	2259815	19.11%	1.942%
11	10.181	1199	1206	1227	rBV	2541088	4081071	34.50%	3.507%
12	10.557	1261	1270	1278	rBV	1742676	3108332	26.28%	2.671%
13	10.687	1283	1292	1309	rBV	2505282	4024370	34.02%	3.458%
14	11.351	1399	1405	1411	rBV8	7690	16348	0.14%	0.014%
15	12.140	1533	1539	1545	rBV	38642	67388	0.57%	0.058%
16	13.804	1813	1822	1828	rBV	3868290	5578723	47.16%	4.793%
17	14.087	1862	1870	1886	rBV2	4628417	7130484	60.28%	6.127%
18	14.398	1916	1923	1934	rBV	3108447	4348890	36.77%	3.737%
19	14.616	1953	1960	1981	rBV	1709973	2812553	23.78%	2.417%
20	14.751	1981	1983	1989	rVV7	12484	27361	0.23%	0.024%
21	14.810	1991	1993	2000	rVB8	8806	14410	0.12%	0.012%
22	15.404	2087	2094	2106	rBV	6254540	8976493	75.89%	7.713%
23	15.510	2106	2112	2127	rVV	1229107	1830984	15.48%	1.573%
24	15.645	2130	2135	2142	rVB	26432	50410	0.43%	0.043%
25	16.863	2337	2342	2349	rVB	6847	12933	0.11%	0.011%
26	16.969	2356	2360	2365	rBV2	15416	23748	0.20%	0.020%
27	17.192	2391	2398	2407	rBV2	3634336	5255045	44.43%	4.515%
28	17.286	2408	2414	2435	rVB	7850621	10056086	85.02%	8.640%
29	17.886	2512	2516	2523	rBV10	14992	25000	0.21%	0.021%
30	18.128	2554	2557	2563	rBV7	10212	14409	0.12%	0.012%
31	19.210	2737	2741	2744	rBV	79753	99331	0.84%	0.085%
32	19.275	2749	2752	2759	rVB	65862	95774	0.81%	0.082%
33	19.657	2811	2817	2833	rBV	9028984	11828272	100.00%	10.163%
34	21.633	3147	3153	3163	rVB	3996255	5826721	49.26%	5.006%
35	24.763	3676	3685	3701	rVB2	4550095	11789347	99.67%	10.130%
36	25.004	3718	3726	3738	rVB	2510479	6123705	51.77%	5.262%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023864.D
Acq On : 01 Feb 2025 19:32
Operator : RC/JU
Sample : PB166436BL
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK436

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 116383823

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023864.D
Acq On : 01 Feb 2025 19:32
Operator : RC/JU
Sample : PB166436BL
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK436

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

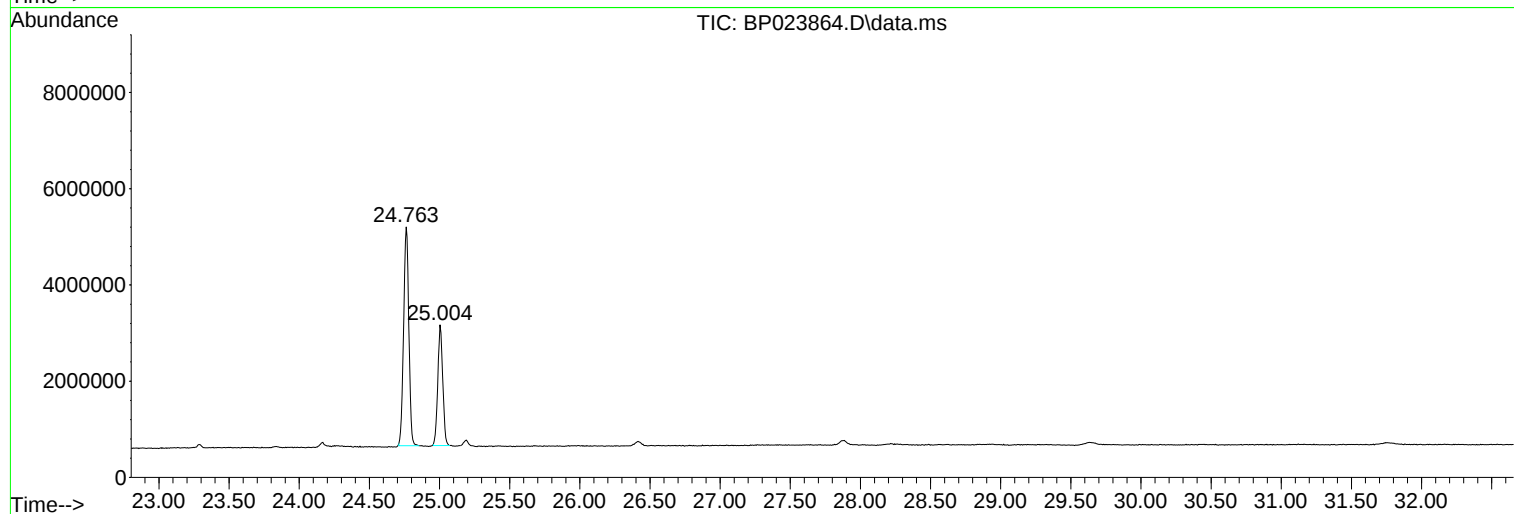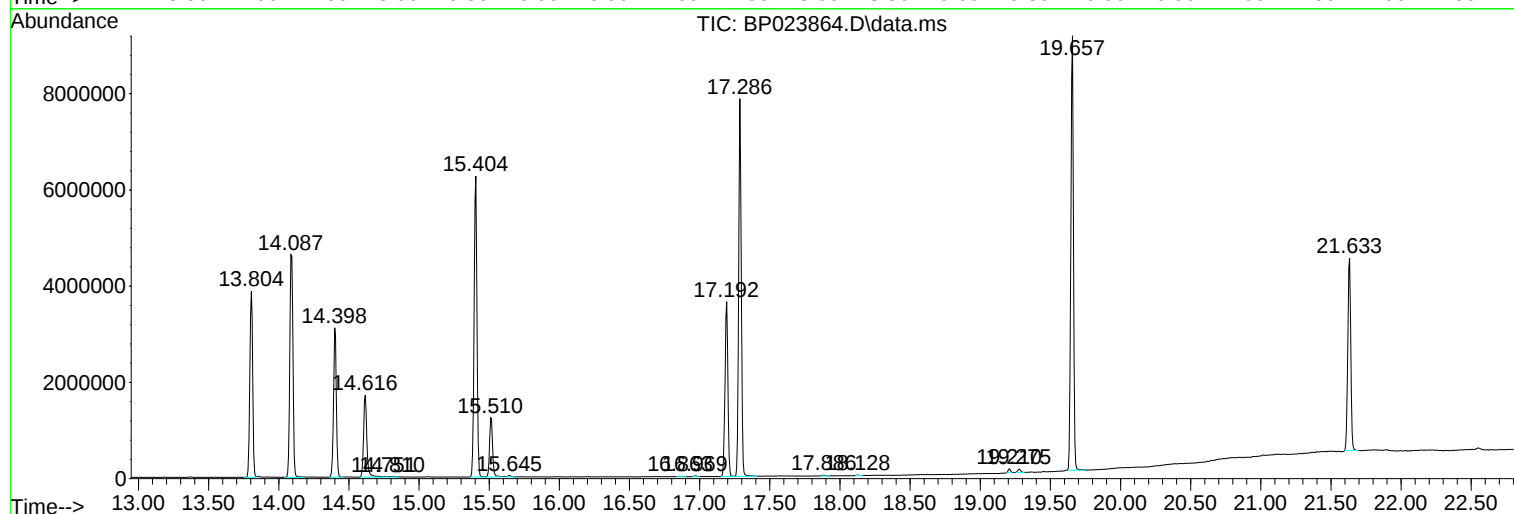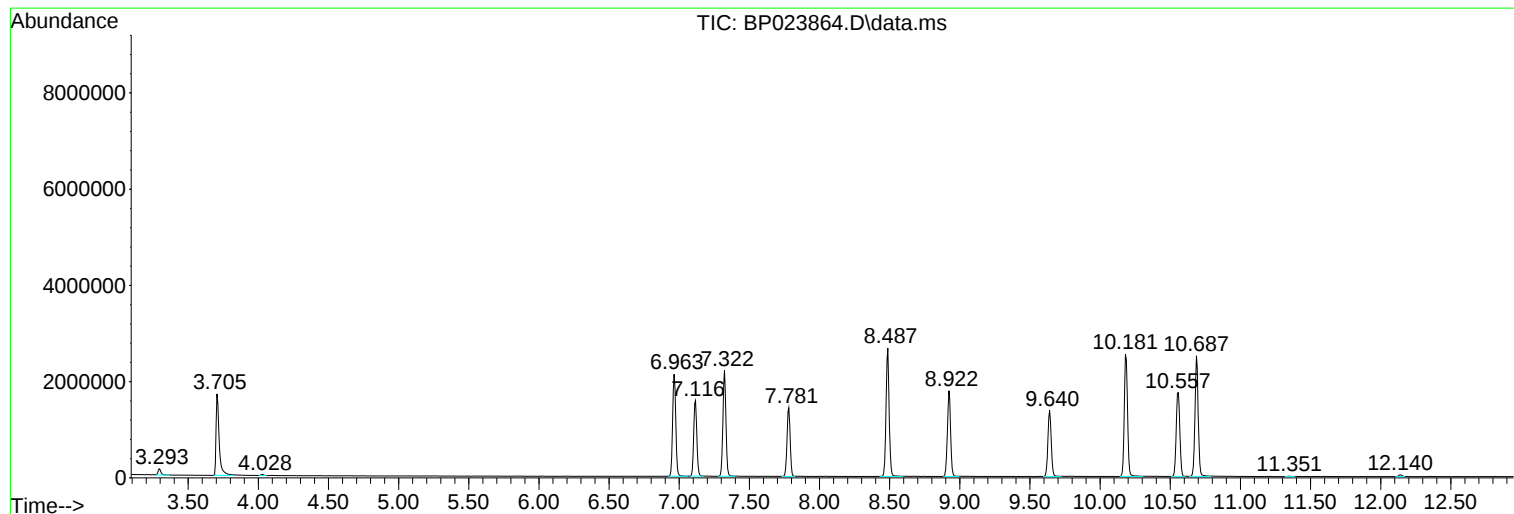

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023864.D
Acq On : 01 Feb 2025 19:32
Operator : RC/JU
Sample : PB166436BL
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK436

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023864.D
Acq On : 01 Feb 2025 19:32
Operator : RC/JU
Sample : PB166436BL
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK436

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc