

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
 Data File : BP023868.D
 Acq On : 01 Feb 2025 22:14
 Operator : RC/JU
 Sample : Q1248-15
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A6346

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023868.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	43	rVB	61441	82517	1.49%	0.132%
2	3.705	101	105	124	rBV	743541	1137069	20.52%	1.822%
3	4.028	156	160	164	rBV	17548	22987	0.41%	0.037%
4	6.963	651	659	672	rBV	994538	1593505	28.76%	2.553%
5	7.110	674	684	693	rBV	845250	1239693	22.37%	1.986%
6	7.322	712	720	730	rBV	963673	1512640	27.30%	2.423%
7	7.410	732	735	743	rVB8	7351	13506	0.24%	0.022%
8	7.775	790	797	805	rBV	1266255	1915305	34.57%	3.069%
9	7.840	805	808	813	rVB2	23198	32767	0.59%	0.052%
10	8.481	909	917	928	rBV	1244374	1983865	35.80%	3.178%
11	8.563	928	931	937	rVB8	7031	11796	0.21%	0.019%
12	8.922	983	992	999	rBV	868640	1407629	25.40%	2.255%
13	9.087	1016	1020	1025	rVB7	6813	11431	0.21%	0.018%
14	9.357	1061	1066	1074	rVB2	35269	57528	1.04%	0.092%
15	9.481	1081	1087	1097	rBV	126218	194447	3.51%	0.312%
16	9.634	1102	1113	1120	rBV	662557	1082808	19.54%	1.735%
17	9.751	1130	1133	1137	rVB4	4613	5595	0.10%	0.009%
18	10.181	1199	1206	1218	rBV	1256324	1912825	34.52%	3.065%
19	10.334	1228	1232	1241	rVB	7592	18245	0.33%	0.029%
20	10.551	1260	1269	1277	rBV	1728456	2865718	51.72%	4.591%
21	10.681	1284	1291	1310	rBV	1123494	1941058	35.03%	3.110%
22	10.910	1325	1330	1334	rBV9	3287	7486	0.14%	0.012%
23	11.087	1355	1360	1368	rVB2	41633	71742	1.29%	0.115%
24	11.345	1400	1404	1411	rBV10	5632	11625	0.21%	0.019%
25	11.845	1485	1489	1498	rVB10	3739	7722	0.14%	0.012%
26	11.981	1506	1512	1517	rBV7	11332	18072	0.33%	0.029%
27	12.134	1534	1538	1545	rVB3	20287	33401	0.60%	0.054%
28	12.375	1575	1579	1583	rVB3	3808	6027	0.11%	0.010%
29	12.798	1647	1651	1656	rVB8	4692	7623	0.14%	0.012%
30	12.863	1656	1662	1667	rVV9	6398	13881	0.25%	0.022%
31	12.939	1670	1675	1679	rBV6	4929	10292	0.19%	0.016%
32	12.998	1683	1685	1690	rVB5	4671	5926	0.11%	0.009%
33	13.181	1709	1716	1719	rBV9	4557	8346	0.15%	0.013%
34	13.222	1719	1723	1730	rVB2	30465	43040	0.78%	0.069%
35	13.375	1741	1749	1753	rVB2	12762	22961	0.41%	0.037%
36	13.628	1787	1792	1797	rBV8	4189	7902	0.14%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
 Data File : BP023868.D
 Acq On : 01 Feb 2025 22:14
 Operator : RC/JU
 Sample : Q1248-15
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A6346

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
 Title : SVOA CALIBRATION

37	13.716	1804	1807	1811	rBV5	6100	7285	0.13%	0.012%
38	13.798	1813	1821	1832	rBV	2267484	3022054	54.54%	4.842%
39	13.928	1840	1843	1850	rVB9	5485	9103	0.16%	0.015%
40	14.086	1859	1870	1879	rBV	2251563	3158563	57.00%	5.061%
41	14.298	1902	1906	1911	rVB3	12256	17125	0.31%	0.027%
42	14.392	1915	1922	1934	rBV	2923789	4030707	72.74%	6.458%
43	14.604	1952	1958	1978	rBV	793912	1278496	23.07%	2.048%
44	14.751	1981	1983	1990	rVV7	8476	14060	0.25%	0.023%
45	14.816	1990	1994	2003	rVB7	11657	21546	0.39%	0.035%
46	15.216	2057	2062	2067	rBV5	10109	18054	0.33%	0.029%
47	15.263	2067	2070	2074	rVB6	5444	7494	0.14%	0.012%
48	15.392	2085	2092	2103	rBV	2538801	3681534	66.44%	5.898%
49	15.510	2106	2112	2123	rBV	452450	642190	11.59%	1.029%
50	15.639	2129	2134	2138	rBV3	9769	15149	0.27%	0.024%
51	15.769	2149	2156	2162	rBV	554676	760408	13.72%	1.218%
52	15.851	2168	2170	2174	rVB5	5201	5914	0.11%	0.009%
53	16.098	2209	2212	2217	rBV5	5497	7397	0.13%	0.012%
54	16.580	2290	2294	2300	rVB8	9707	15370	0.28%	0.025%
55	16.839	2334	2338	2344	rVB8	13791	22595	0.41%	0.036%
56	16.963	2354	2359	2365	rBV2	14280	25525	0.46%	0.041%
57	17.122	2383	2386	2389	rVB5	10881	12642	0.23%	0.020%
58	17.180	2389	2396	2407	rBV2	3320202	4869329	87.88%	7.801%
59	17.286	2407	2414	2425	rVV	2860870	3767493	67.99%	6.036%
60	17.380	2426	2430	2436	rVV7	28310	47783	0.86%	0.077%
61	17.433	2436	2439	2445	rVB8	7038	13830	0.25%	0.022%
62	17.604	2465	2468	2472	rVB5	10360	14147	0.26%	0.023%
63	18.116	2550	2555	2563	rBV	190041	276937	5.00%	0.444%
64	18.569	2630	2632	2636	rBV4	14605	15007	0.27%	0.024%
65	19.445	2778	2781	2786	rBV5	29968	41089	0.74%	0.066%
66	19.645	2810	2815	2826	rBV	2813497	3700406	66.78%	5.929%
67	21.621	3145	3151	3159	rVB	3247389	5233220	94.44%	8.384%
68	24.745	3675	3682	3696	rVB	1079409	2803114	50.59%	4.491%
69	24.986	3715	3723	3738	rVB2	1972261	5541080	100.00%	8.878%




Sum of corrected areas: 62415626

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023868.D
Acq On : 01 Feb 2025 22:14
Operator : RC/JU
Sample : Q1248-15
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A6346

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

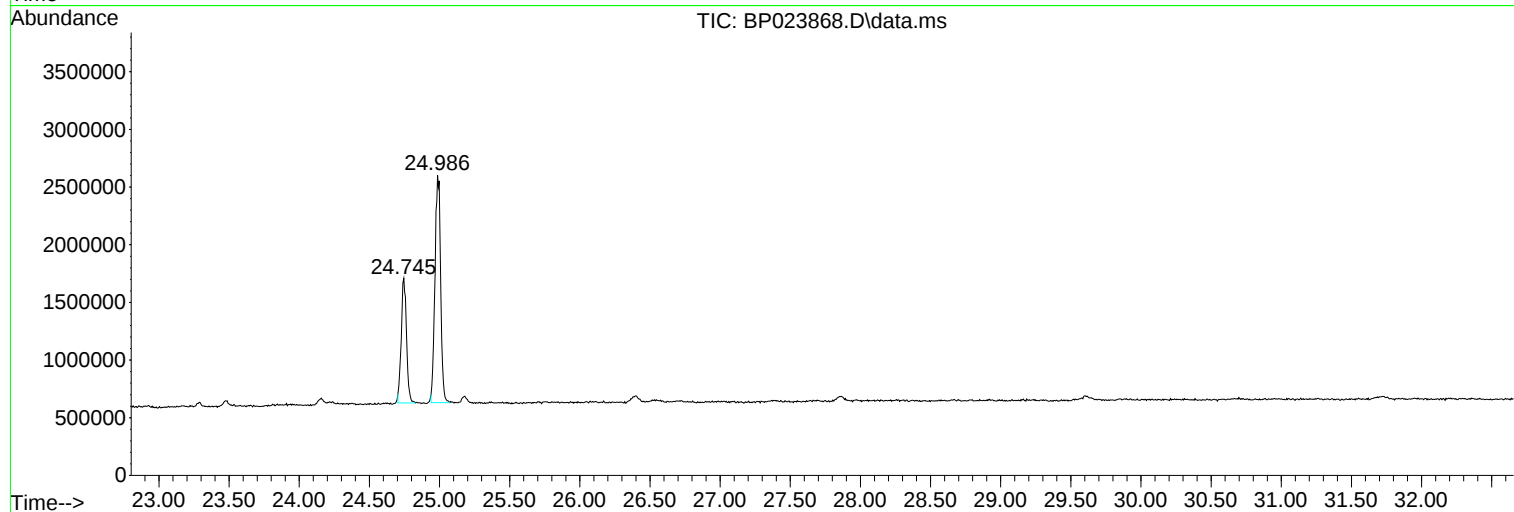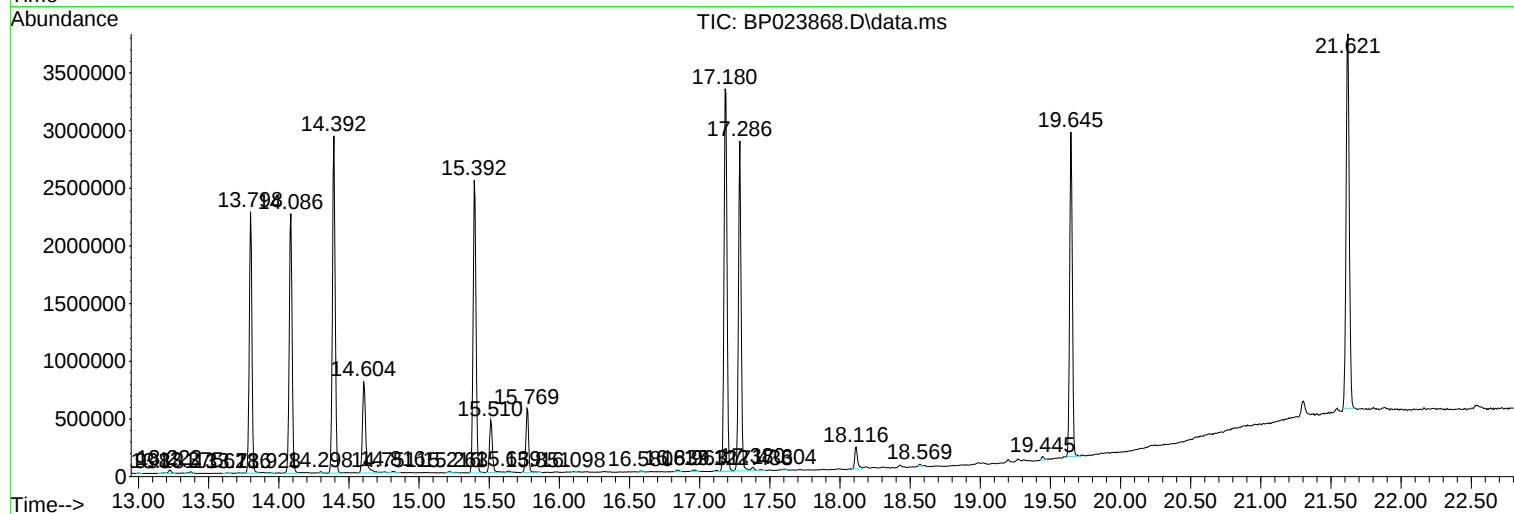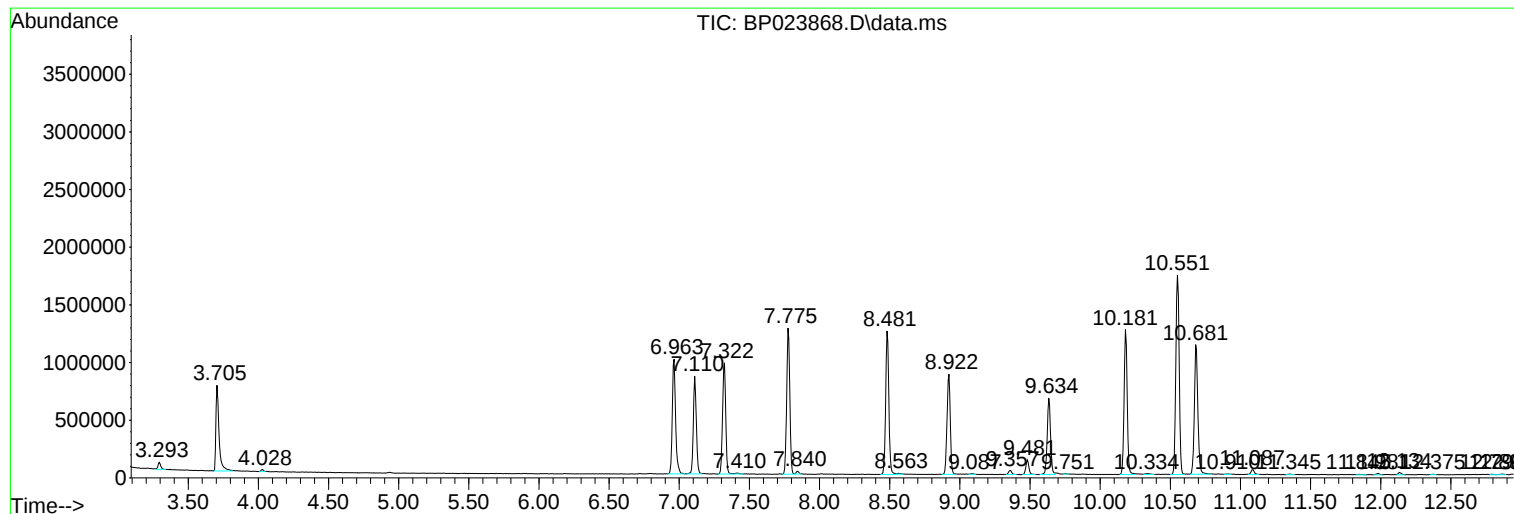

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023868.D
Acq On : 01 Feb 2025 22:14
Operator : RC/JU
Sample : Q1248-15
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A6346










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.769	3.77 ng/ul	760408	Acenaphthene-d10	14.392

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	96
2			Benzophenone	182	C13H10O	000119-61-9	96
3			Benzophenone	182	C13H10O	000119-61-9	96
4			Benzophenone	182	C13H10O	000119-61-9	91
5			Benzophenone	182	C13H10O	000119-61-9	90

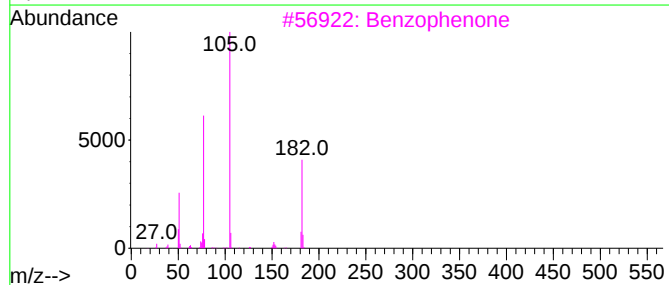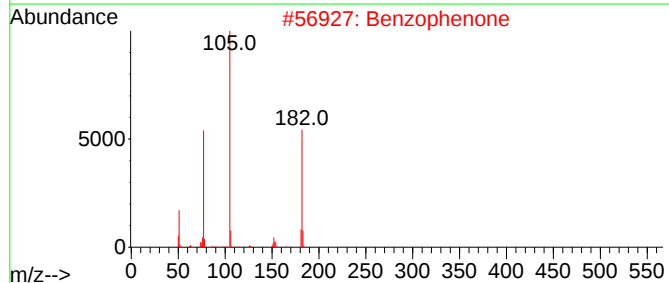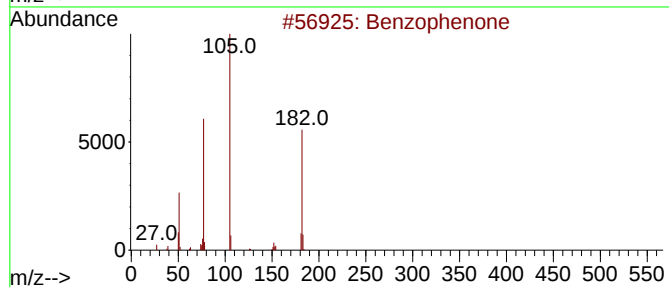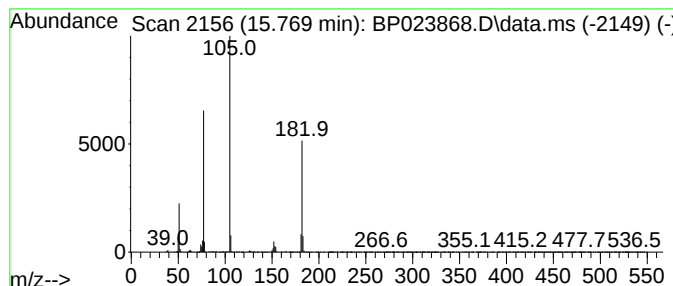

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP013125\
Data File : BP023868.D
Acq On : 01 Feb 2025 22:14
Operator : RC/JU
Sample : Q1248-15
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A6346

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012925.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	15.769	3.8	ng/u1	760408	3	14.392	4030710	20.0