

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020822\
 Data File : BP009056.D
 Acq On : 08 Feb 2022 13:51
 Operator : CG/JU
 Sample : N1411-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 282-284

Quant Time: Feb 08 14:27:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 07 15:13:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.804	152	148055	20.000	ng	0.00
21) Naphthalene-d8	10.604	136	600582	20.000	ng	0.00
39) Acenaphthene-d10	14.445	164	333747	20.000	ng	0.00
64) Phenanthrene-d10	17.210	188	708434	20.000	ng	0.00
76) Chrysene-d12	21.304	240	875148	20.000	ng	0.00
86) Perylene-d12	23.704	264	1001601	20.000	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.434	112	917390	110.530	ng	0.04
7) Phenol-d6	6.993	99	1077299	98.504	ng	0.00
23) Nitrobenzene-d5	8.963	82	695814	65.336	ng	0.00
42) 2,4,6-Tribromophenol	15.951	330	503343	112.955	ng	0.00
45) 2-Fluorobiphenyl	13.069	172	1897032	79.570	ng	0.00
79) Terphenyl-d14	19.774	244	2951679	60.654	ng	0.00
Target Compounds						
15) Benzyl Alcohol	8.057	79	74056	10.637	ng	Qvalue 93
32) Benzoic acid	9.946	122	22294	6.636	ng	93
84) Bis(2-ethylhexyl)phtha...	21.215	149	116417	4.111	ng	# 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020822\
Data File : BP009056.D
Acq On : 08 Feb 2022 13:51
Operator : CG/JU
Sample : N1411-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
282-284

Quant Time: Feb 08 14:27:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 07 15:13:17 2022
Response via : Initial Calibration




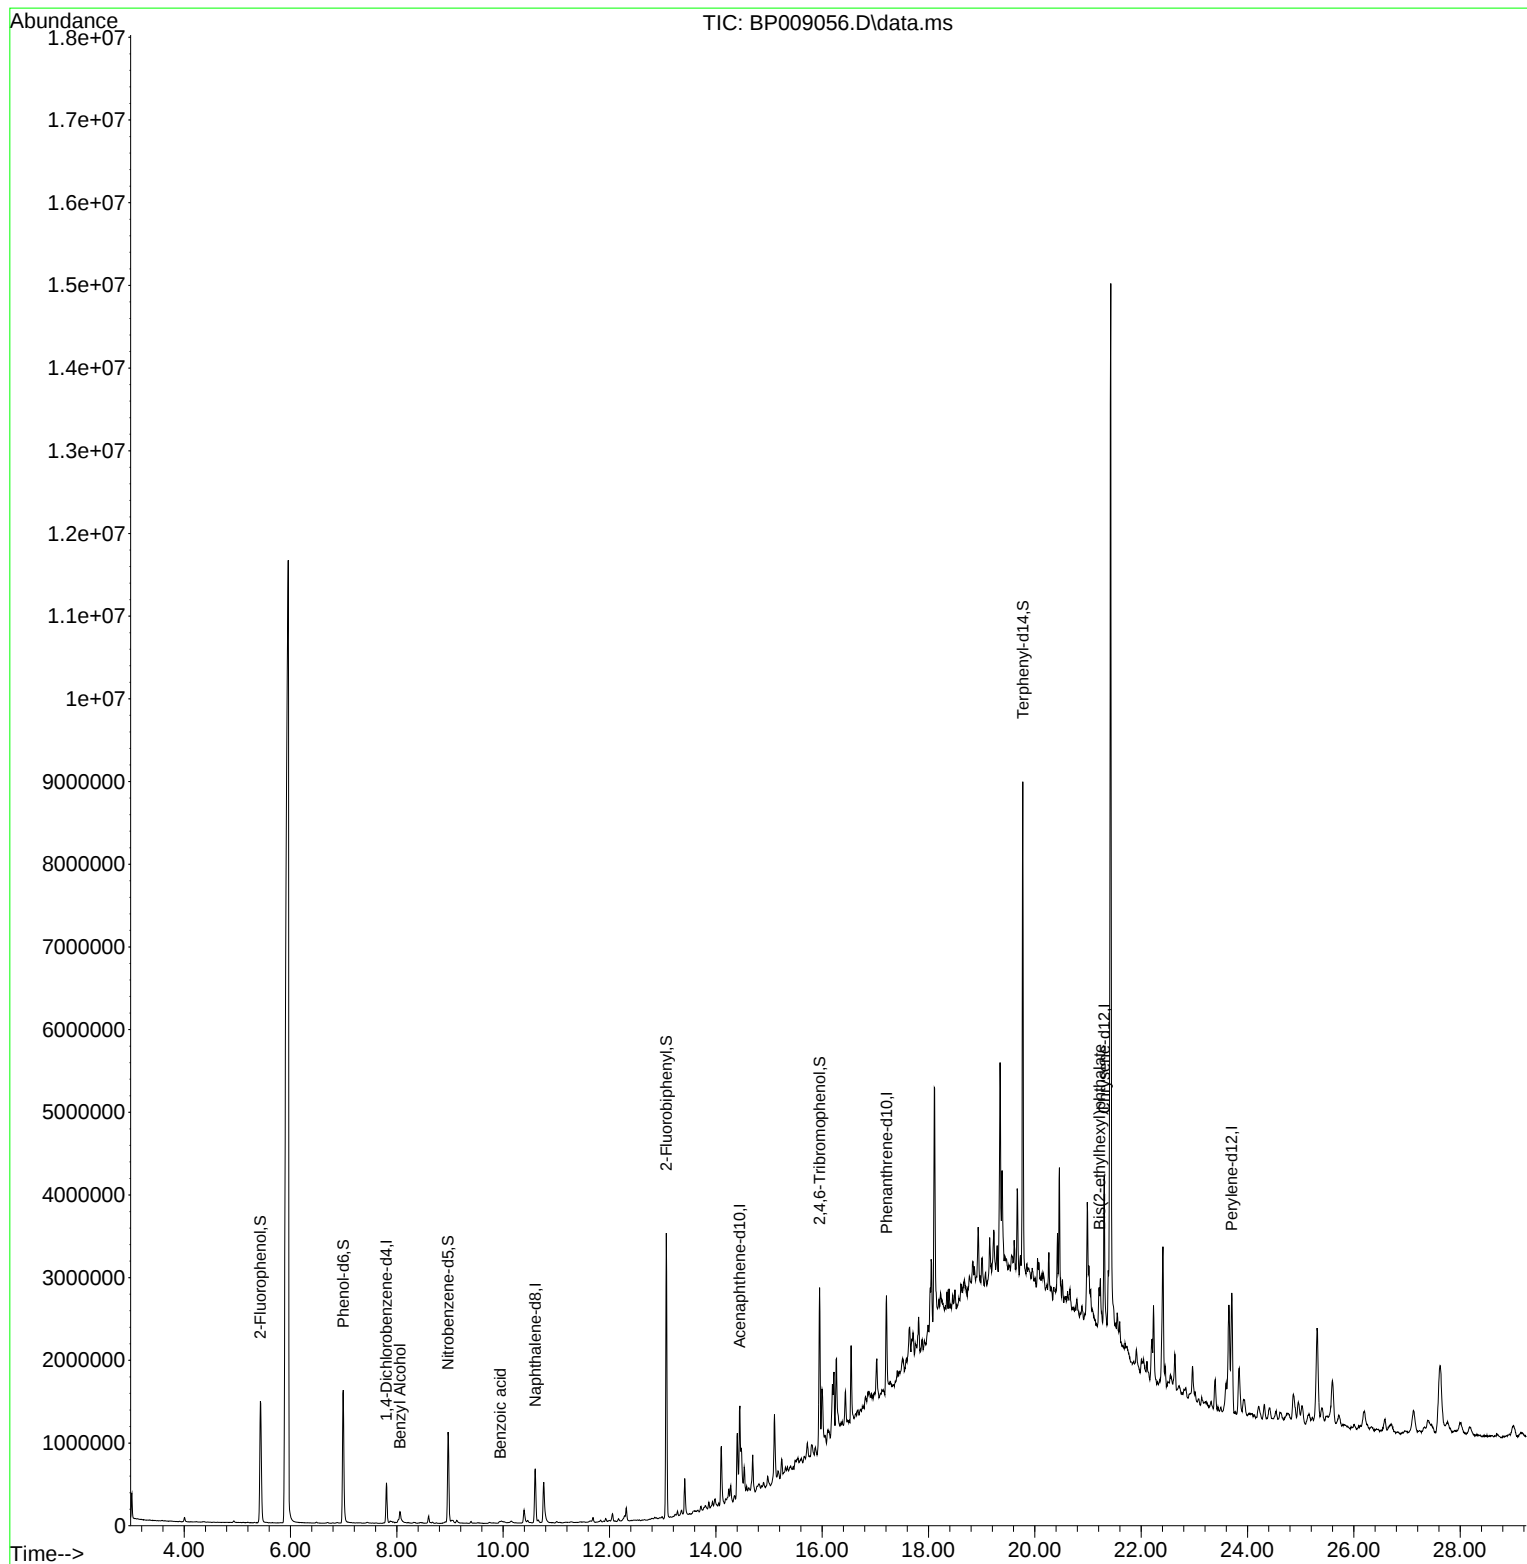




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.804 min Scan# 81
Delta R.T. -0.001 min
Lab File: BP009056.D
Acq: 08 Feb 2022 13:51




Instrument :
BNA_P
ClientSampleId :
282-284


Tgt Ion:152 Resp: 148055
Ion Ratio Lower Upper
152 100
150 159.7 127.0 190.6
115 56.1 43.7 65.5

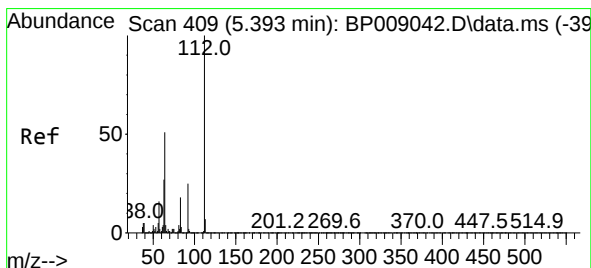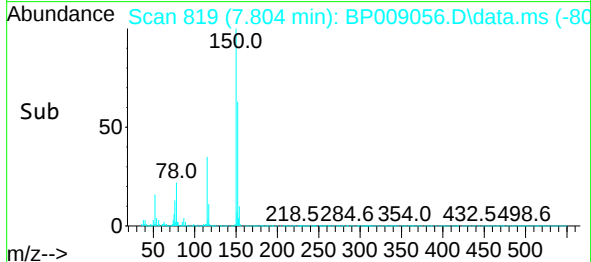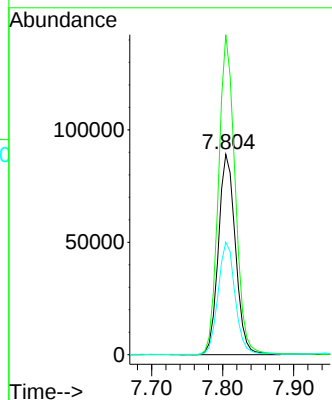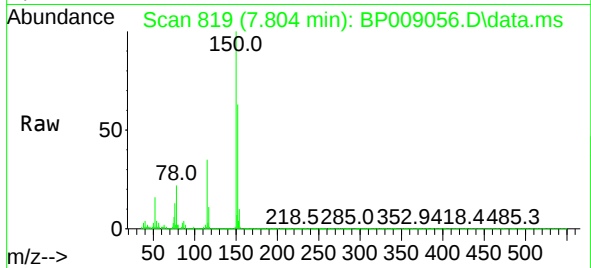

#5
2-Fluorophenol
Concen: 110.530 ng
RT: 5.434 min Scan# 416
Delta R.T. 0.041 min
Lab File: BP009056.D
Acq: 08 Feb 2022 13:51

Tgt Ion:112 Resp: 917390
Ion Ratio Lower Upper
112 100
64 51.8 39.7 59.5
63 27.1 20.0 30.0


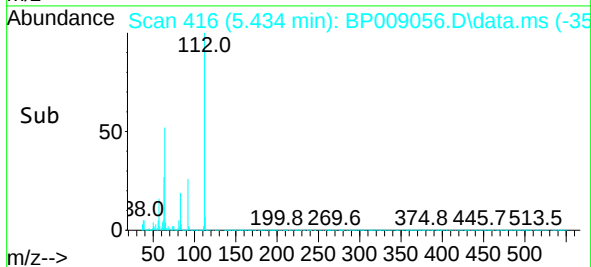
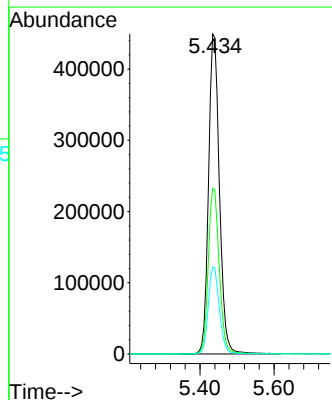
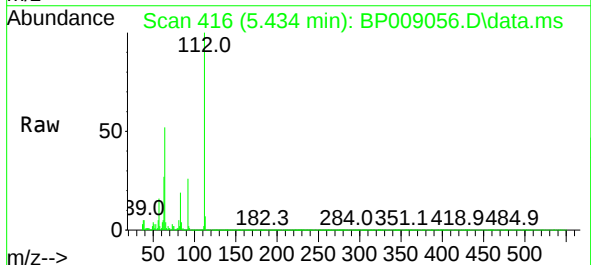


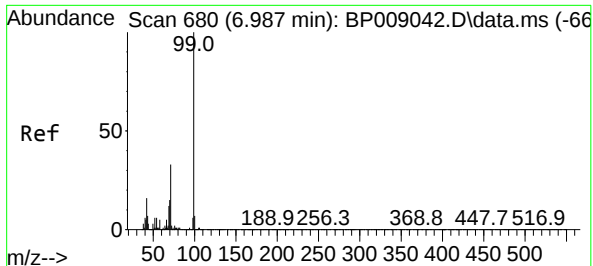

#7
Phenol-d6
Concen: 98.504 ng
RT: 6.993 min Scan# 61
Delta R.T. 0.006 min
Lab File: BP009056.D
Acq: 08 Feb 2022 13:51




Instrument :
BNA_P
ClientSampleId :
282-284


Tgt Ion: 99 Resp: 1077299
Ion Ratio Lower Upper
99 100
42 15.6 10.8 16.2
71 34.2 23.8 35.6

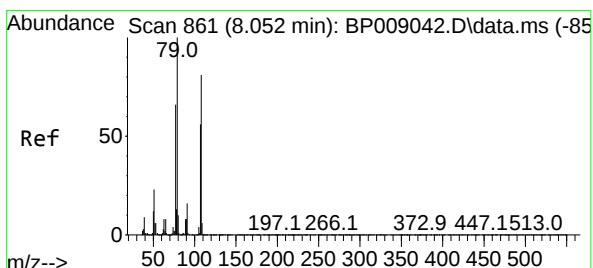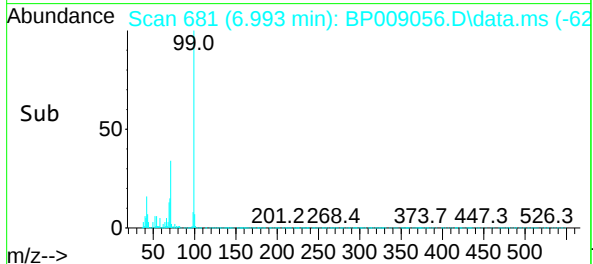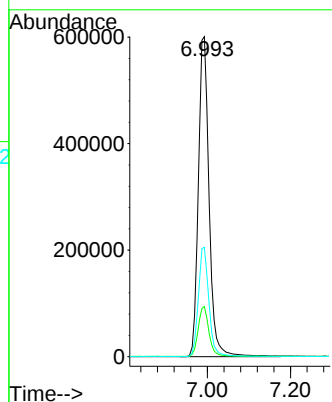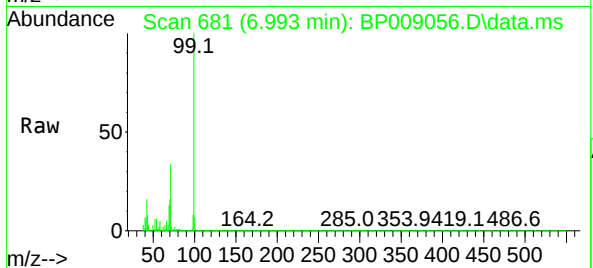

#15
Benzyl Alcohol
Concen: 10.637 ng
RT: 8.057 min Scan# 862
Delta R.T. 0.006 min
Lab File: BP009056.D
Acq: 08 Feb 2022 13:51

Tgt Ion: 79 Resp: 74056
Ion Ratio Lower Upper
79 100
108 74.8 67.8 101.8
77 62.4 50.7 76.1


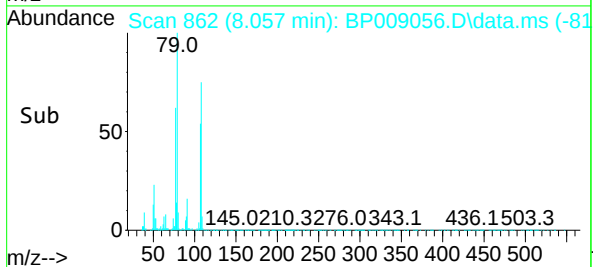
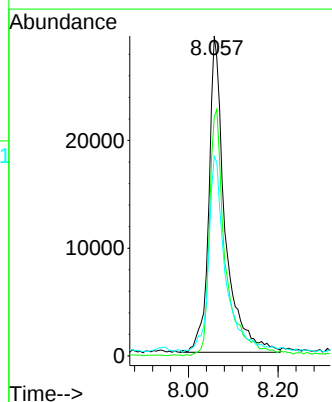
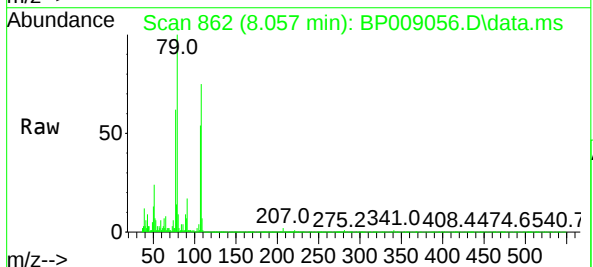


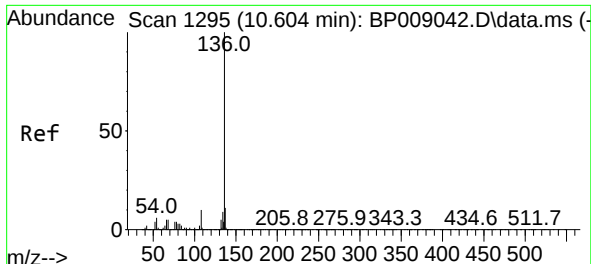

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.604 min Scan# 11
Delta R.T. 0.000 min
Lab File: BP009056.D
Acq: 08 Feb 2022 13:51




Instrument :
BNA_P
ClientSampleId :
282-284


Tgt Ion:	136	Resp:	600582
Ion	Ratio	Lower	Upper
136	100		
137	10.6	9.0	13.4
54	6.1	4.9	7.3
68	5.0	4.3	6.5

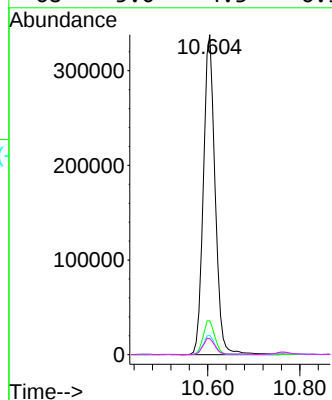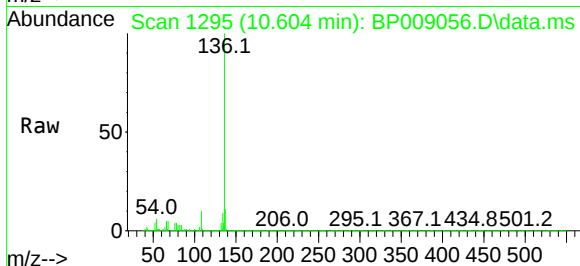

#23
Nitrobenzene-d5
Concen: 65.336 ng
RT: 8.963 min Scan# 1016
Delta R.T. -0.006 min
Lab File: BP009056.D
Acq: 08 Feb 2022 13:51

Tgt Ion:	82	Resp:	695814
Ion	Ratio	Lower	Upper
82	100		
128	46.1	39.4	59.2
54	43.1	32.6	48.8


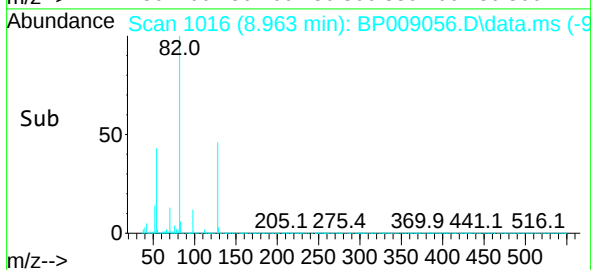
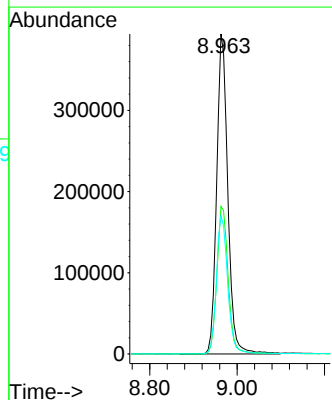
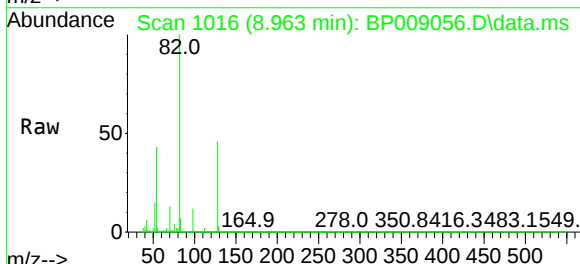




#32
Benzoic acid
Concen: 6.636 ng
RT: 9.946 min Scan# 1183
Delta R.T. -0.023 min
Lab File: BP009056.D
Acq: 08 Feb 2022 13:51




Instrument :
BNA_P
ClientSampleId :
282-284


Tgt Ion:	122	Resp:	22294
Ion	Ratio	Lower	Upper
122	100		
105	117.0	100.1	140.1
77	98.4	65.5	105.5

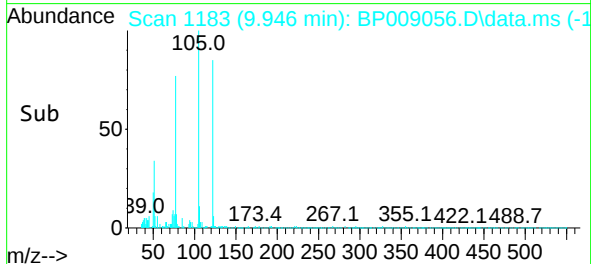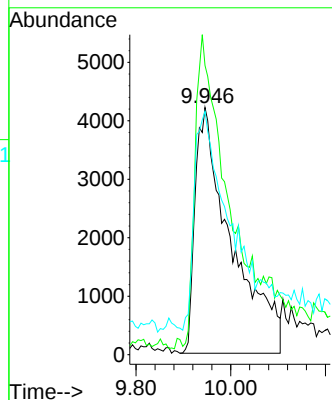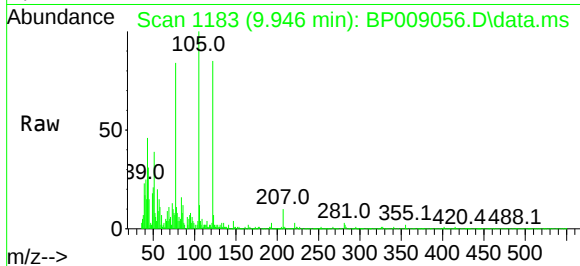

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.445 min Scan# 1948
Delta R.T. 0.000 min
Lab File: BP009056.D
Acq: 08 Feb 2022 13:51

Tgt Ion:	164	Resp:	333747
Ion	Ratio	Lower	Upper
164	100		
162	100.0	79.9	119.9
160	42.3	35.5	53.3


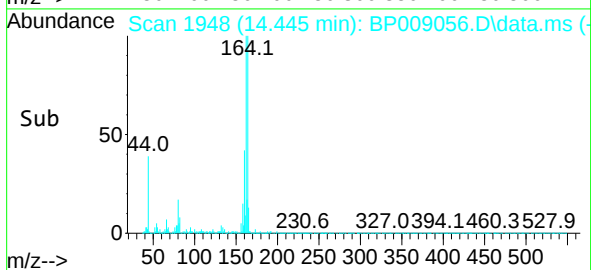
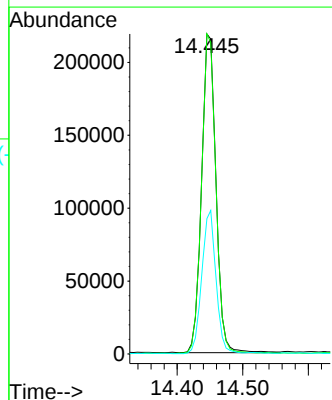
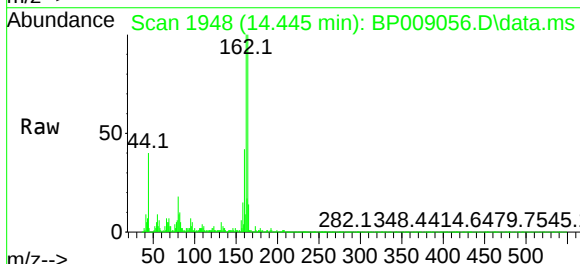




#42
2,4,6-Tribromophenol
Concen: 112.955 ng
RT: 15.951 min Scan# 21
Delta R.T. 0.006 min
Lab File: BP009056.D
Acq: 08 Feb 2022 13:51




Instrument :
BNA_P
ClientSampleId :
282-284


Tgt Ion: 330 Resp: 503343
Ion Ratio Lower Upper
330 100
332 97.2 77.0 115.4
141 26.9 21.3 31.9

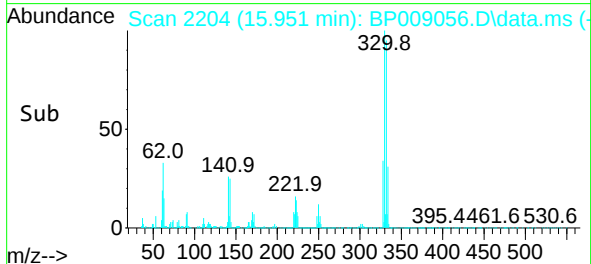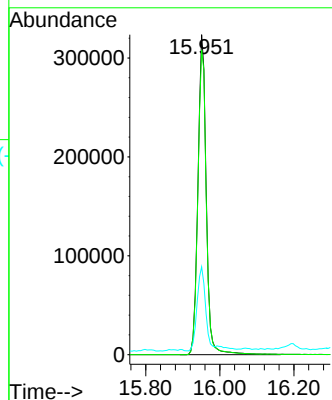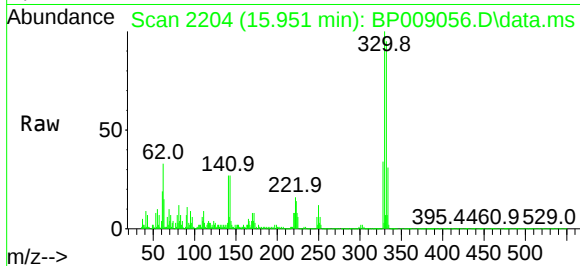

#45
2-Fluorobiphenyl
Concen: 79.570 ng
RT: 13.069 min Scan# 1714
Delta R.T. -0.000 min
Lab File: BP009056.D
Acq: 08 Feb 2022 13:51

Tgt Ion: 172 Resp: 1897032
Ion Ratio Lower Upper
172 100
171 34.8 29.3 43.9
170 23.1 19.5 29.3

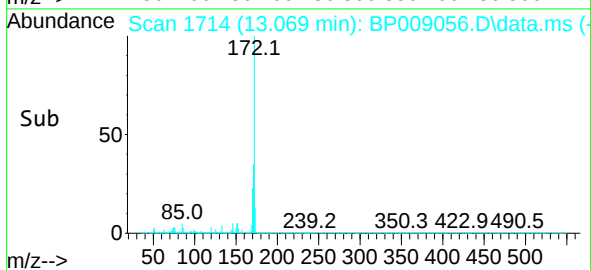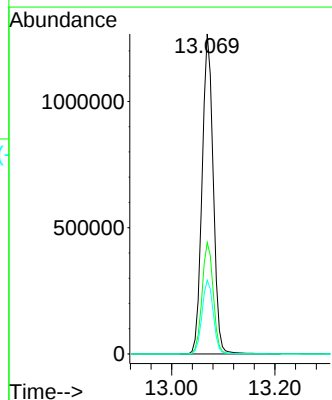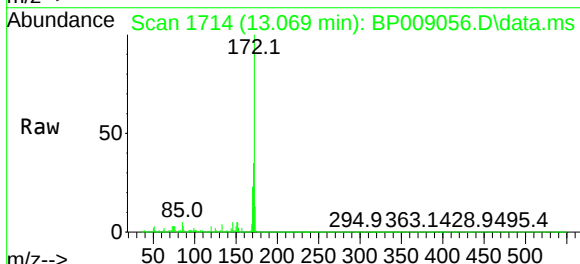

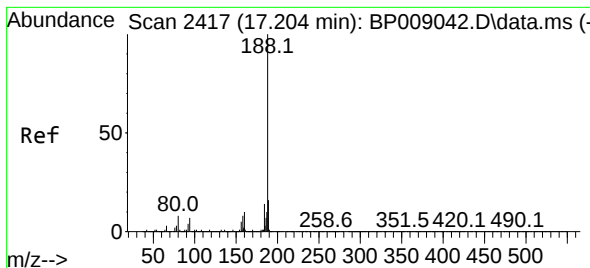

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.210 min Scan# 2418

Delta R.T. 0.006 min

Lab File: BP009056.D

Acq: 08 Feb 2022 13:51

Instrument :

BNA_P

ClientSampleId :

282-284





Tgt Ion:188 Resp: 708434

Ion Ratio Lower Upper

188 100

94 9.1 6.8 10.2

80 8.9 7.2 10.8

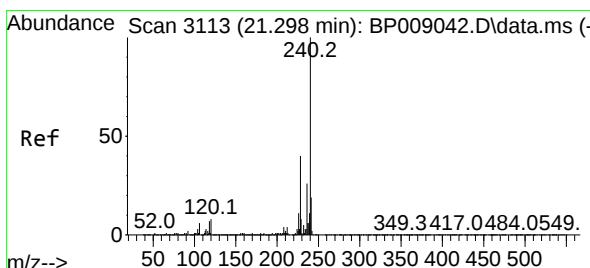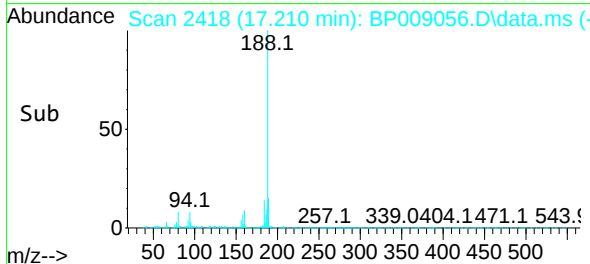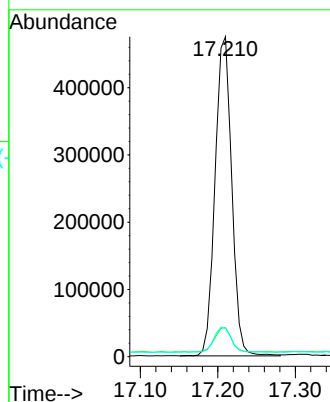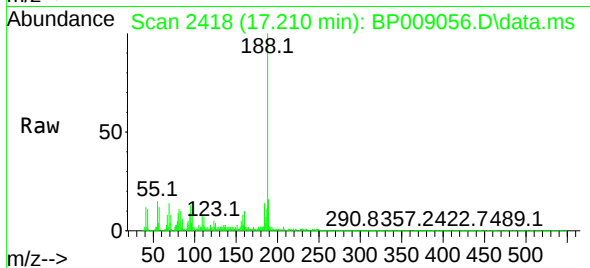

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.304 min Scan# 3114

Delta R.T. 0.006 min

Lab File: BP009056.D

Acq: 08 Feb 2022 13:51




Tgt Ion:240 Resp: 875148


Ion Ratio Lower Upper

240 100

120 8.8 7.7 11.5

236 26.7 21.2 31.8


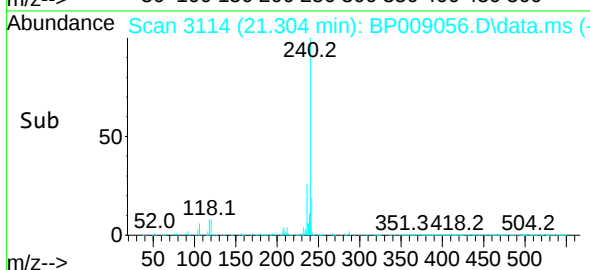
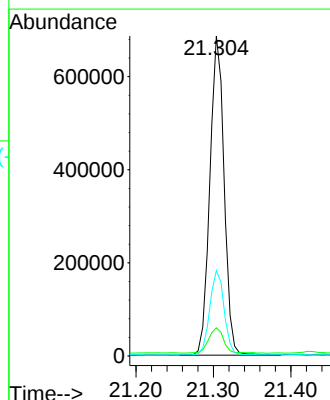
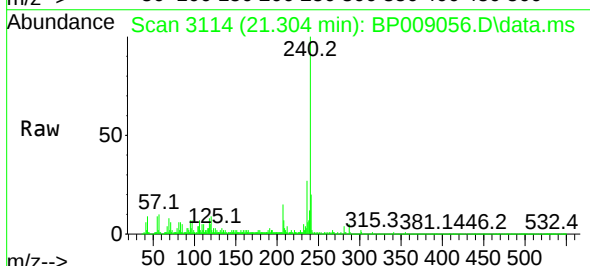




#79
 Terphenyl-d14
 Concen: 60.654 ng
 RT: 19.774 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: BP009056.D
 Acq: 08 Feb 2022 13:51




Instrument :
 BNA_P
 ClientSampleId :
 282-284


Tgt Ion:244 Resp: 2951679
 Ion Ratio Lower Upper
 244 100
 212 7.1 6.5 9.7
 122 8.1 9.2 13.8#

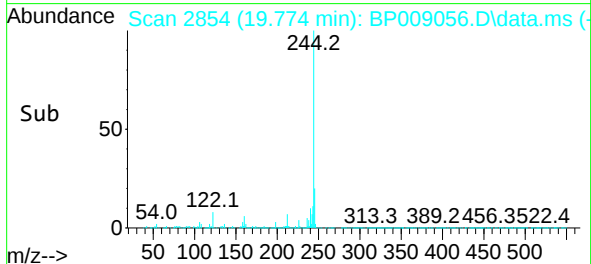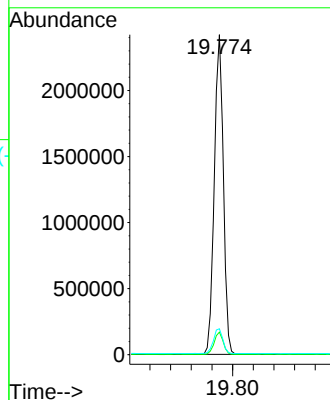

#84
 Bis(2-ethylhexyl)phthalate
 Concen: 4.111 ng
 RT: 21.215 min Scan# 3099
 Delta R.T. 0.006 min
 Lab File: BP009056.D
 Acq: 08 Feb 2022 13:51

Tgt Ion:149 Resp: 116417
 Ion Ratio Lower Upper
 149 100
 167 32.4 25.0 37.4
 279 7.4 4.8 7.2#

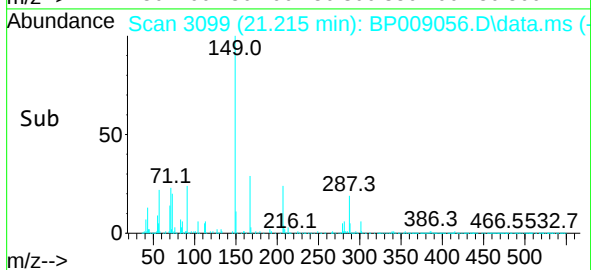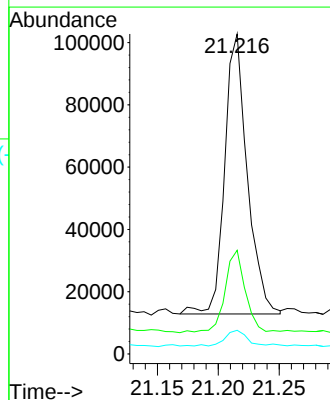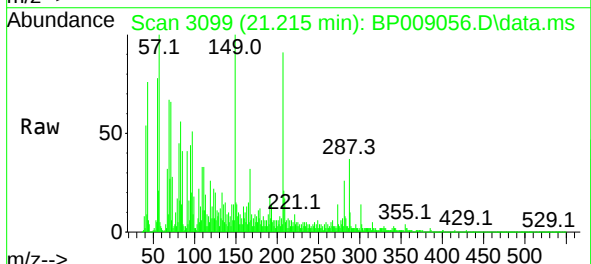

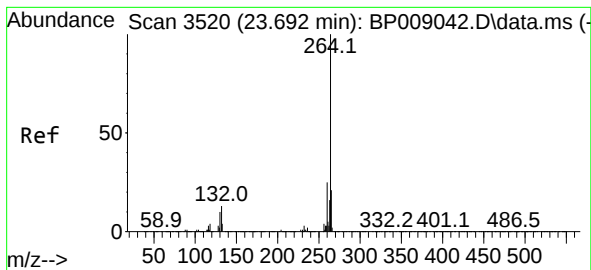

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.704 min Scan# 31

Delta R.T. 0.012 min

Lab File: BP009056.D


Acq: 08 Feb 2022 13:51

Instrument :

BNA_P

ClientSampleId :

282-284

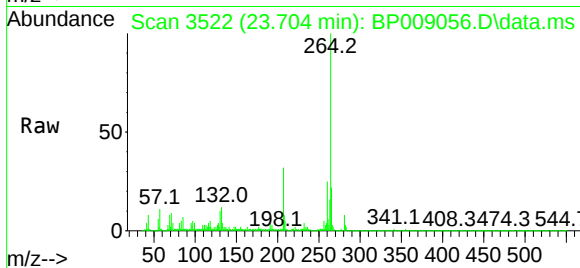

Tgt Ion:264 Resp: 1001601

Ion	Ratio	Lower	Upper
264	100		
260	24.7	19.1	28.7
265	22.1	17.1	25.7

264 100

260 24.7 19.1 28.7

265 22.1 17.1 25.7

