
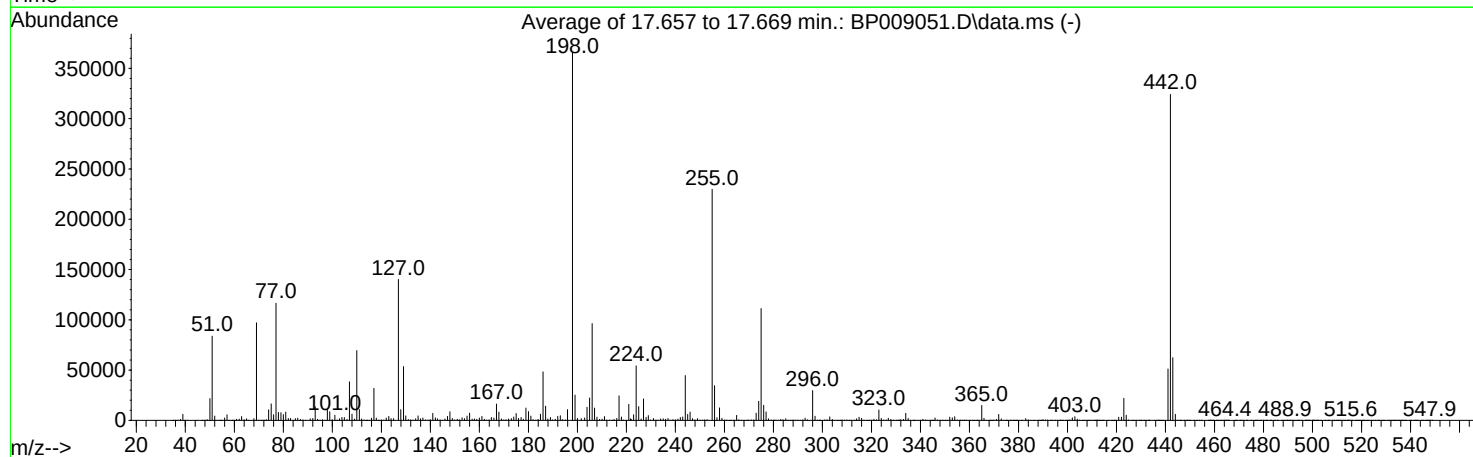


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020822\
 Data File : BP009051.D
 Acq On : 08 Feb 2022 10:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 07 15:13:17 2022

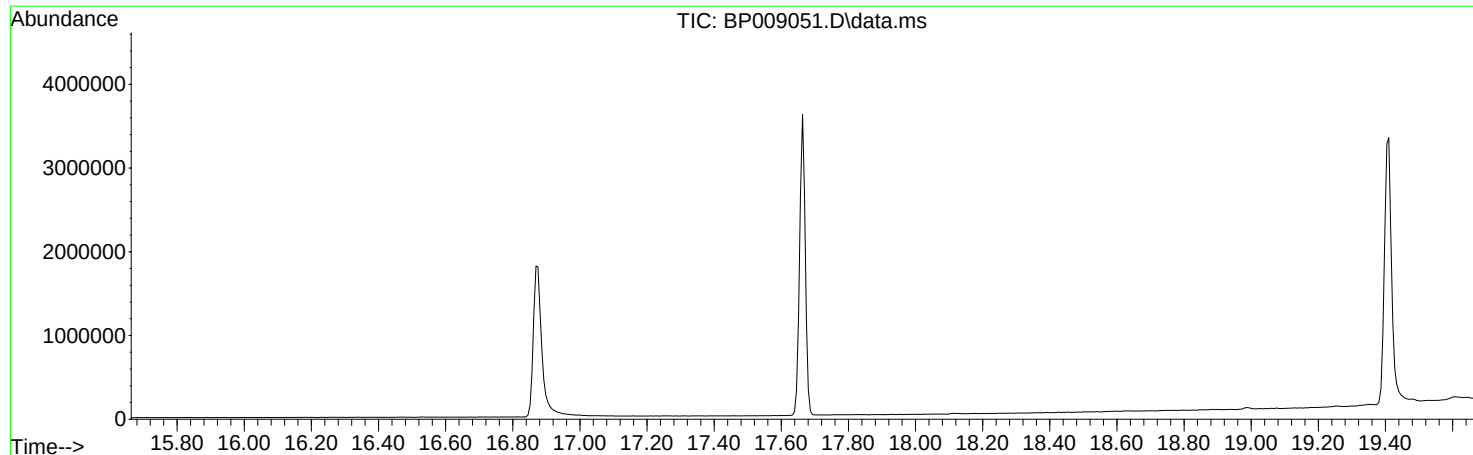




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.9	83624	PASS
68	69	0.00	2	1.8	1791	PASS
69	198	0.00	100	26.5	97009	PASS
70	69	0.00	2	0.4	400	PASS
127	198	10	80	38.3	140141	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	365801	PASS
199	198	5	9	6.9	25097	PASS
275	198	10	60	30.4	111170	PASS
365	198	1	100	4.0	14742	PASS
441	198	0.01	100	14.0	51141	PASS
442	442	100	100	100.0	324181	PASS
443	442	15	24	19.2	62359	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020822\  
Data File : BP009051.D  
Acq On    : 08 Feb 2022  10:27  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 08 12:57:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 07 15:13:17 2022
Response via : Initial Calibration

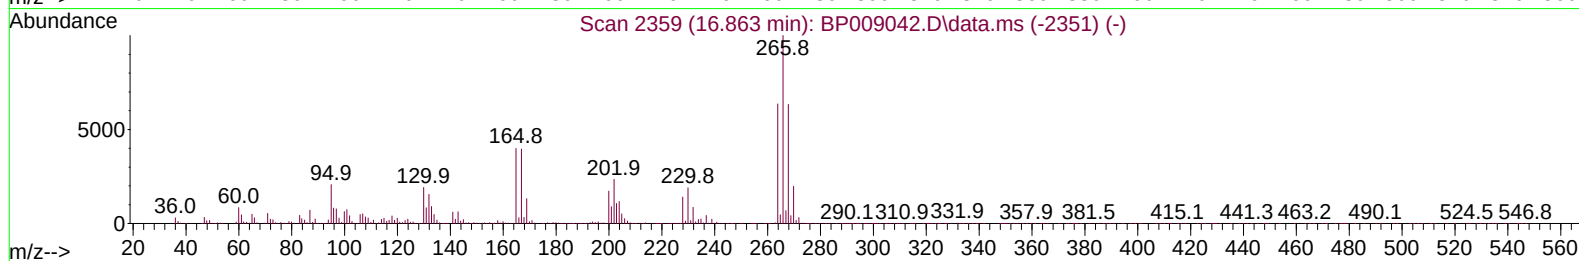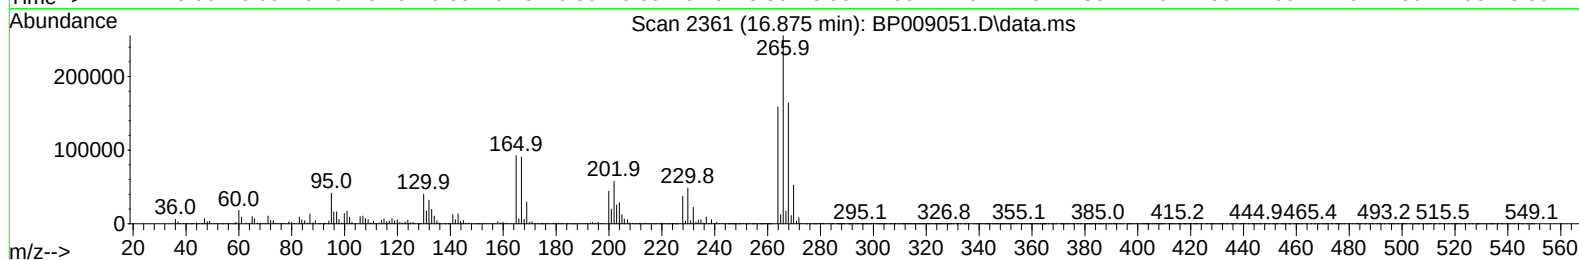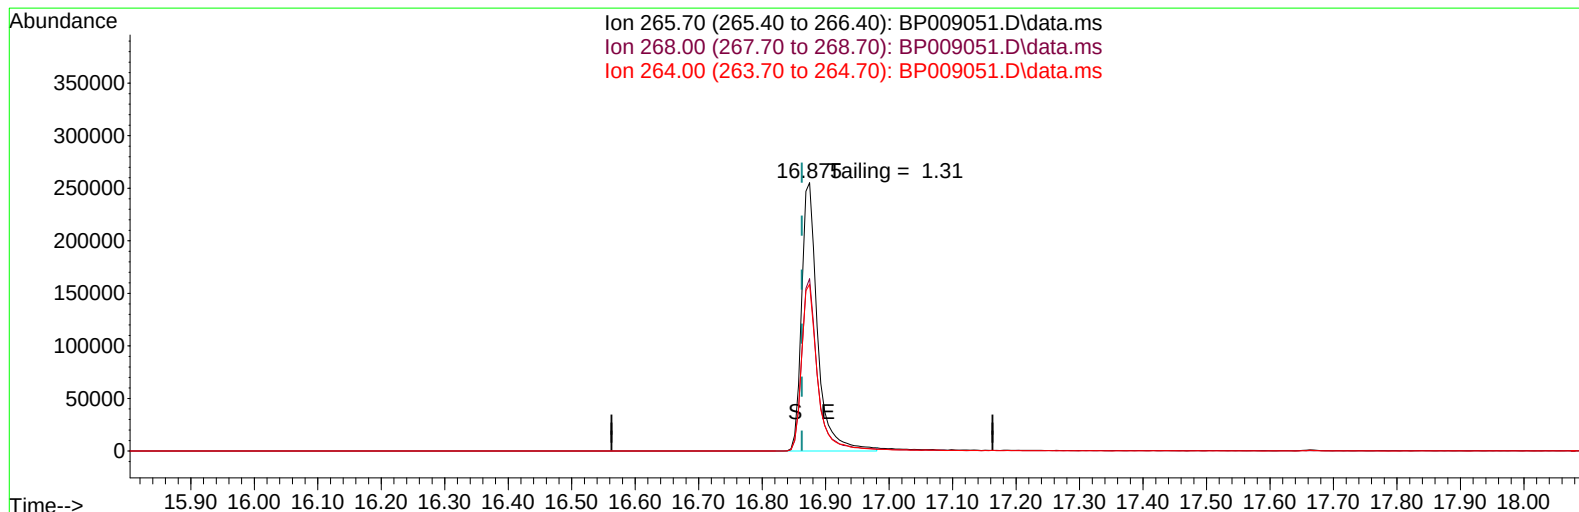

TIC: BP009051.D\data.ms

(70) Pentachlorophenol (C)

16.875min (+ 0.012) 850104.98 ng

response **459020**

Ion	Exp%	Act%
-----	------	------

265.70	100.00	100.00
--------	--------	--------

268.00	63.60	64.24
--------	-------	-------




264.00	62.90	62.13
--------	-------	-------

0.00 0.00 0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020822\
Data File : BP009051.D
Acq On : 08 Feb 2022 10:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 08 12:57:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 07 15:13:17 2022
Response via : Initial Calibration

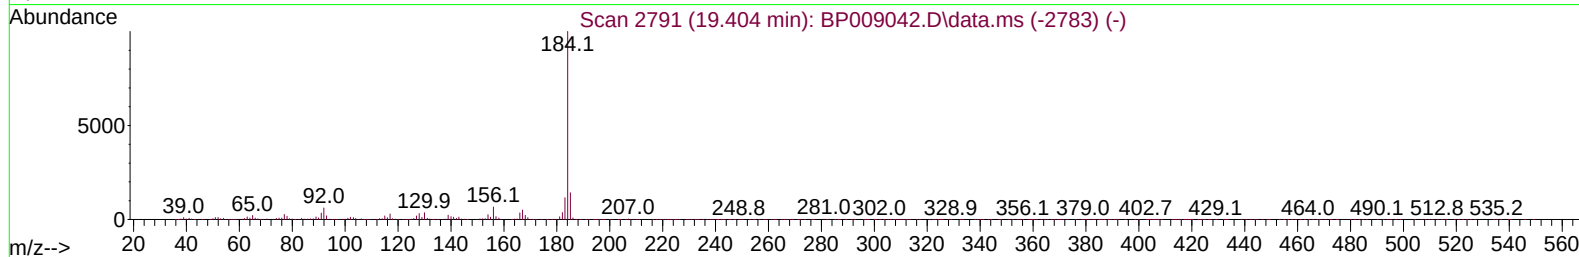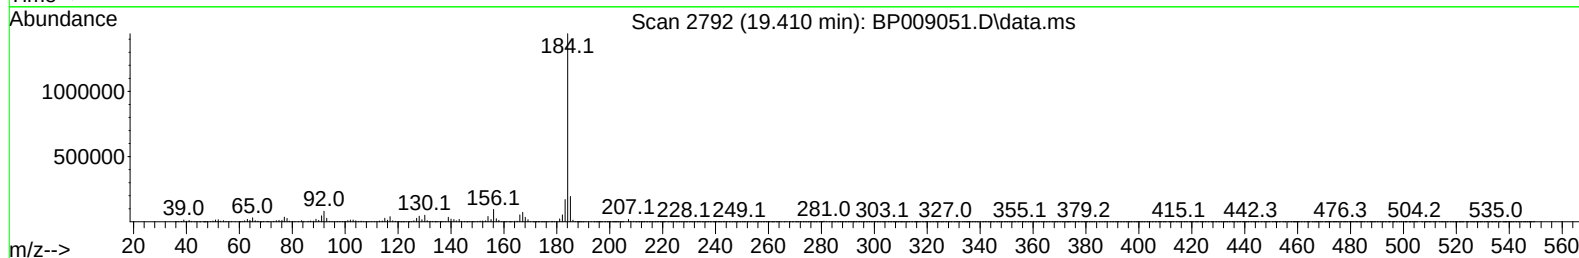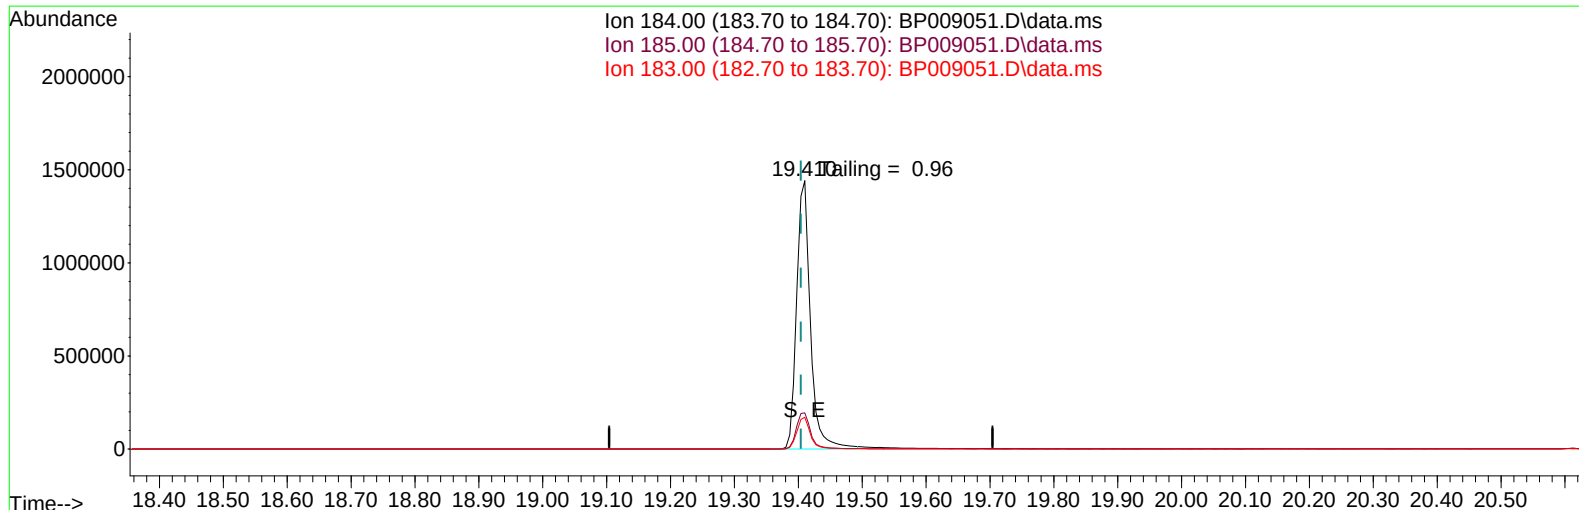

TIC: BP009051.D\data.ms

(77) Benzidine

19.410min (+ 0.006) 564871.60 ng

response 2207267

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	13.49
183.00	11.90	11.82
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/8/2022	BNA_P	<u>BP009051.D</u>
Compound Name	Response	Retention Time
DDT	1071599	20.61
DDD	13348	20.18
DDE	1650	19.68
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14998	1086597	1.38