

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP020823\  
 Data File : BP013792.D  
 Acq On : 08 Feb 2023 12:22  
 Operator : CG/JU  
 Sample : 01381-10DL2 3000X  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 A44K7DL2

Quant Time: Feb 08 23:55:10 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP020723.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Wed Feb 08 00:37:14 2023  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc   | Units  | Dev(Min) |
|-------------------------------|--------|------|----------|--------|--------|----------|
| -----                         |        |      |          |        |        |          |
| Internal Standards            |        |      |          |        |        |          |
| 1) 1,4-Dichlorobenzene-d4     | 8.122  | 152  | 134128   | 20.000 | ng/ul  | 0.00     |
| 20) Naphthalene-d8            | 10.951 | 136  | 573643   | 20.000 | ng/ul  | 0.00     |
| 38) Acenaphthene-d10          | 14.763 | 164  | 418061   | 20.000 | ng/ul  | 0.00     |
| 64) Phenanthrene-d10          | 17.516 | 188  | 1054910  | 20.000 | ng/ul  | 0.00     |
| 79) Chrysene-d12              | 21.586 | 240  | 1159768  | 20.000 | ng/ul  | 0.00     |
| 88) Perylene-d12              | 24.151 | 264  | 1239884  | 20.000 | ng/ul  | 0.00     |
| System Monitoring Compounds   |        |      |          |        |        |          |
| 3) 1,4-Dioxane-d8             | 3.481  | 96   | 150      | 0.046  | ng/uL  | 0.01     |
| 4) Pyridine-d5                | 3.893  | 84   | 65       | 0.007  | ng/ul  | -0.01    |
| 7) Phenol-d5                  | 7.281  | 99   | 19       | 0.002  | ng/ul  | 0.01     |
| 9) Bis-(2-Chloroethyl)eth...  | 7.457  | 67   | 87       | 0.012  | ng/ul  | 0.02     |
| 11) 2-Chlorophenol-d4         | 7.634  | 132  | 17       | 0.002  | ng/ul  | -0.01    |
| 15) 4-Methylphenol-d8         | 8.828  | 113  | 13       | 0.001  | ng/ul  | 0.00     |
| 21) Nitrobenzene-d5           | 9.299  | 128  | 56       | 0.014  | ng/ul  | 0.00     |
| 24) 2-Nitrophenol-d4          | 10.034 | 143  | 24       | 0.005  | ng/ul  | 0.01     |
| 28) 2,4-Dichlorophenol-d3     | 10.716 | 165  | 12       | 0.001  | ng/ul  | 0.15     |
| 31) 4-Chloroaniline-d4        | 11.098 | 131  | 12       | 0.001  | ng/ul  | 0.01     |
| 46) Dimethylphthalate-d6      | 14.181 | 166  | 234      | 0.007  | ng/ul  | 0.02     |
| 49) Acenaphthylene-d8         | 14.457 | 160  | 396      | 0.011  | ng/ul  | 0.00     |
| 54) 4-Nitrophenol-d4          | 14.939 | 143  | 20       | 0.003  | ng/ul  | 0.00     |
| 60) Fluorene-d10              | 15.751 | 176  | 386      | 0.014  | ng/ul  | 0.00     |
| 65) 4,6-Dinitro-2-methylph... | 15.863 | 200  | 12       | 0.002  | ng/ul  | 0.00     |
| 73) Anthracene-d10            | 17.516 | 188  | 1054910  | 21.869 | ng/ul  | -0.10    |
| 81) Pyrene-d10                | 19.833 | 212  | 932      | 0.014  | ng/ul  | 0.00     |
| 92) Benzo(a)pyrene-d12        | 24.151 | 264  | 810730   | 13.050 | ng/ul  | 0.16     |
| Target Compounds              |        |      |          |        |        |          |
|                               |        |      |          |        | Qvalue |          |
| 22) Nitrobenzene              | 9.340  | 77   | 272034   | 25.907 | ng/ul  | 97       |
| -----                         |        |      |          |        |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP020823\  
Data File : BP013792.D  
Acq On : 08 Feb 2023 12:22  
Operator : CG/JU  
Sample : 01381-10DL2 3000X  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
A44K7DL2

Quant Time: Feb 08 23:55:10 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP020723.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Wed Feb 08 00:37:14 2023  
Response via : Initial Calibration

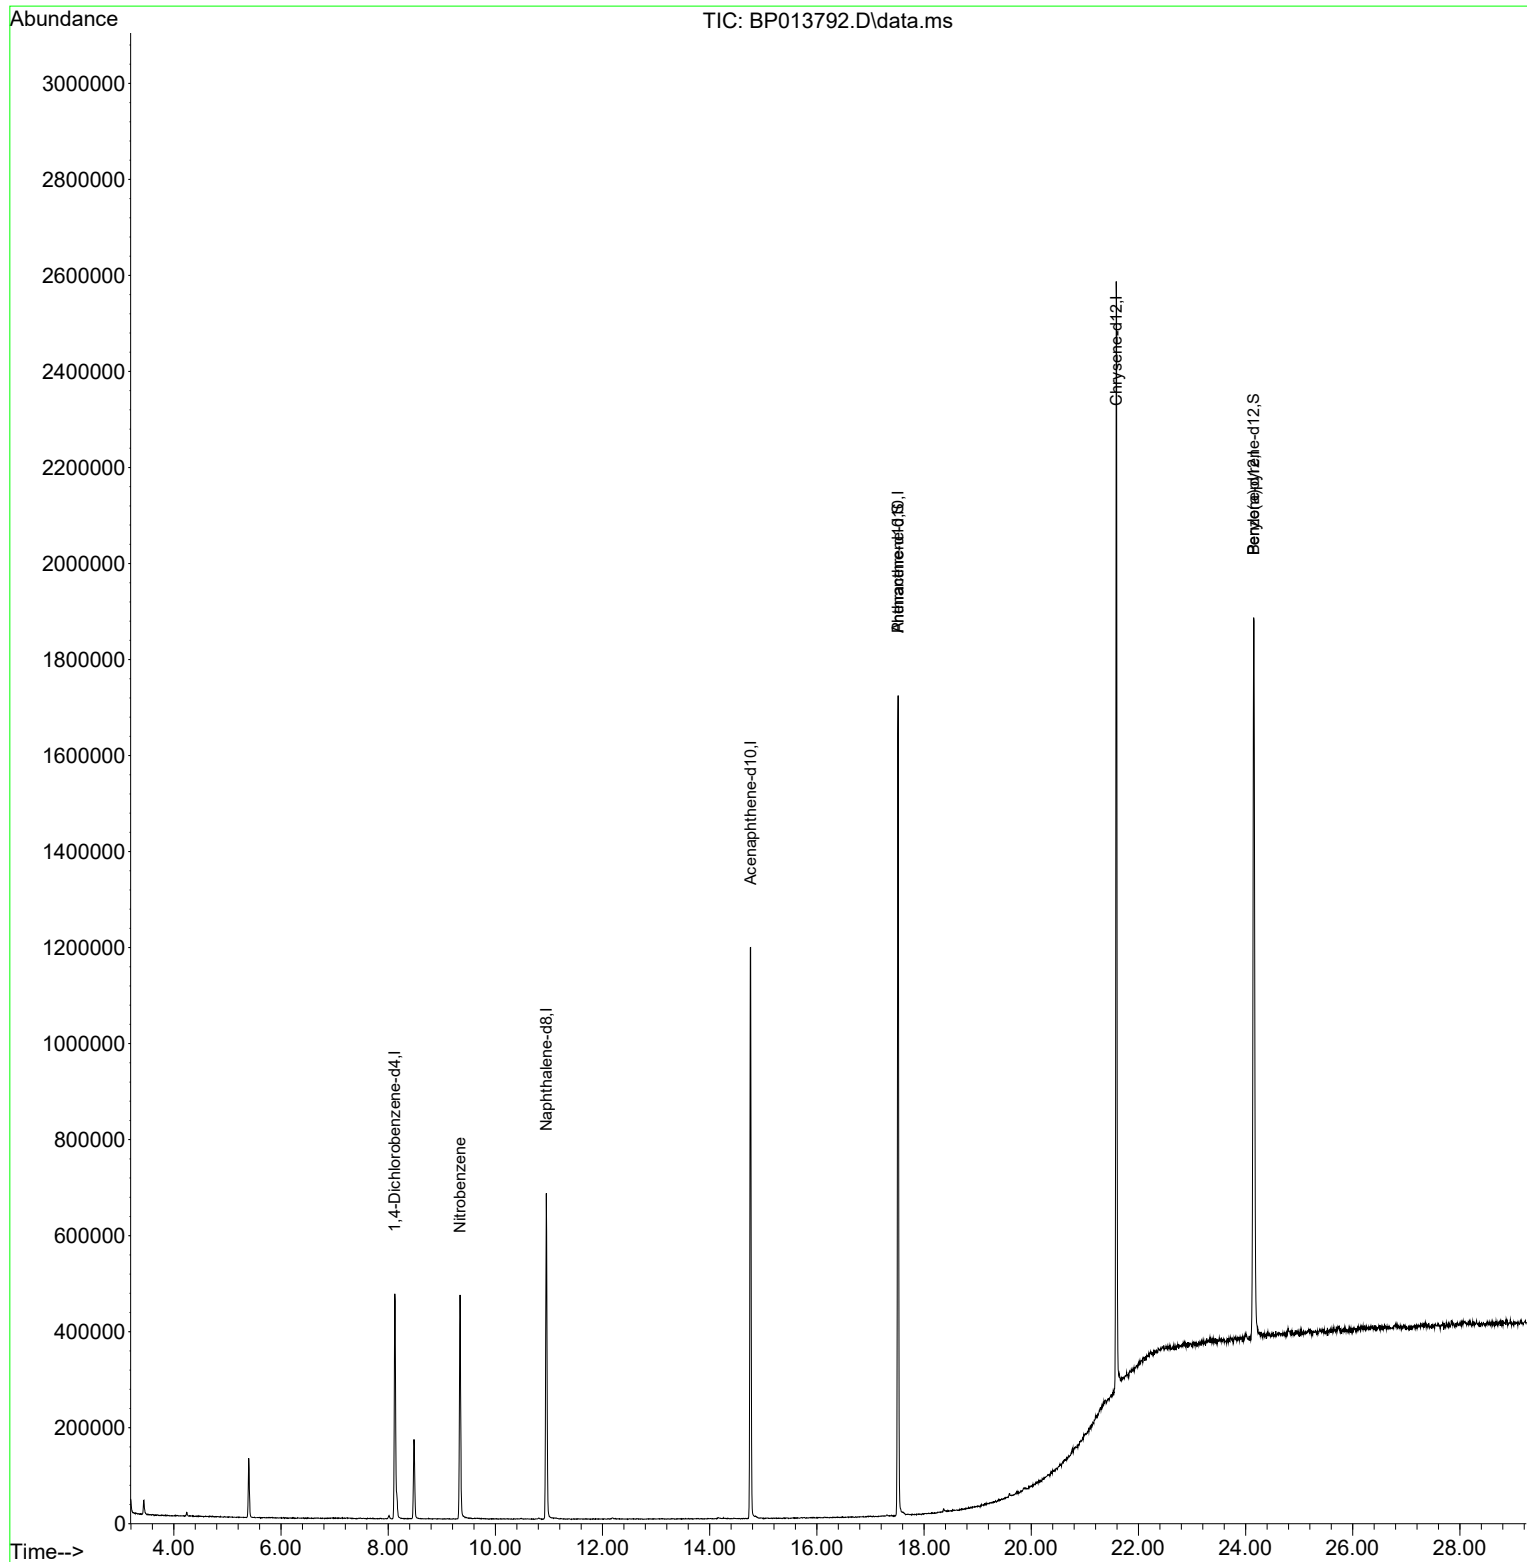

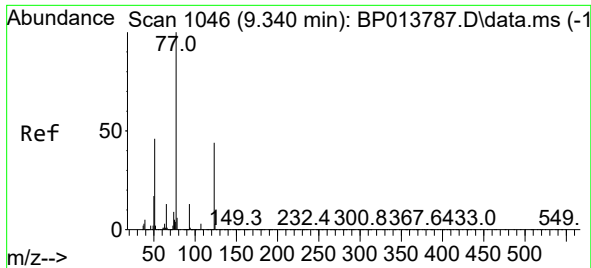

#22  
 Nitrobenzene  
 Concen: 25.907 ng/ul  
 RT: 9.340 min Scan# 10  
 Delta R.T. -0.000 min  
 Lab File: BP013792.D  
 Acq: 08 Feb 2023 12:22

Instrument :  
 BNA\_P  
 ClientSampleId :  
 A44K7DL2

Tgt Ion: 77 Resp: 272034  
 Ion Ratio Lower Upper  
 77 100  
 123 41.7 35.1 52.7  
 65 12.5 10.6 16.0

