

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
 Data File : BP013794.D
 Acq On : 08 Feb 2023 13:31
 Operator : CG/JU
 Sample : 01412-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44L9

Quant Time: Feb 08 23:55:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 08 00:37:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.122	152	162239	20.000	ng/ul	0.00
20) Naphthalene-d8	10.952	136	728698	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.757	164	515326	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.510	188	1254481	20.000	ng/ul	0.00
79) Chrysene-d12	21.586	240	1333687	20.000	ng/ul	0.00
88) Perylene-d12	24.151	264	1314206	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.470	96	17956	4.587	ng/uL	0.00
4) Pyridine-d5	3.905	84	143701	12.383	ng/ul	0.00
7) Phenol-d5	7.269	99	75125	5.197	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.440	67	218585	25.805	ng/ul	0.00
11) 2-Chlorophenol-d4	7.646	132	206245	19.382	ng/ul	0.00
15) 4-Methylphenol-d8	8.822	113	158967	13.455	ng/ul	0.00
21) Nitrobenzene-d5	9.293	128	136259	26.875	ng/ul	0.00
24) 2-Nitrophenol-d4	10.022	143	145760	24.899	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.563	165	303707	25.458	ng/ul	0.00
31) 4-Chloroaniline-d4	11.081	131	614942	36.366	ng/ul	0.00
46) Dimethylphthalate-d6	14.157	166	1263023	31.118	ng/ul	0.00
49) Acenaphthylene-d8	14.451	160	1282856	29.198	ng/ul	0.00
54) 4-Nitrophenol-d4	14.945	143	27792	3.843	ng/ul	0.00
60) Fluorene-d10	15.751	176	1062441	30.731	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.857	200	79918	10.384	ng/ul	0.00
73) Anthracene-d10	17.610	188	1832112	31.939	ng/ul	0.00
81) Pyrene-d10	19.828	212	2350943	31.084	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.986	264	2192080	33.289	ng/ul	0.00
Target Compounds						
					Qvalue	
13) 2-Methylphenol	8.481	108	14743	1.302	ng/ul	99
32) 4-Chloroaniline	11.105	127	23311	1.367	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013794.D
Acq On : 08 Feb 2023 13:31
Operator : CG/JU
Sample : 01412-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44L9

Quant Time: Feb 08 23:55:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 08 00:37:14 2023
Response via : Initial Calibration




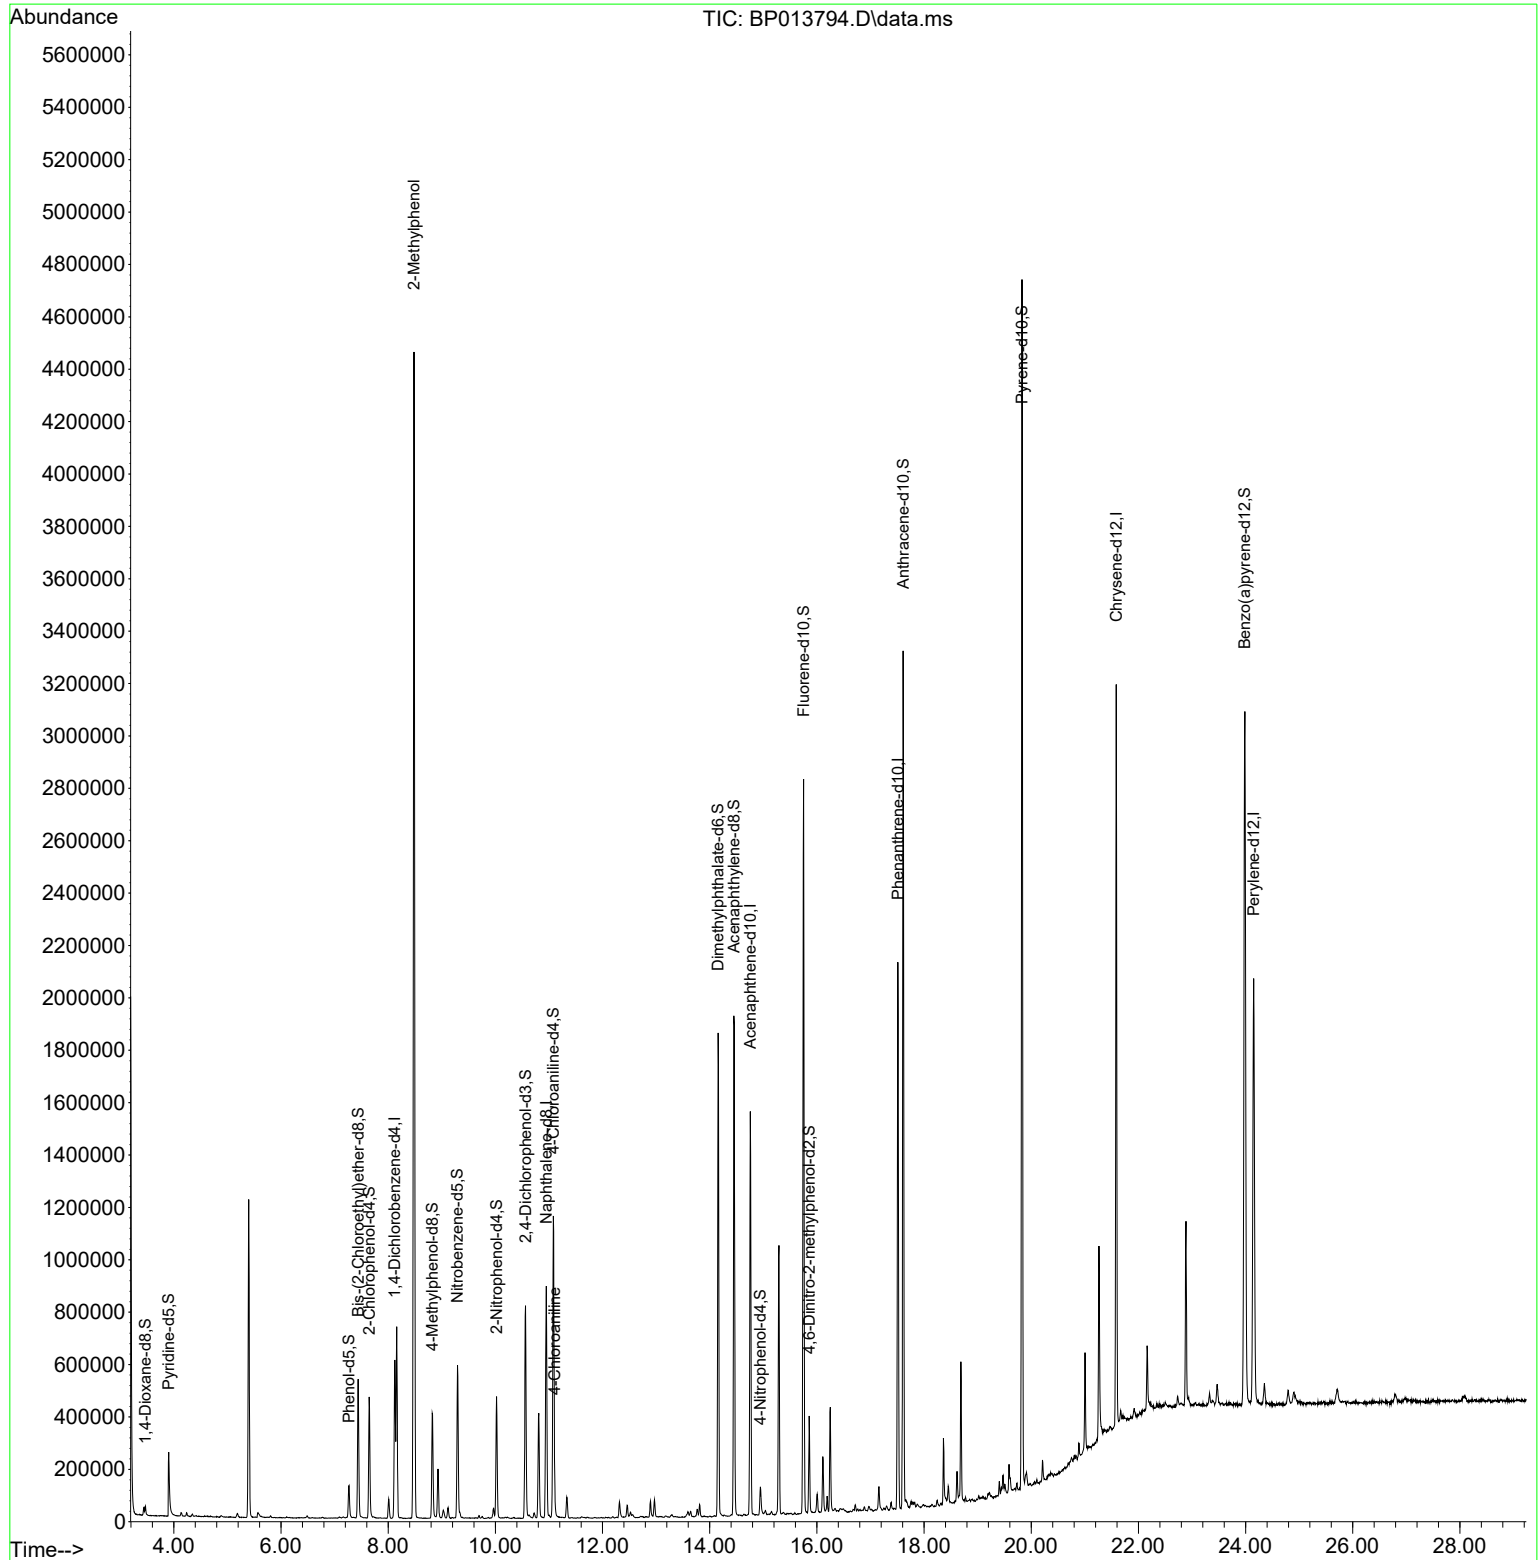


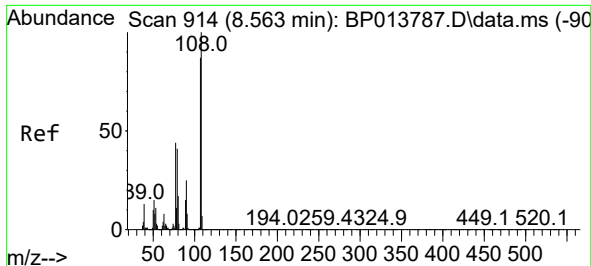

#13
2-Methylphenol
Concen: 1.302 ng/ul
RT: 8.481 min Scan# 90
Delta R.T. -0.082 min
Lab File: BP013794.D
Acq: 08 Feb 2023 13:31

Instrument :
BNA_P
ClientSampleId :
A44L9

Tgt Ion:108 Resp: 14743
Ion Ratio Lower Upper
108 100
107 90.9 71.9 107.9

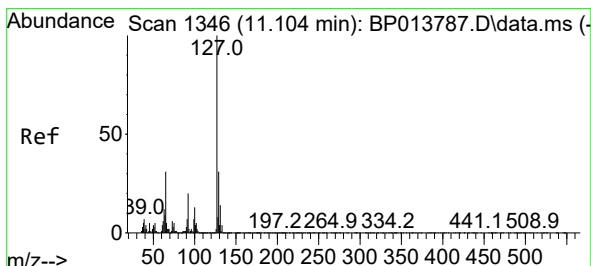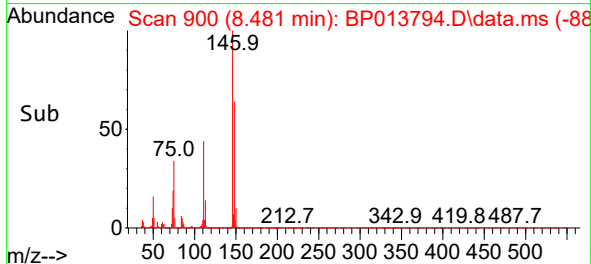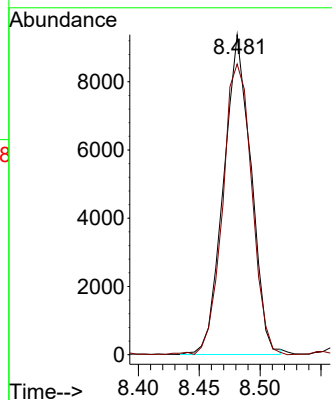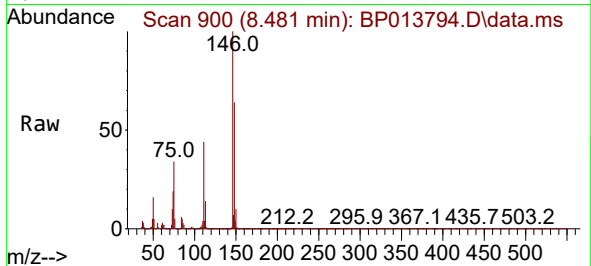

#32
4-Chloroaniline
Concen: 1.367 ng/ul
RT: 11.105 min Scan# 1346
Delta R.T. -0.006 min
Lab File: BP013794.D
Acq: 08 Feb 2023 13:31

Tgt Ion:127 Resp: 23311
Ion Ratio Lower Upper
127 100
129 31.5 26.2 39.4

