

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
 Data File : BP013795.D
 Acq On : 08 Feb 2023 14:05
 Operator : CG/JU
 Sample : 01412-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44M3

Quant Time: Feb 08 23:55:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 08 00:37:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.122	152	159627	20.000	ng/ul	0.00
20) Naphthalene-d8	10.951	136	715495	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.757	164	521276	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.510	188	1259981	20.000	ng/ul	0.00
79) Chrysene-d12	21.586	240	1329498	20.000	ng/ul	0.00
88) Perylene-d12	24.151	264	1309631	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.469	96	14092	3.659	ng/uL	0.00
4) Pyridine-d5	3.916	84	19655	1.721	ng/ul	0.01
7) Phenol-d5	7.269	99	70350	4.946	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.440	67	218793	26.252	ng/ul	0.00
11) 2-Chlorophenol-d4	7.646	132	217303	20.756	ng/ul	0.00
15) 4-Methylphenol-d8	8.828	113	147434	12.683	ng/ul	0.00
21) Nitrobenzene-d5	9.293	128	137888	27.698	ng/ul	0.00
24) 2-Nitrophenol-d4	10.022	143	159497	27.749	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.563	165	292961	25.011	ng/ul	0.00
31) 4-Chloroaniline-d4	11.081	131	136147	8.200	ng/ul	0.00
46) Dimethylphthalate-d6	14.157	166	1208393	29.432	ng/ul	0.00
49) Acenaphthylene-d8	14.451	160	1245376	28.022	ng/ul	0.00
54) 4-Nitrophenol-d4	14.945	143	30271	4.139	ng/ul	0.00
60) Fluorene-d10	15.751	176	1030285	29.461	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.857	200	171839	22.230	ng/ul	0.00
73) Anthracene-d10	17.610	188	1850708	32.123	ng/ul	0.00
81) Pyrene-d10	19.827	212	2433016	32.271	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.986	264	2222369	33.867	ng/ul	0.00
Target Compounds						
					Qvalue	
22) Nitrobenzene	9.340	77	212373	16.215	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013795.D
Acq On : 08 Feb 2023 14:05
Operator : CG/JU
Sample : 01412-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44M3

Quant Time: Feb 08 23:55:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 08 00:37:14 2023
Response via : Initial Calibration

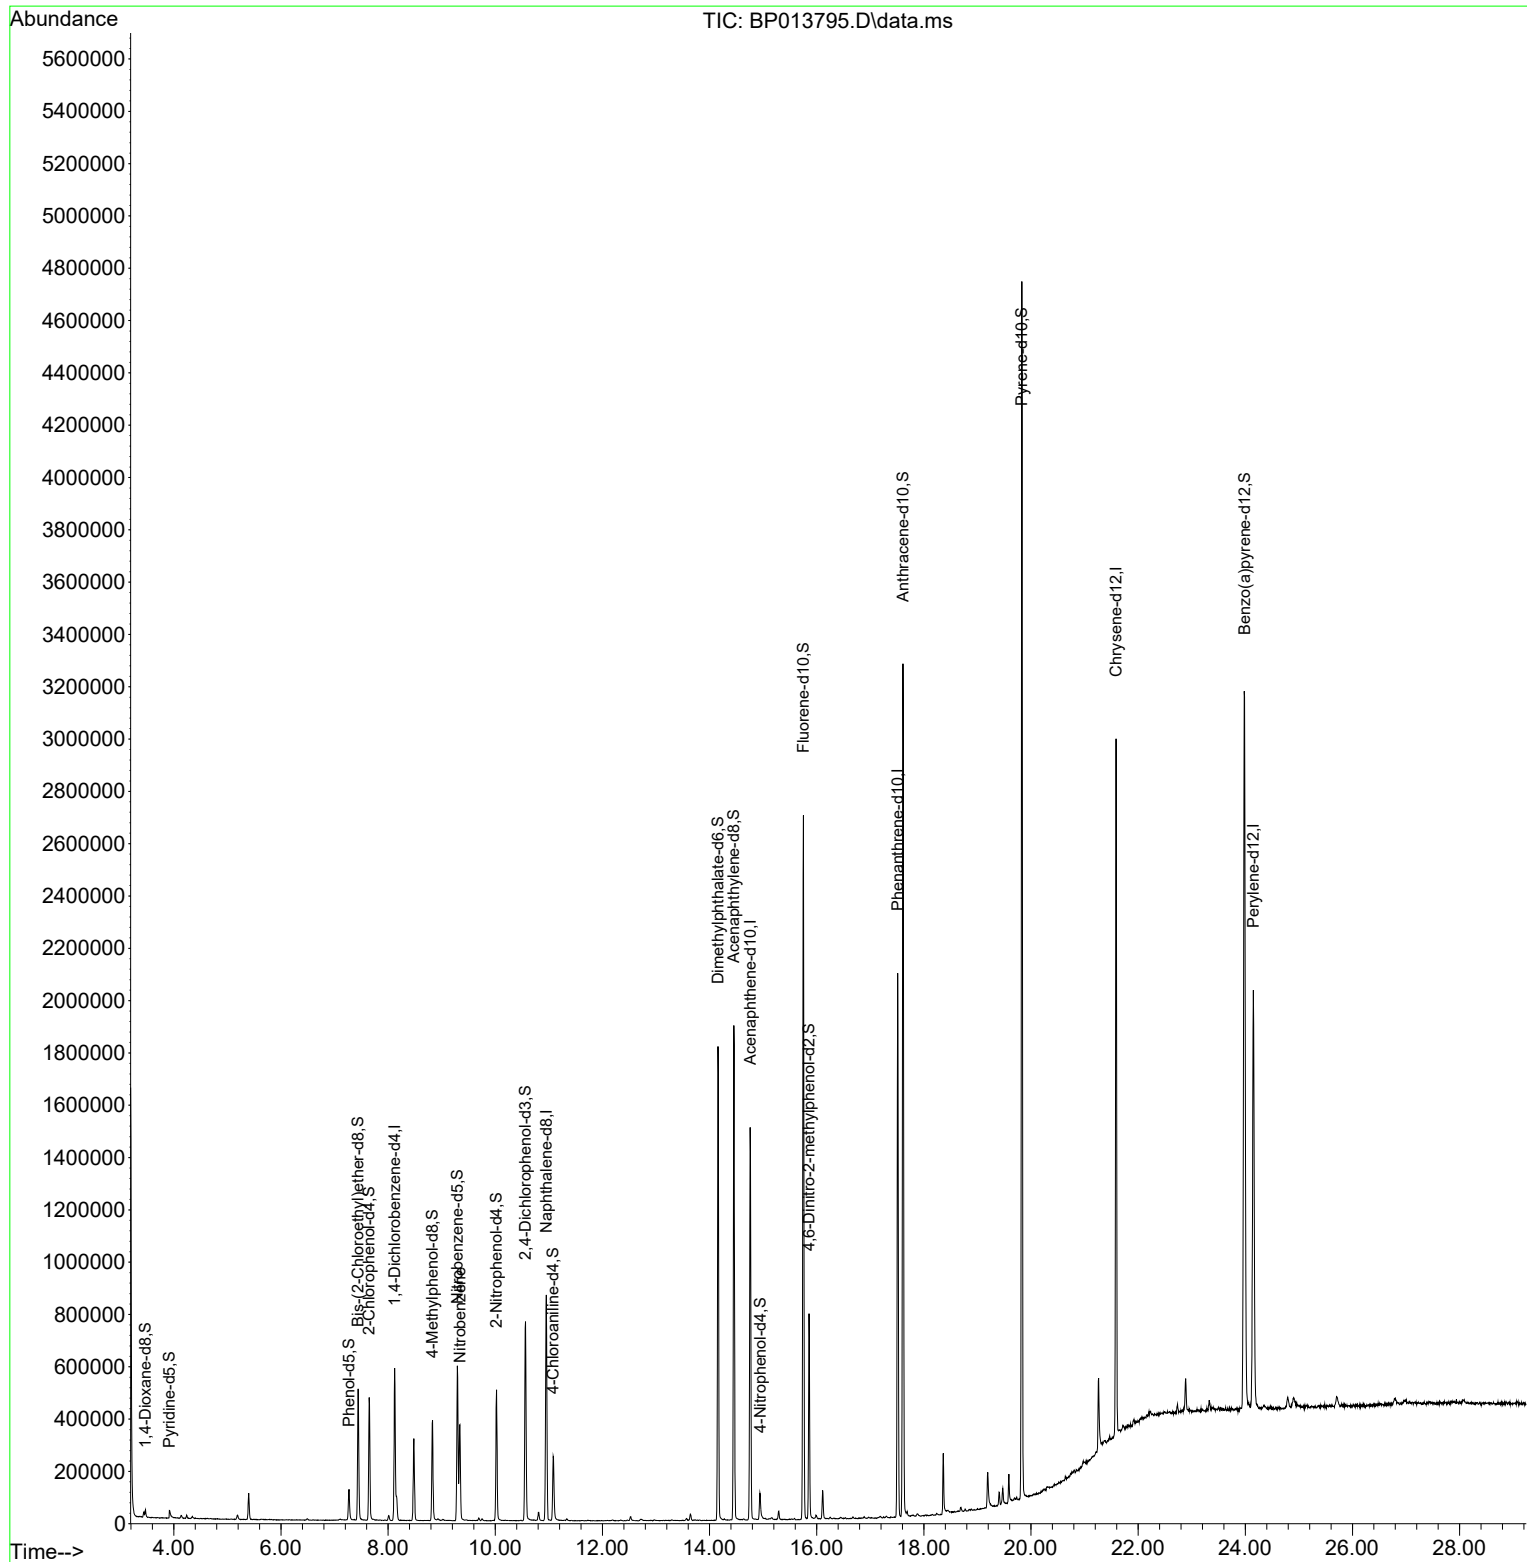

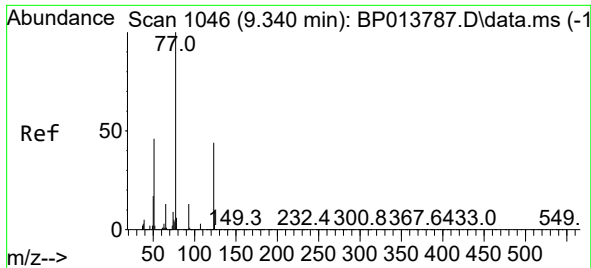

#22
 Nitrobenzene
 Concen: 16.215 ng/ul
 RT: 9.340 min Scan# 10
 Delta R.T. -0.000 min
 Lab File: BP013795.D
 Acq: 08 Feb 2023 14:05

Instrument :
 BNA_P
 ClientSampleId :
 A44M3

Tgt Ion: 77 Resp: 212373
 Ion Ratio Lower Upper
 77 100
 123 44.0 35.1 52.7
 65 12.7 10.6 16.0

