

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
 Data File : BP013796.D
 Acq On : 08 Feb 2023 14:39
 Operator : CG/JU
 Sample : 01422-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B45

Quant Time: Feb 08 23:55:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 08 00:37:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.122	152	183997	20.000	ng/ul	0.00
20) Naphthalene-d8	10.951	136	817491	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.757	164	575791	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.510	188	1390142	20.000	ng/ul	0.00
79) Chrysene-d12	21.586	240	1423518	20.000	ng/ul	0.00
88) Perylene-d12	24.151	264	1349400	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.470	96	16482	3.713	ng/uL	0.00
4) Pyridine-d5	3.911	84	67507	5.129	ng/ul	0.00
7) Phenol-d5	7.269	99	72878	4.445	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.440	67	226250	23.551	ng/ul	0.00
11) 2-Chlorophenol-d4	7.646	132	221071	18.319	ng/ul	0.00
15) 4-Methylphenol-d8	8.822	113	155264	11.587	ng/ul	0.00
21) Nitrobenzene-d5	9.293	128	136076	23.924	ng/ul	0.00
24) 2-Nitrophenol-d4	10.022	143	149939	22.831	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.563	165	287030	21.447	ng/ul	0.00
31) 4-Chloroaniline-d4	11.081	131	308610	16.268	ng/ul	0.00
46) Dimethylphthalate-d6	14.157	166	1211321	26.710	ng/ul	0.00
49) Acenaphthylene-d8	14.451	160	1191460	24.270	ng/ul	0.00
54) 4-Nitrophenol-d4	14.940	143	31190	3.860	ng/ul	0.00
60) Fluorene-d10	15.751	176	1015726	26.295	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.857	200	155374	18.218	ng/ul	0.00
73) Anthracene-d10	17.610	188	1861397	29.283	ng/ul	0.00
81) Pyrene-d10	19.828	212	2411933	29.878	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.986	264	2072784	30.656	ng/ul	0.00
Target Compounds						
78) Di-n-butylphthalate	18.439	149	441870	5.588	ng/ul	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013796.D
Acq On : 08 Feb 2023 14:39
Operator : CG/JU
Sample : 01422-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B45


Quant Time: Feb 08 23:55:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 08 00:37:14 2023
Response via : Initial Calibration

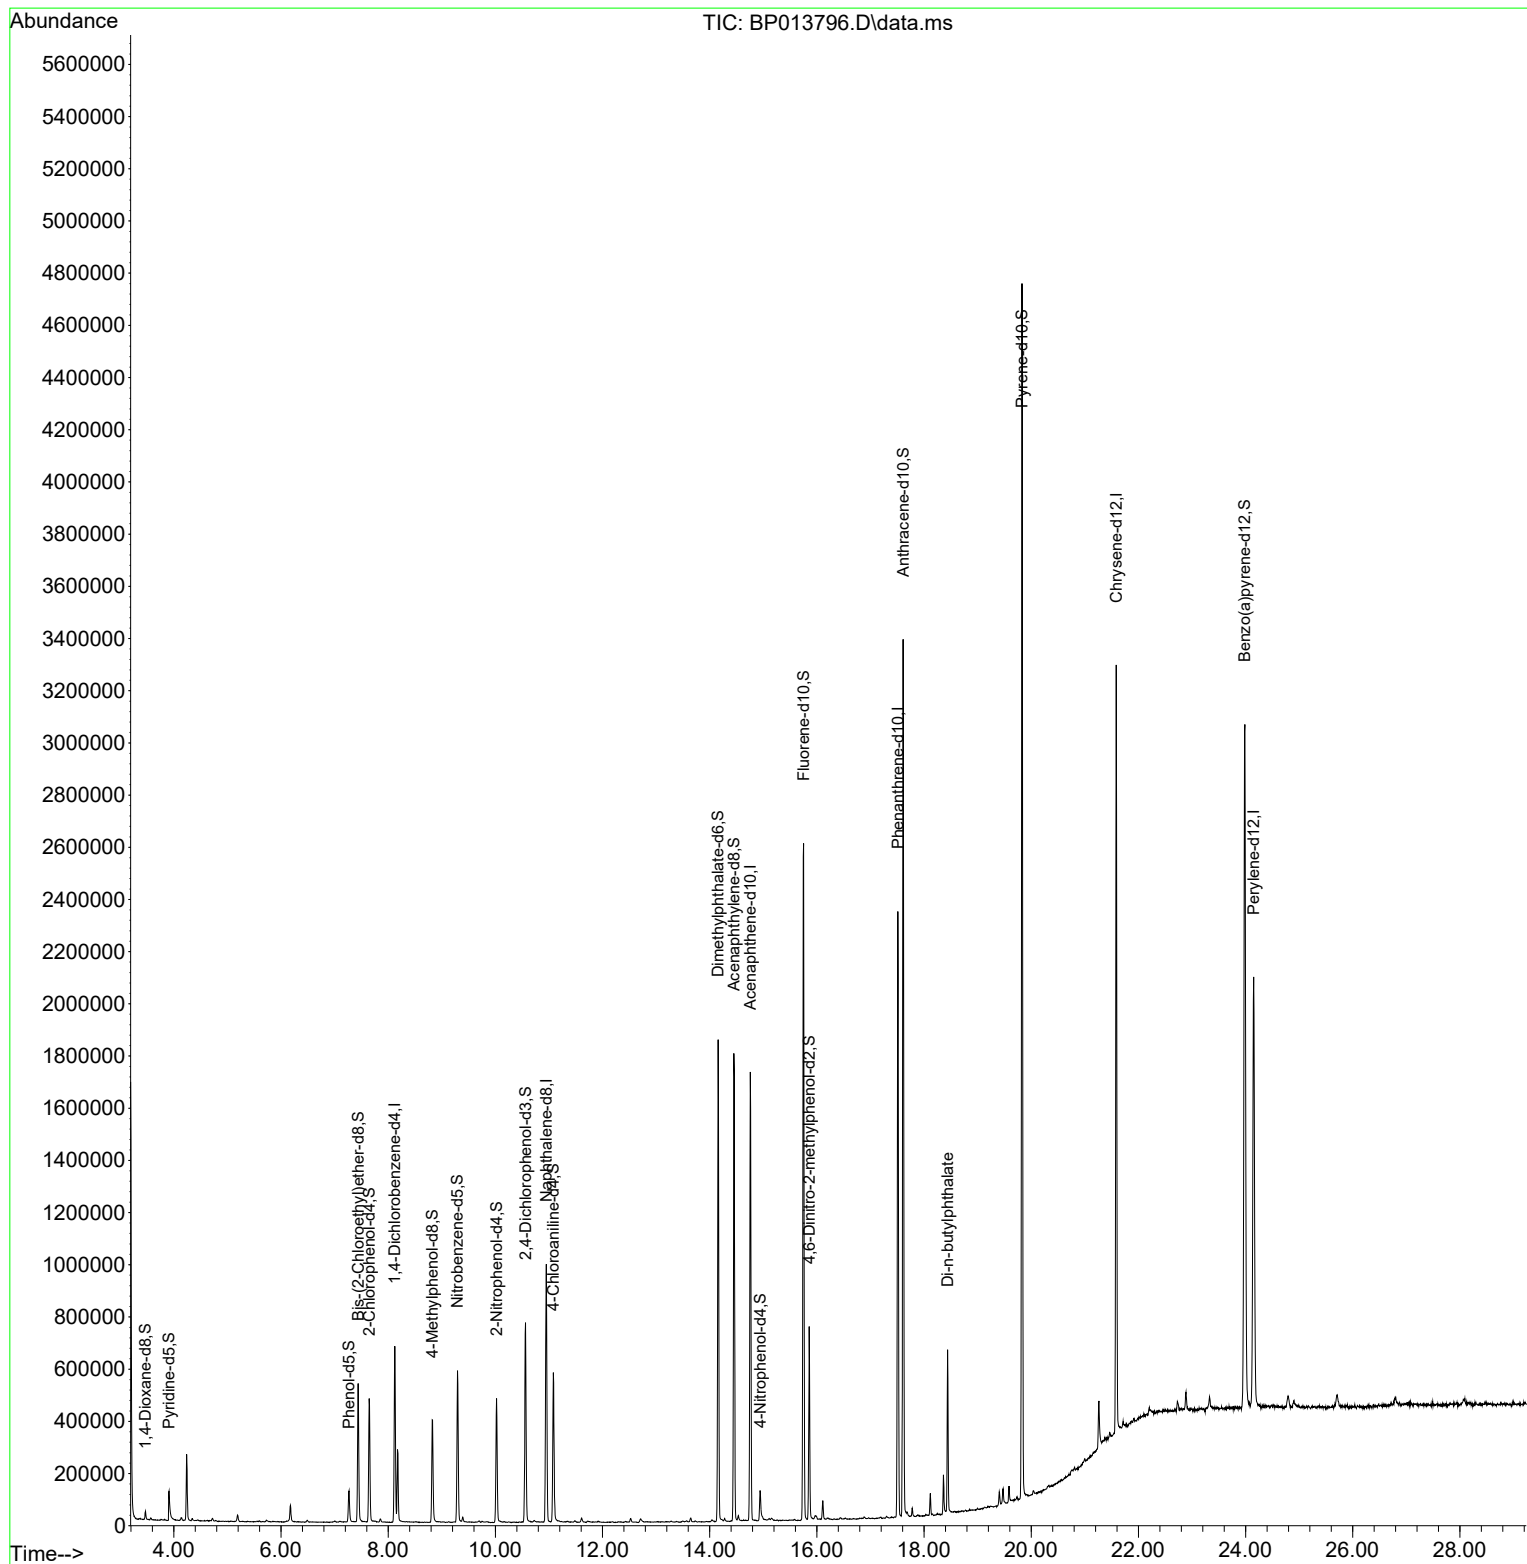

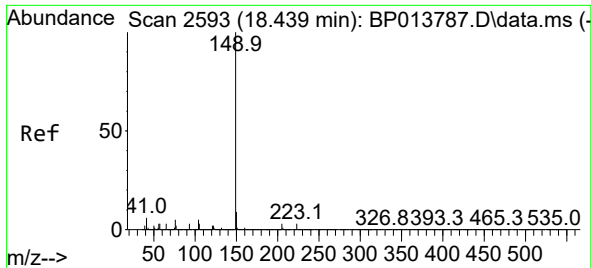

#78
 Di-n-butylphthalate
 Concen: 5.588 ng/ul
 RT: 18.439 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP013796.D
 Acq: 08 Feb 2023 14:39

Instrument :
 BNA_P
 ClientSampleId :
 C0B45

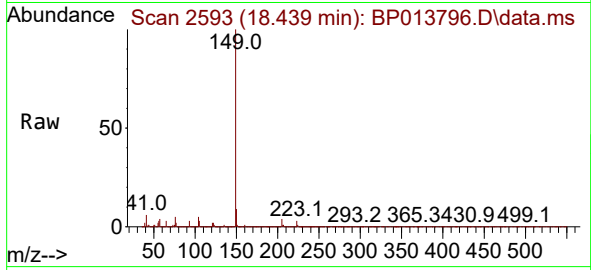

Tgt Ion:149 Resp: 441870
 Ion Ratio Lower Upper
 149 100
 150 8.9 7.1 10.7
 104 5.1 4.1 6.1

