




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013790.D
Acq On : 08 Feb 2023 11:07
Operator : CG/JU
Sample : 01381-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44M8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/09/2023
Supervised By :Sohil Jodhani 02/09/2023

Quant Time: Feb 08 23:54:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 08 00:37:14 2023
Response via : Initial Calibration

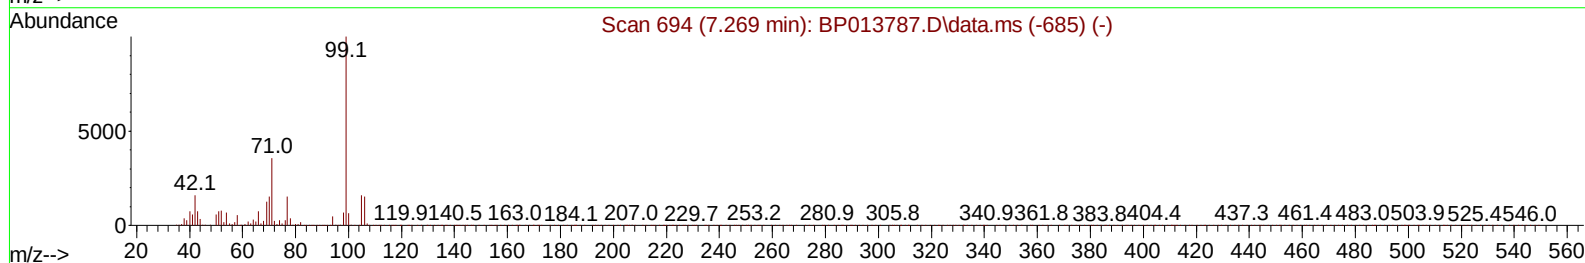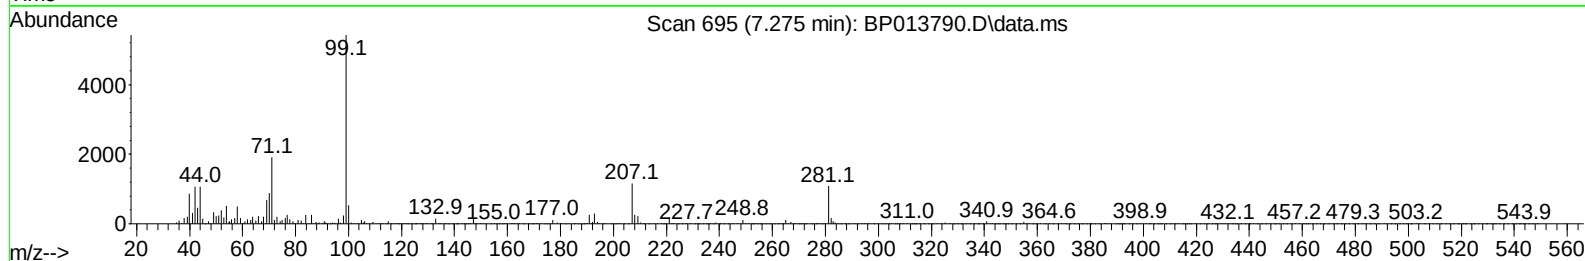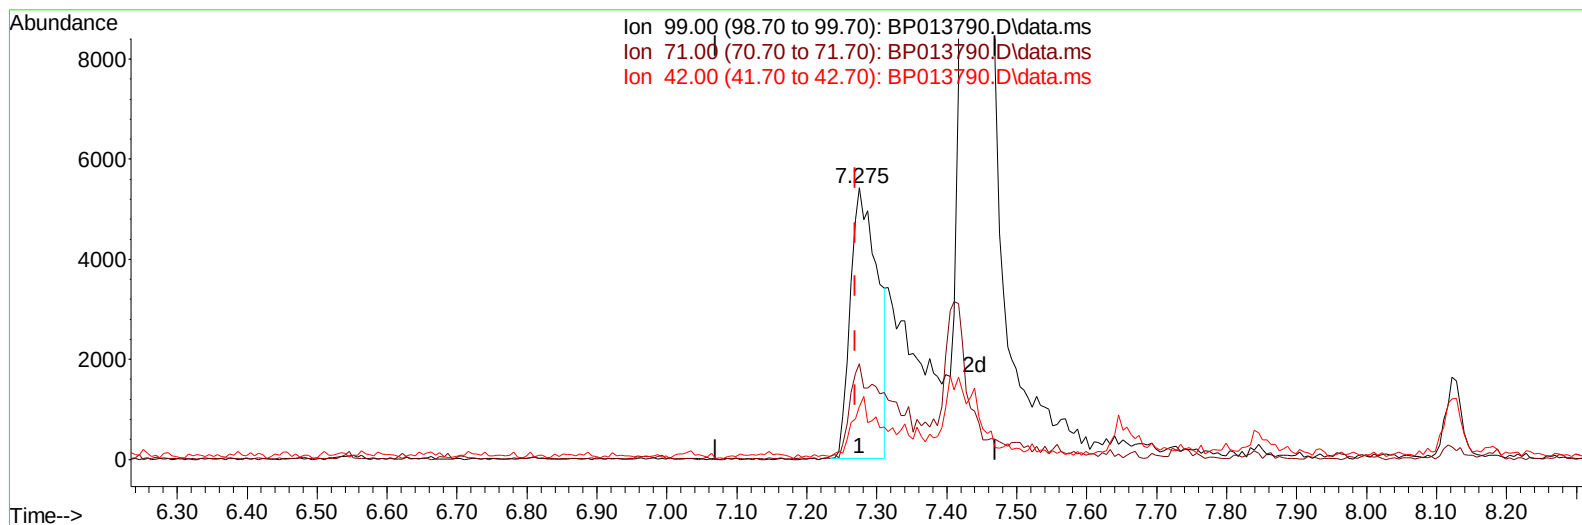

TIC: BP013790.D\data.ms

(7) Phenol-d5 (S)

7.275min (+ 0.006) 1.08 ng/ul

response 14539

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	34.70	35.18
42.00	16.20	19.55#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
 Data File : BP013790.D
 Acq On : 08 Feb 2023 11:07
 Operator : CG/JU
 Sample : 01381-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44M8

Manual IntegrationsAPPROVED

Quant Time: Feb 08 23:54:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 08 00:37:14 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/09/2023
 Supervised By :Sohil Jodhani 02/09/2023

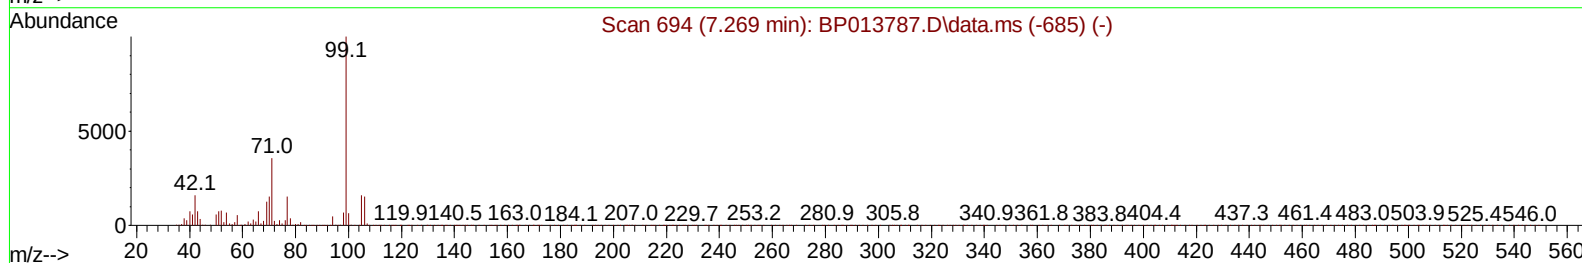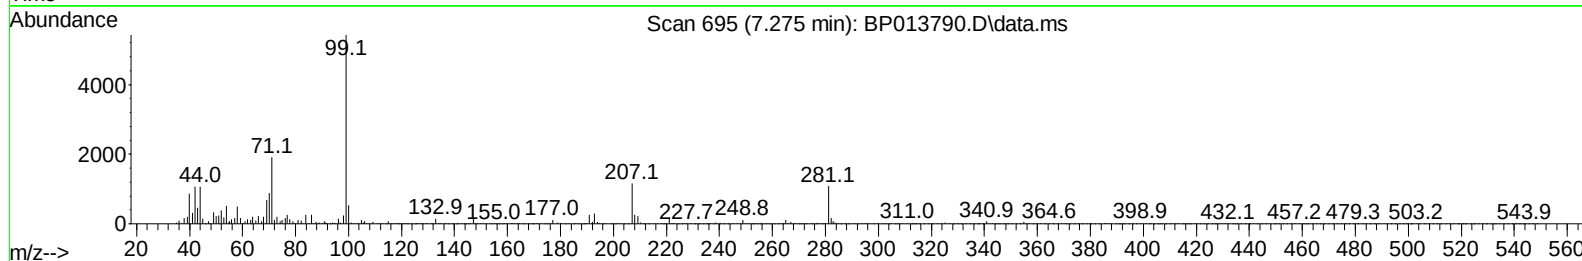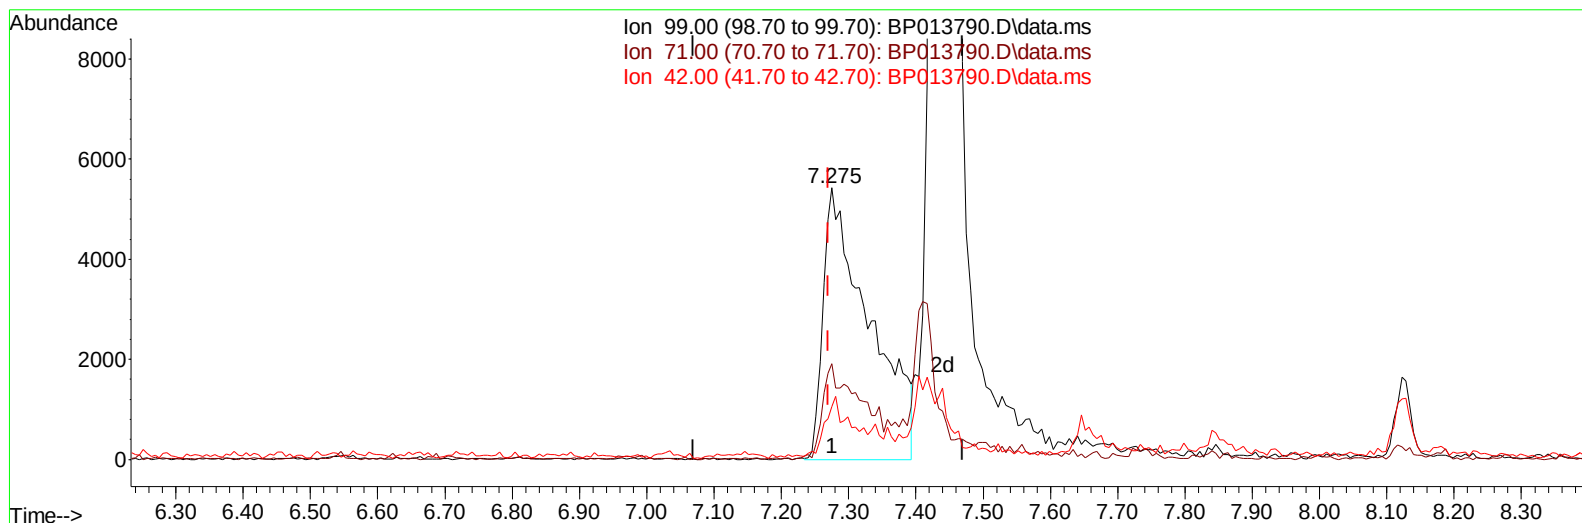

TIC: BP013790.D\data.ms

(7) Phenol-d5 (S)

7.275min (+ 0.006) 1.90 ng/ul m

response 25689

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	34.70	35.18
42.00	16.20	19.55#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013790.D
Acq On : 08 Feb 2023 11:07
Operator : CG/JU
Sample : 01381-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44M8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/09/2023
Supervised By :Sohil Jodhani 02/09/2023

Quant Time: Feb 08 23:54:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 08 00:37:14 2023
Response via : Initial Calibration

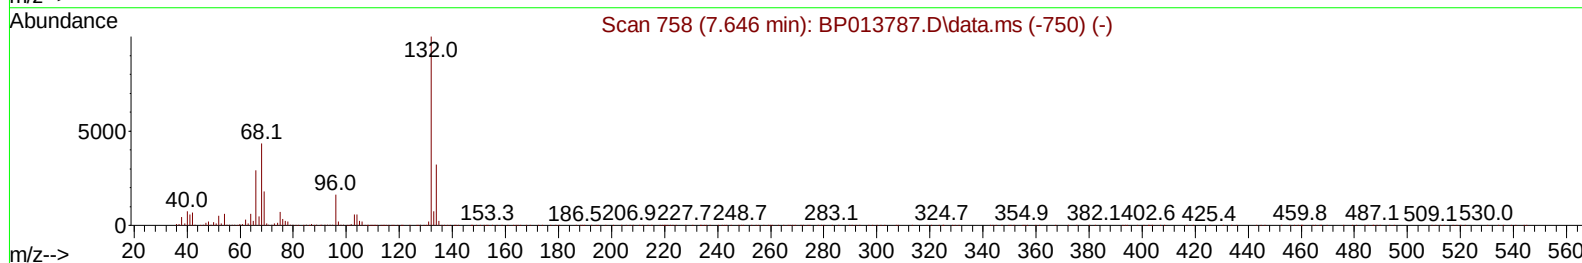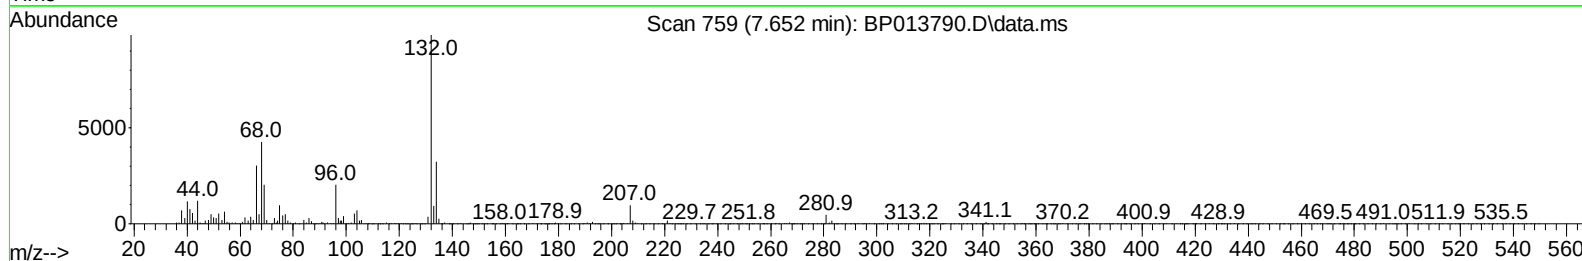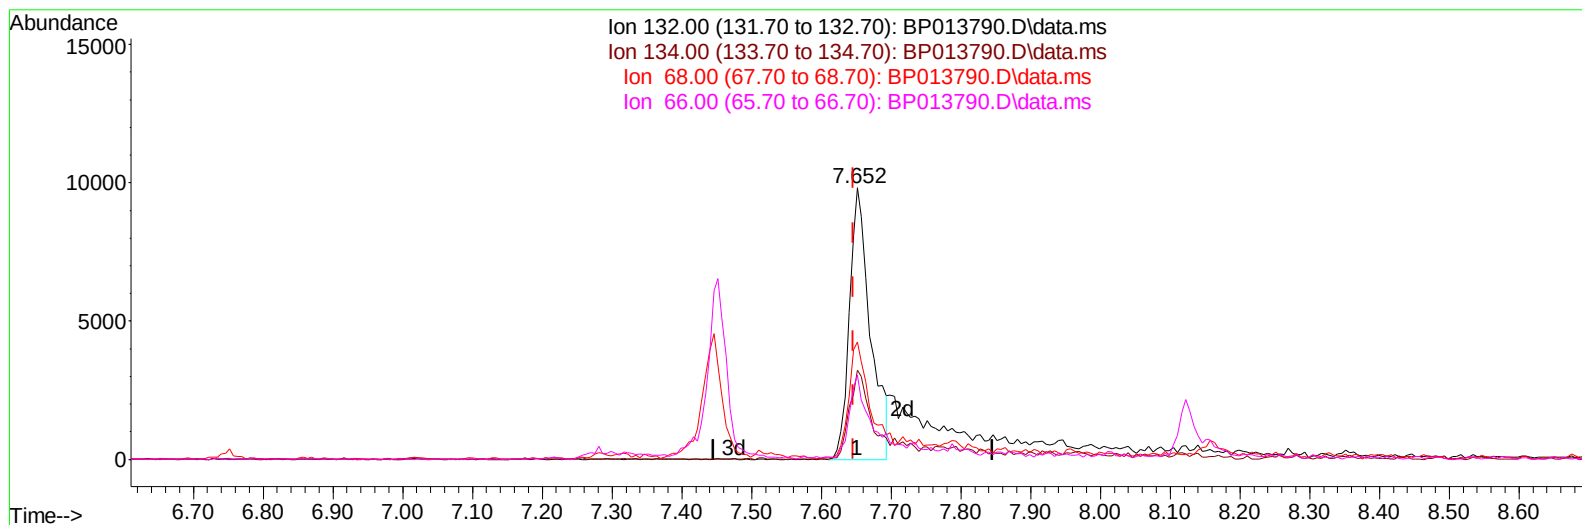

TIC: BP013790.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.652min (+ 0.006) 2.06 ng/u1

response 20464

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	33.40	32.84
68.00	43.20	43.33
66.00	29.40	30.99




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013790.D
Acq On : 08 Feb 2023 11:07
Operator : CG/JU
Sample : 01381-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44M8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/09/2023
Supervised By :Sohil Jodhani 02/09/2023

Quant Time: Feb 08 23:54:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 08 00:37:14 2023
Response via : Initial Calibration

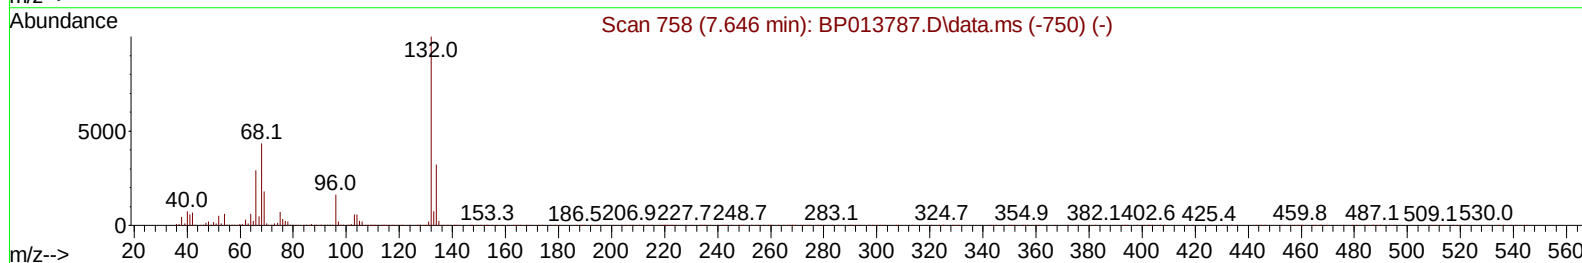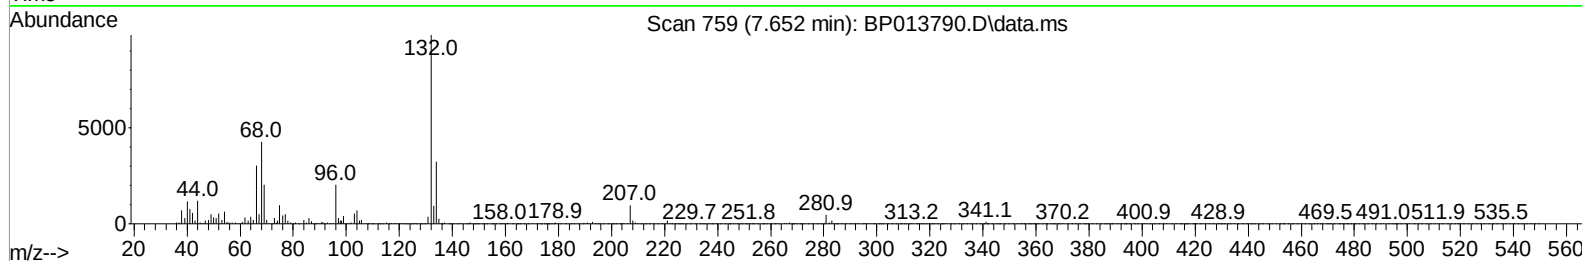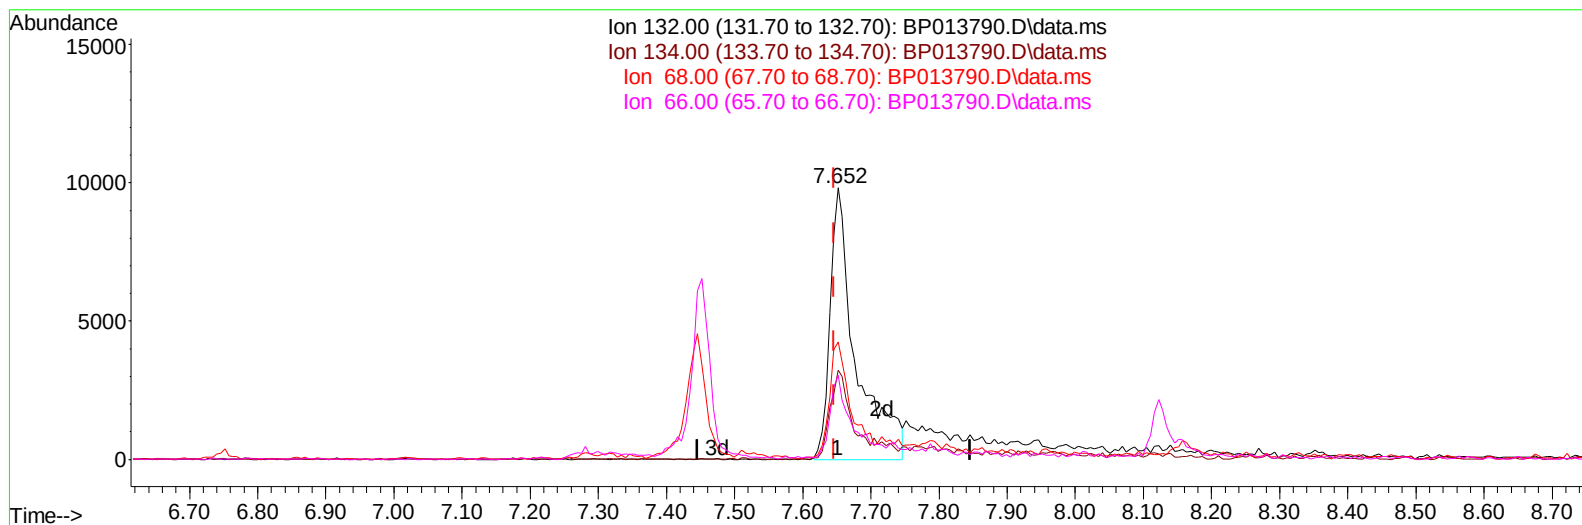

TIC: BP013790.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.652min (+ 0.006) 2.60 ng/ul m

response 25858

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	33.40	32.84
68.00	43.20	43.33
66.00	29.40	30.99




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
 Data File : BP013790.D
 Acq On : 08 Feb 2023 11:07
 Operator : CG/JU
 Sample : 01381-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44M8

Manual IntegrationsAPPROVED

Quant Time: Feb 08 23:54:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 08 00:37:14 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/09/2023
 Supervised By :Sohil Jodhani 02/09/2023

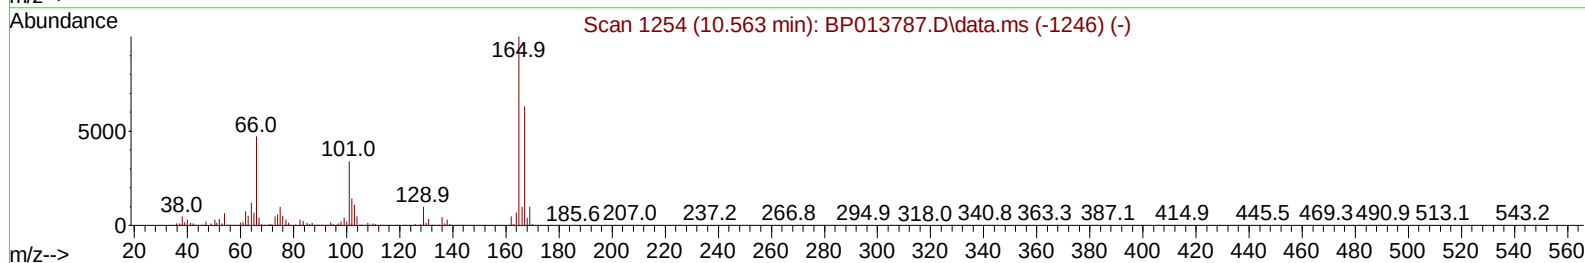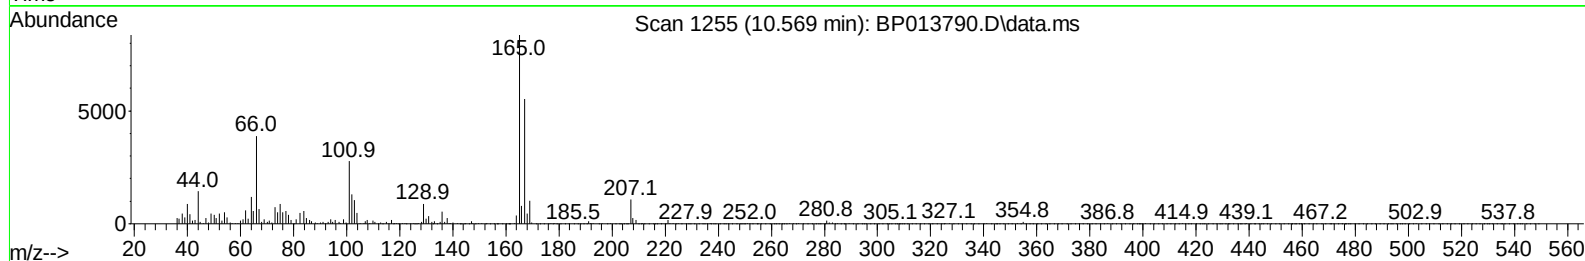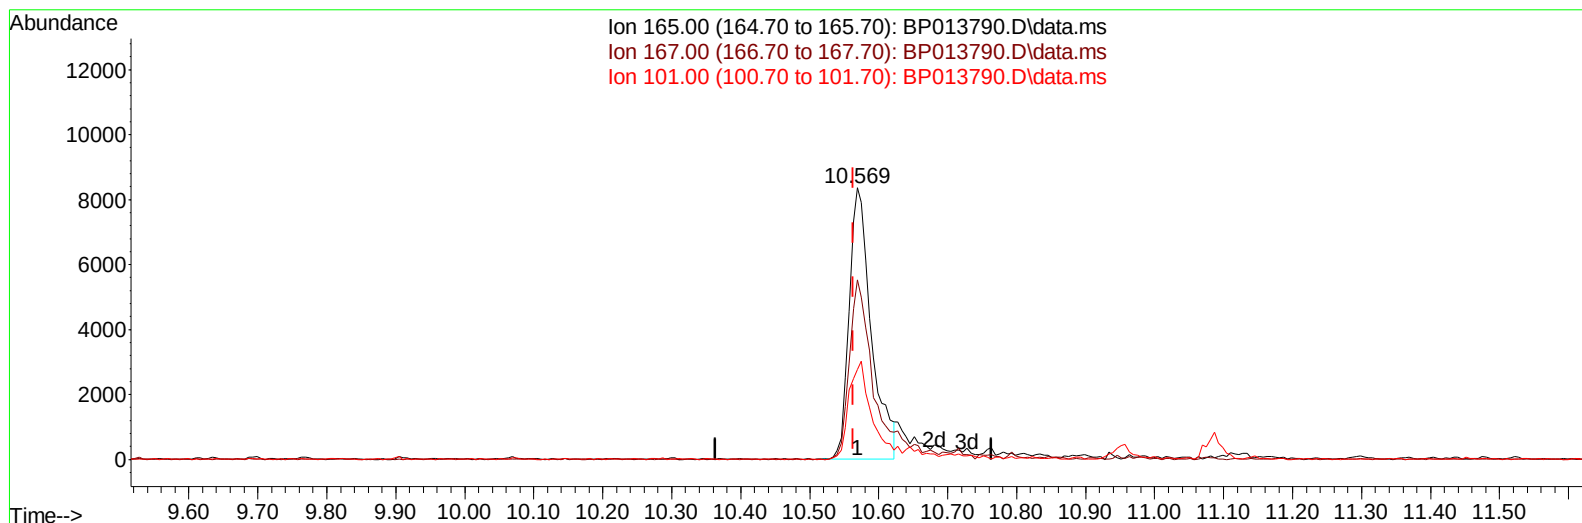

TIC: BP013790.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.569min (+ 0.006) 1.68 ng/ul

response 18708

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	63.60	66.09
101.00	33.90	33.07
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
 Data File : BP013790.D
 Acq On : 08 Feb 2023 11:07
 Operator : CG/JU
 Sample : 01381-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44M8

Manual IntegrationsAPPROVED

Quant Time: Feb 08 23:54:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 08 00:37:14 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/09/2023
 Supervised By :Sohil Jodhani 02/09/2023

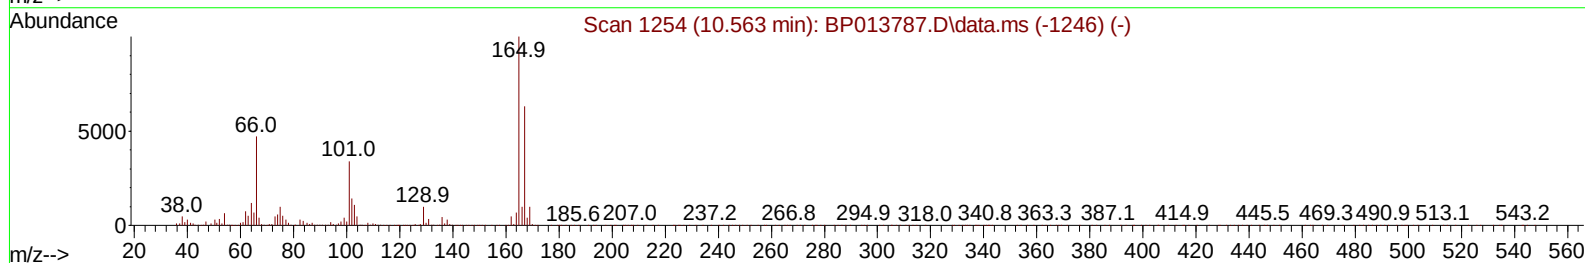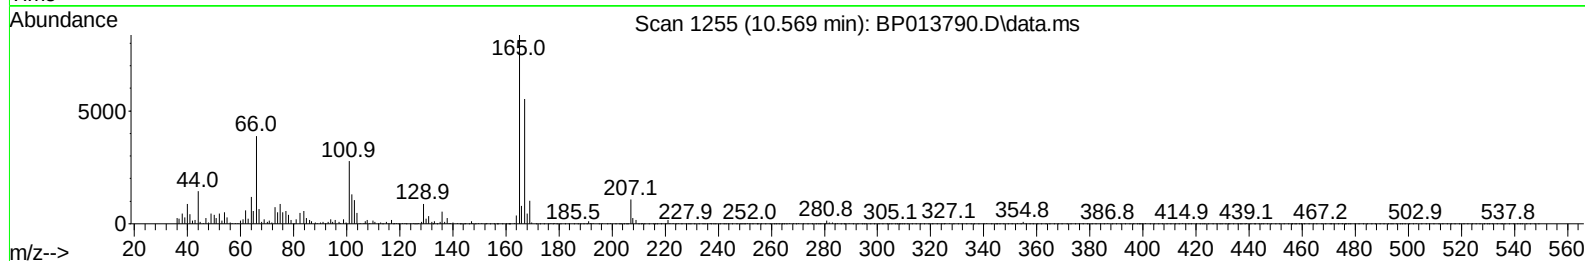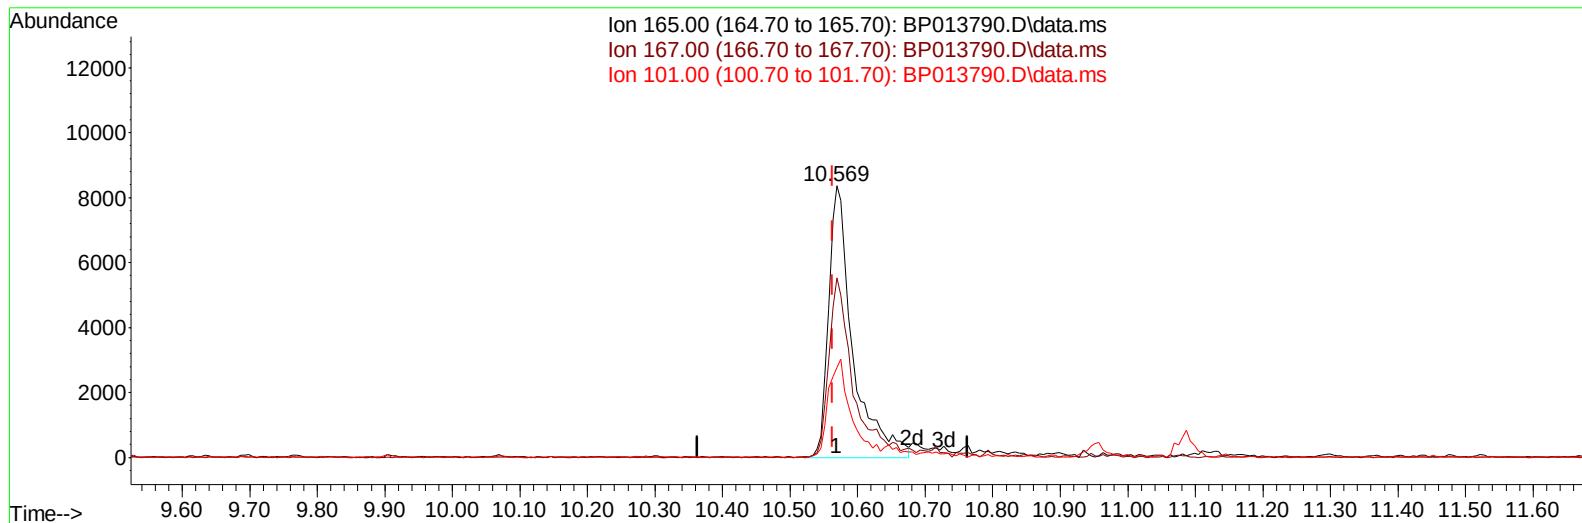

TIC: BP013790.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.569min (+ 0.006) 1.86 ng/ul m

response 20761

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	63.60	66.09
101.00	33.90	33.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
 Data File : BP013790.D
 Acq On : 08 Feb 2023 11:07
 Operator : CG/JU
 Sample : 01381-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44M8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/09/2023
 Supervised By :Sohil Jodhani 02/09/2023

Quant Time: Feb 08 23:54:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 08 00:37:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.122	152	151734	20.000	ng/ul	0.00
20) Naphthalene-d8	10.951	136	680645	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.757	164	499521	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.510	188	1211043	20.000	ng/ul	0.00
79) Chrysene-d12	21.586	240	1325324	20.000	ng/ul	0.00
88) Perylene-d12	24.151	264	1351412	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.469	96	15432	4.215	ng/uL	0.00
4) Pyridine-d5	3.911	84	71533	6.591	ng/ul	0.00
7) Phenol-d5	7.275	99	25689m	1.900	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.440	67	201290	25.408	ng/ul	0.00
11) 2-Chlorophenol-d4	7.652	132	25858m	2.598	ng/ul	0.00
15) 4-Methylphenol-d8	8.834	113	38450	3.480	ng/ul	0.00
21) Nitrobenzene-d5	9.299	128	91867	19.399	ng/ul	0.00
24) 2-Nitrophenol-d4	10.022	143	2104	0.385	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.569	165	20761m	1.863	ng/ul	0.00
31) 4-Chloroaniline-d4	11.081	131	370496	23.457	ng/ul	0.00
46) Dimethylphthalate-d6	14.157	166	787355	20.012	ng/ul	0.00
49) Acenaphthylene-d8	14.457	160	1311079	30.785	ng/ul	0.00
54) 4-Nitrophenol-d4	14.934	143	11	0.002	ng/ul	-0.01
60) Fluorene-d10	15.751	176	1064443	31.763	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.857	200	14	0.002	ng/ul	0.00
73) Anthracene-d10	17.610	188	1894866	34.218	ng/ul	0.00
81) Pyrene-d10	19.827	212	2464543	32.792	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.986	264	2405349	35.522	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013790.D
Acq On : 08 Feb 2023 11:07
Operator : CG/JU
Sample : 01381-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44M8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/09/2023
Supervised By :Sohil Jodhani 02/09/2023

Quant Time: Feb 08 23:54:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 08 00:37:14 2023
Response via : Initial Calibration

