

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
 Data File : BP013793.D
 Acq On : 08 Feb 2023 12:56
 Operator : CG/JU
 Sample : 01412-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44M4

Quant Time: Feb 08 23:55:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 08 00:37:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.122	152	172278	20.000	ng/u1	0.00
20) Naphthalene-d8	10.951	136	768834	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.757	164	547135	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.510	188	1353545	20.000	ng/u1	0.00
79) Chrysene-d12	21.586	240	1467704	20.000	ng/u1	0.00
88) Perylene-d12	24.151	264	1459274	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.469	96	16606	3.995	ng/uL	0.00
4) Pyridine-d5	3.905	84	86807	7.044	ng/u1	0.00
7) Phenol-d5	7.269	99	73975	4.819	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.440	67	189837	21.105	ng/u1	0.00
11) 2-Chlorophenol-d4	7.646	132	193298	17.107	ng/u1	0.00
15) 4-Methylphenol-d8	8.822	113	141427	11.273	ng/u1	0.00
21) Nitrobenzene-d5	9.293	128	114165	21.342	ng/u1	0.00
24) 2-Nitrophenol-d4	10.022	143	125662	20.346	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.563	165	259207	20.594	ng/u1	0.00
31) 4-Chloroaniline-d4	11.081	131	292138	16.374	ng/u1	0.00
46) Dimethylphthalate-d6	14.157	166	979503	22.730	ng/u1	0.00
49) Acenaphthylene-d8	14.451	160	1049309	22.494	ng/u1	0.00
54) 4-Nitrophenol-d4	14.945	143	26501	3.452	ng/u1	0.00
60) Fluorene-d10	15.751	176	860121	23.433	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.857	200	90468	10.895	ng/u1	0.00
73) Anthracene-d10	17.610	188	1458537	23.566	ng/u1	0.00
81) Pyrene-d10	19.827	212	1880144	22.589	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.986	264	1721856	23.549	ng/u1	0.00
Target Compounds						
32) 4-Chloroaniline	11.110	127	20790	1.156	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
 Data File : BP013793.D
 Acq On : 08 Feb 2023 12:56
 Operator : CG/JU
 Sample : 01412-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44M4

Quant Time: Feb 08 23:55:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 08 00:37:14 2023
 Response via : Initial Calibration

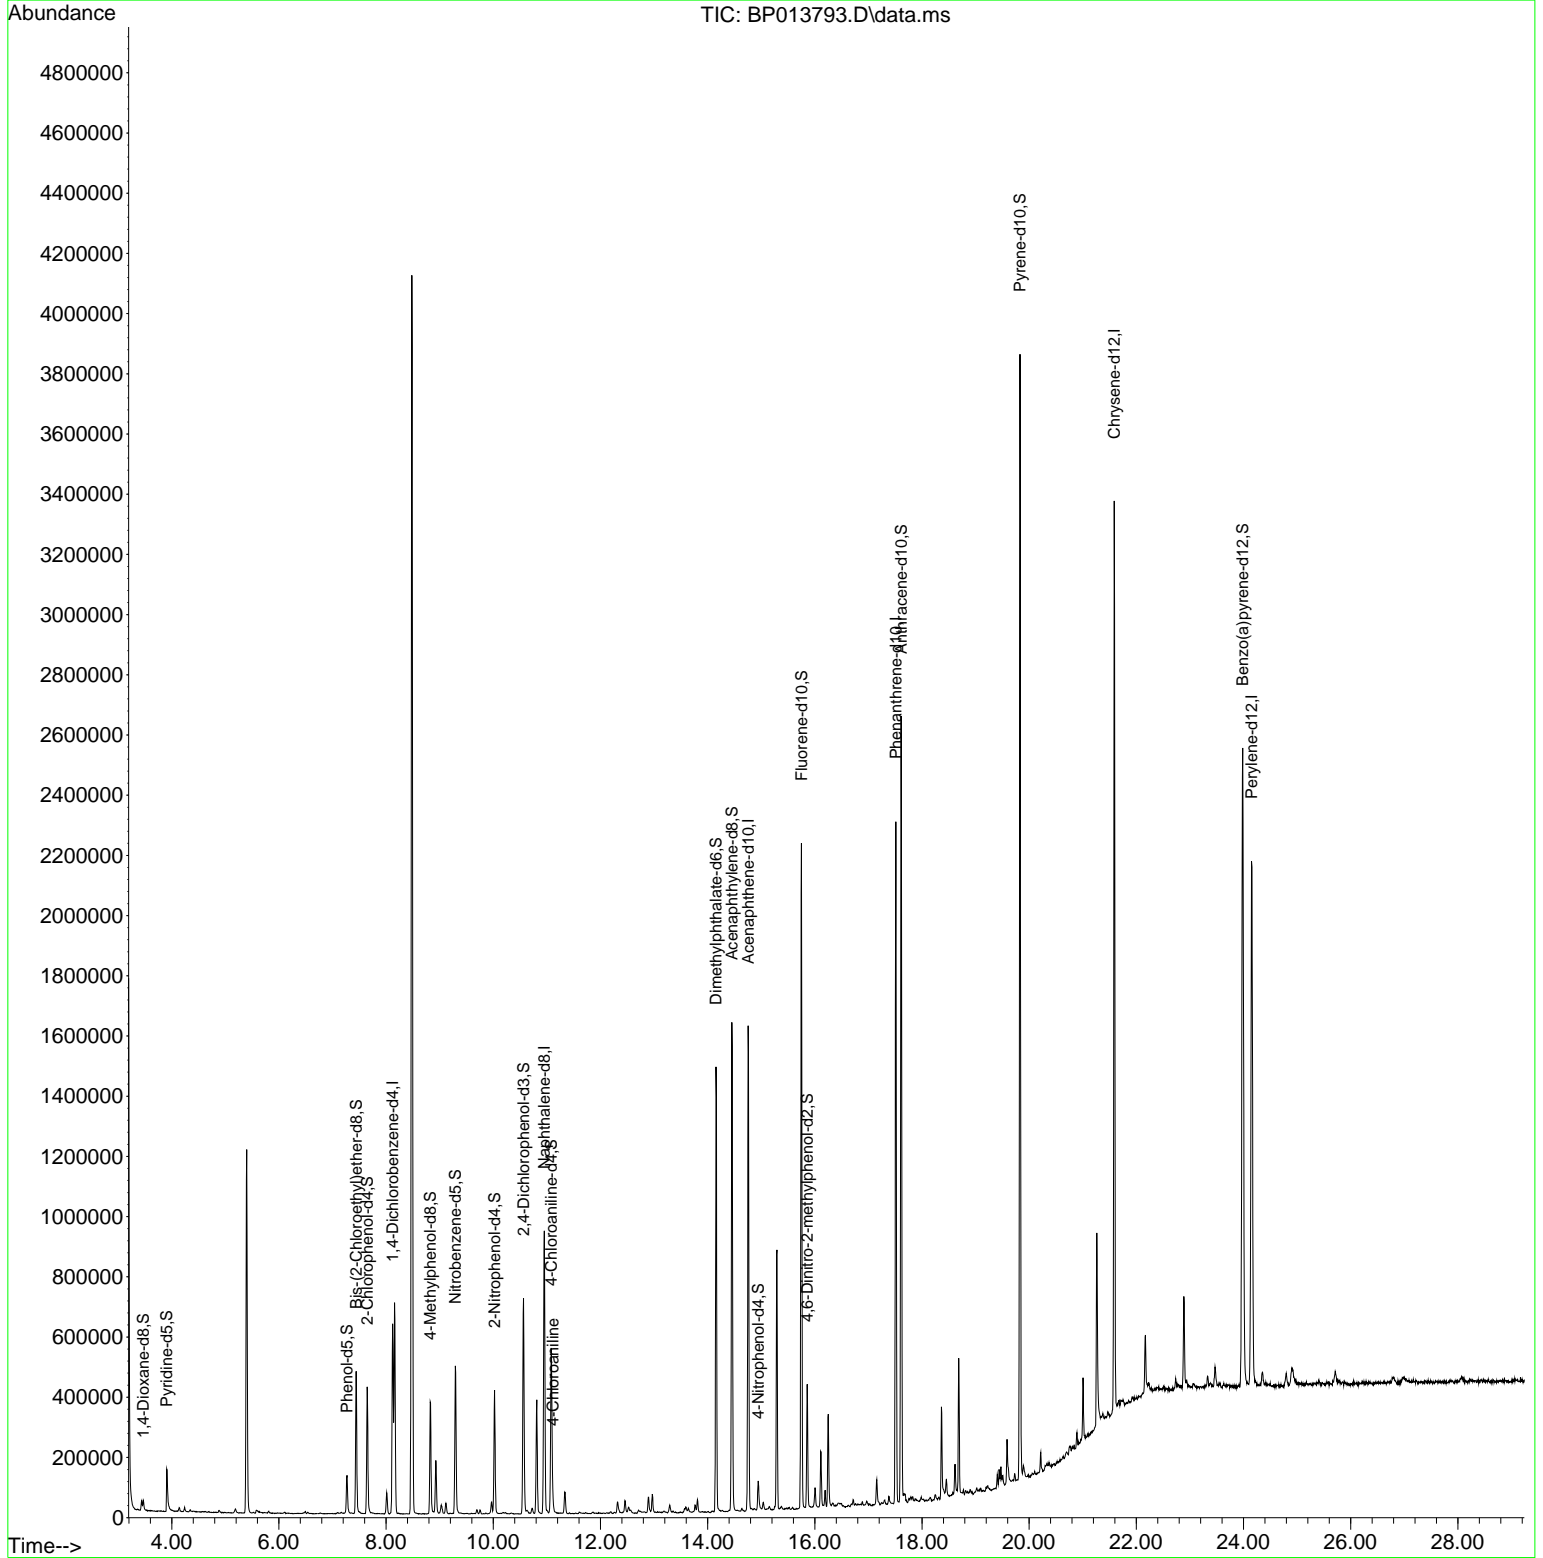

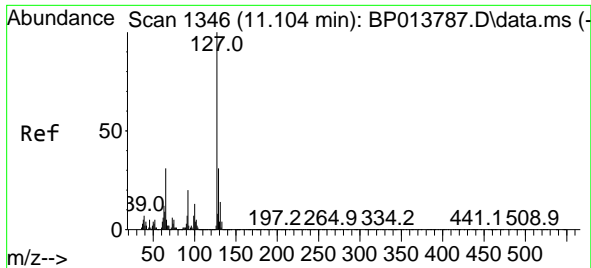

#32
 4-Chloroaniline
 Concen: 1.156 ng/ul
 RT: 11.110 min Scan# 1347
 Delta R.T. -0.000 min
 Lab File: BP013793.D
 Acq: 08 Feb 2023 12:56

Instrument :
 BNA_P
 ClientSampleId :
 A44M4

Tgt Ion:127 Resp: 20790
 Ion Ratio Lower Upper
 127 100
 129 32.0 26.2 39.4

